

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034909.D
 Acq On : 29 Mar 2024 16:37
 Operator : SY/MD
 Sample : P1934-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	207475	218346	16.17%	2.149%
2	1.532	146	153	172	rVB	188967	217554	16.11%	2.141%
3	2.060	307	317	334	rBV	365388	528409	39.13%	5.200%
4	2.452	434	439	444	rVB6	1351	1577	0.12%	0.016%
5	2.648	498	500	501	rBV	342	135	0.01%	0.001%
6	2.728	523	525	530	rVB3	586	436	0.03%	0.004%
7	2.754	530	533	534	rBV2	263	146	0.01%	0.001%
8	2.847	560	562	564	rVB	532	203	0.02%	0.002%
9	2.896	575	577	579	rVB	323	144	0.01%	0.001%
10	3.069	627	631	635	rBV4	479	365	0.03%	0.004%
11	3.088	635	637	640	rVV2	205	106	0.01%	0.001%
12	3.127	647	649	652	rVB2	480	197	0.01%	0.002%
13	3.143	652	654	657	rBV2	281	220	0.02%	0.002%
14	3.236	680	683	686	rVB2	485	244	0.02%	0.002%
15	3.288	696	699	702	rBV	398	213	0.02%	0.002%
16	3.314	702	707	709	rBV2	335	359	0.03%	0.004%
17	3.365	721	723	725	rBV	215	67	0.00%	0.001%
18	3.404	730	735	737	rBV2	501	498	0.04%	0.005%
19	3.490	760	762	765	rVB2	260	126	0.01%	0.001%
20	3.516	765	770	776	rBV2	302	452	0.03%	0.004%
21	3.603	793	797	800	rBV2	306	269	0.02%	0.003%
22	3.616	800	801	805	rBV2	278	164	0.01%	0.002%
23	3.658	810	814	817	rBV2	582	526	0.04%	0.005%
24	3.789	843	855	898	rBV2	109395	354895	26.28%	3.493%
25	4.249	983	998	1037	rBV	210063	547493	40.54%	5.388%
26	4.822	1174	1176	1179	rBV2	418	214	0.02%	0.002%
27	4.854	1183	1186	1189	rVB2	685	379	0.03%	0.004%
28	4.870	1189	1191	1194	rBV	404	282	0.02%	0.003%
29	4.892	1194	1198	1200	rBV4	557	425	0.03%	0.004%
30	4.957	1202	1218	1256	rBV2	510531	1350359	100.00%	13.290%
31	5.468	1374	1377	1378	rBV	464	228	0.02%	0.002%
32	5.535	1386	1398	1429	rBV	361194	756843	56.05%	7.448%
33	5.831	1479	1490	1510	rBV4	14226	33711	2.50%	0.332%
34	5.989	1525	1539	1575	rBV	293105	618343	45.79%	6.085%
35	6.394	1663	1665	1668	rVB2	444	217	0.02%	0.002%
36	6.490	1694	1695	1697	rBV	191	84	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034909.D
 Acq On : 29 Mar 2024 16:37
 Operator : SY/MD
 Sample : P1934-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.500	1697	1698	1704	rVB	281	184	0.01%	0.002%
38	6.555	1713	1715	1716	rVB2	166	38	0.00%	0.000%
39	6.728	1766	1769	1771	rBV2	251	180	0.01%	0.002%
40	6.757	1775	1778	1780	rBV2	505	265	0.02%	0.003%
41	6.915	1817	1827	1851	rBV2	146675	283634	21.00%	2.791%
42	7.243	1917	1929	1969	rBV	590342	1056370	78.23%	10.396%
43	7.555	2017	2026	2049	rBV	100435	187389	13.88%	1.844%
44	7.828	2109	2111	2113	rBV2	368	171	0.01%	0.002%
45	7.992	2160	2162	2164	rBV2	339	179	0.01%	0.002%
46	8.027	2164	2173	2221	rBV2	259608	589143	43.63%	5.798%
47	8.407	2289	2291	2297	rBV3	558	570	0.04%	0.006%
48	8.783	2397	2408	2441	rBV	564934	946388	70.08%	9.314%
49	9.198	2534	2537	2539	rBV2	508	335	0.02%	0.003%
50	9.342	2577	2582	2590	rVB5	598	721	0.05%	0.007%
51	9.384	2590	2595	2598	rBV3	604	462	0.03%	0.005%
52	9.426	2606	2608	2610	rBV	465	214	0.02%	0.002%
53	9.458	2615	2618	2623	rVB3	421	349	0.03%	0.003%
54	9.500	2628	2631	2632	rBV2	383	191	0.01%	0.002%
55	9.673	2681	2685	2688	rBV	644	476	0.04%	0.005%
56	9.853	2739	2741	2743	rBV	207	122	0.01%	0.001%
57	9.899	2753	2755	2758	rBV	372	203	0.02%	0.002%
58	9.944	2767	2769	2771	rBV	439	196	0.01%	0.002%
59	9.982	2779	2781	2784	rVB	448	198	0.01%	0.002%
60	9.998	2784	2786	2790	rBV	503	303	0.02%	0.003%
61	10.043	2797	2800	2803	rBV	284	221	0.02%	0.002%
62	10.153	2823	2834	2861	rBV	392533	629117	46.59%	6.191%
63	10.384	2902	2906	2909	rBV2	597	566	0.04%	0.006%
64	10.525	2948	2950	2952	rBV2	447	207	0.02%	0.002%
65	10.609	2974	2976	2978	rBV2	358	172	0.01%	0.002%
66	10.789	3028	3032	3035	rBV2	574	505	0.04%	0.005%
67	10.873	3054	3058	3060	rBV2	486	334	0.02%	0.003%
68	10.982	3090	3092	3095	rVB2	414	150	0.01%	0.001%
69	11.185	3144	3155	3188	rBV	558334	878679	65.07%	8.648%
70	11.468	3239	3243	3245	rBV2	439	337	0.02%	0.003%
71	11.558	3260	3271	3303	rBV	588209	934868	69.23%	9.200%
72	12.911	3690	3692	3695	rBV2	432	213	0.02%	0.002%
73	13.210	3776	3785	3792	rBV6	5702	9793	0.73%	0.096%
74	13.686	3927	3933	3941	rBV5	2186	2928	0.22%	0.029%
75	13.863	3986	3988	3989	rBV	482	210	0.02%	0.002%
76	14.310	4125	4127	4129	rBV2	513	261	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034909.D
Acq On : 29 Mar 2024 16:37
Operator : SY/MD
Sample : P1934-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R40

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis




Sum of corrected areas: 10161071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034909.D
Acq On : 29 Mar 2024 16:37
Operator : SY/MD
Sample : P1934-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

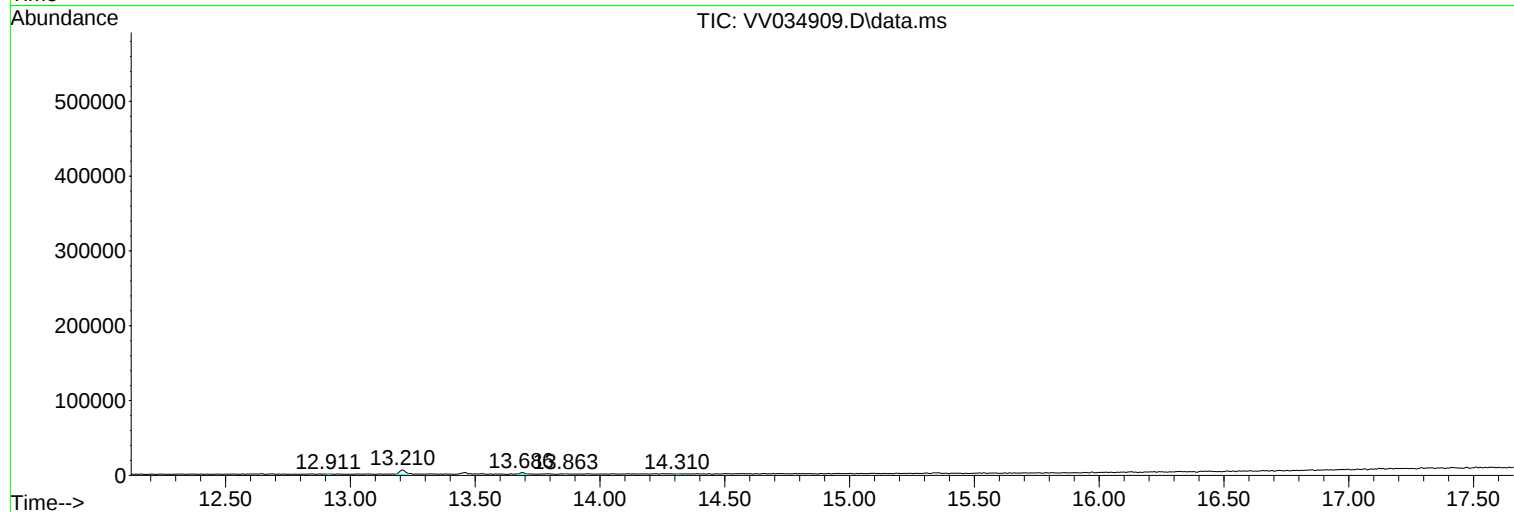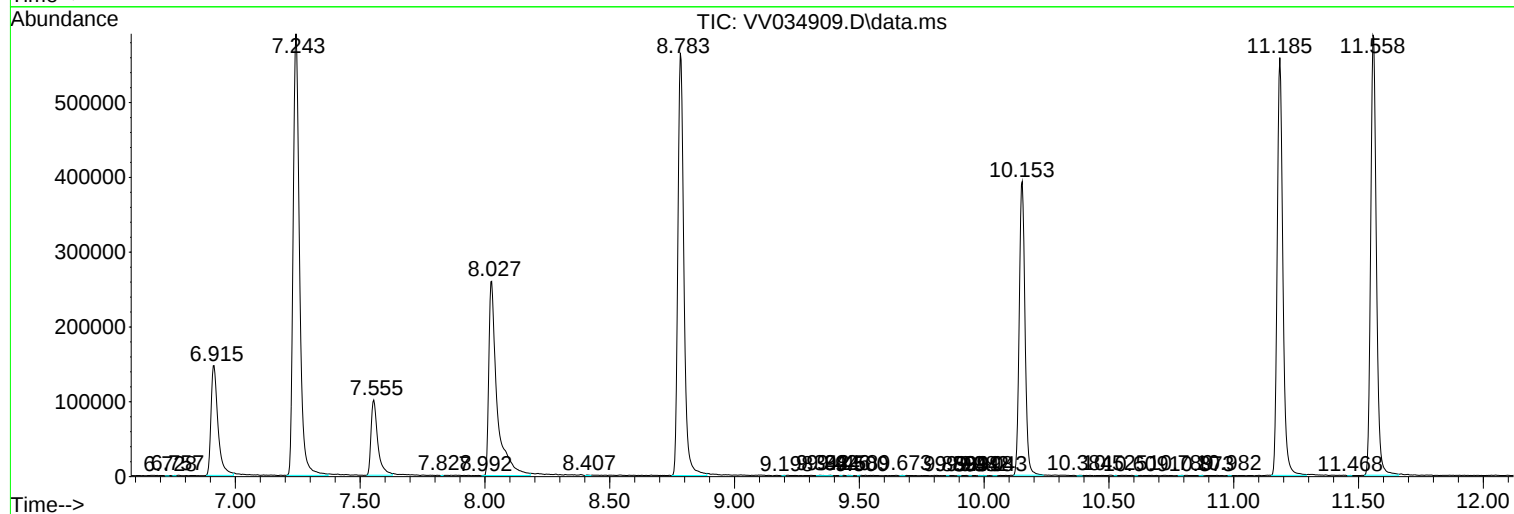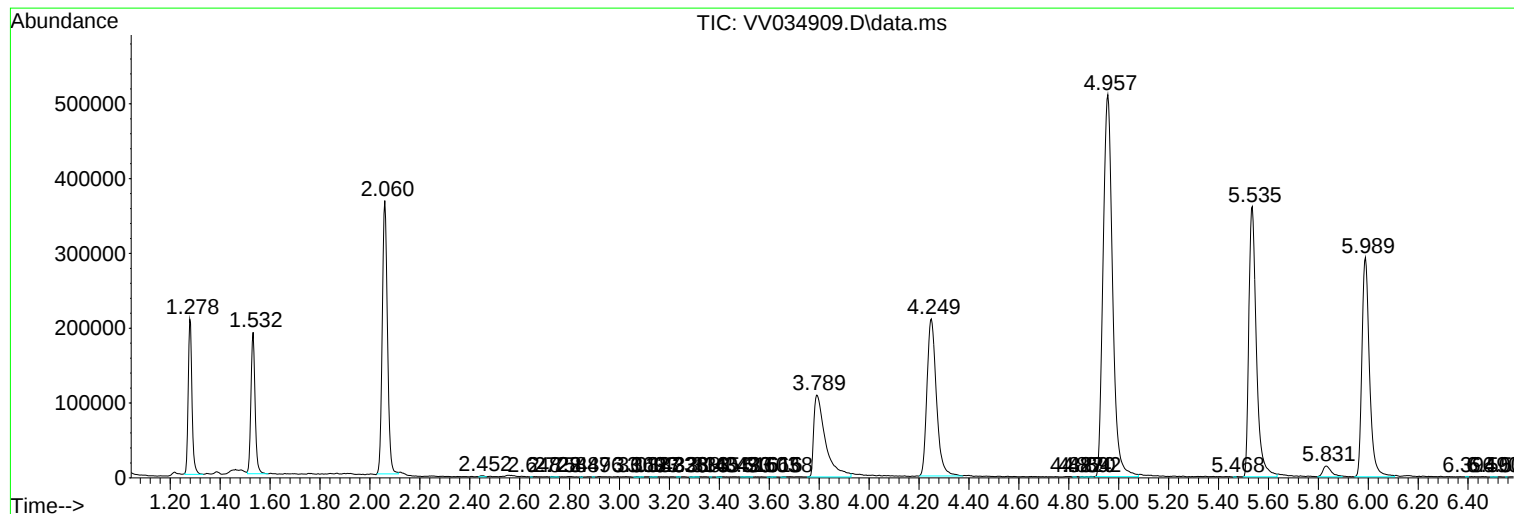

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034909.D
Acq On : 29 Mar 2024 16:37
Operator : SY/MD
Sample : P1934-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034909.D
Acq On : 29 Mar 2024 16:37
Operator : SY/MD
Sample : P1934-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------