

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034910.D
 Acq On : 29 Mar 2024 17:01
 Operator : SY/MD
 Sample : P1934-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	218461	231693	4.20%	1.109%
2	1.532	146	153	169	rVB	192978	232219	4.21%	1.111%
3	2.059	307	317	353	rVB	390862	584865	10.61%	2.798%
4	2.449	430	438	443	rBV7	1906	2711	0.05%	0.013%
5	2.715	519	521	526	rBV3	332	235	0.00%	0.001%
6	2.738	526	528	534	rBV2	444	349	0.01%	0.002%
7	2.821	552	554	557	rBV2	328	150	0.00%	0.001%
8	2.899	576	578	579	rBV2	248	95	0.00%	0.000%
9	2.928	585	587	590	rBV2	519	363	0.01%	0.002%
10	2.947	591	593	595	rVV	661	399	0.01%	0.002%
11	2.969	598	600	606	rVB2	658	452	0.01%	0.002%
12	2.992	606	607	609	rVB	217	62	0.00%	0.000%
13	3.002	609	610	611	rBV	218	82	0.00%	0.000%
14	3.014	612	614	621	rVB2	660	567	0.01%	0.003%
15	3.050	621	625	628	rBV3	359	341	0.01%	0.002%
16	3.121	643	647	651	rBB3	563	434	0.01%	0.002%
17	3.191	663	669	672	rBV2	643	541	0.01%	0.003%
18	3.259	688	690	691	rBV2	259	77	0.00%	0.000%
19	3.288	695	699	702	rBV2	513	310	0.01%	0.001%
20	3.320	706	709	711	rVV3	293	174	0.00%	0.001%
21	3.336	712	714	716	rVB	316	135	0.00%	0.001%
22	3.400	730	734	735	rBV	432	310	0.01%	0.001%
23	3.439	743	746	750	rBV	214	161	0.00%	0.001%
24	3.458	750	752	755	rVV2	297	133	0.00%	0.001%
25	3.471	755	756	758	rVV	223	81	0.00%	0.000%
26	3.497	762	764	765	rVB	254	76	0.00%	0.000%
27	3.526	771	773	775	rBV2	206	89	0.00%	0.000%
28	3.545	775	779	784	rVB4	467	513	0.01%	0.002%
29	3.571	785	787	788	rBV	253	75	0.00%	0.000%
30	3.580	788	790	792	rVB	376	145	0.00%	0.001%
31	3.612	796	800	802	rBV3	306	224	0.00%	0.001%
32	3.625	802	804	805	rBV	165	45	0.00%	0.000%
33	3.638	805	808	810	rBV2	442	221	0.00%	0.001%
34	3.657	810	814	815	rBV2	1102	696	0.01%	0.003%
35	3.789	846	855	897	rBV	95301	289835	5.26%	1.387%
36	4.249	983	998	1030	rBV	221032	572031	10.38%	2.737%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034910.D
 Acq On : 29 Mar 2024 17:01
 Operator : SY/MD
 Sample : P1934-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.651	1121	1123	1127	rBV	500	342	0.01%	0.002%
38	4.956	1198	1218	1228	rBV2	552091	1418905	25.74%	6.789%
39	5.317	1327	1330	1331	rBV3	583	333	0.01%	0.002%
40	5.384	1349	1351	1352	rBV2	315	123	0.00%	0.001%
41	5.535	1386	1398	1430	rBV	391407	822730	14.93%	3.936%
42	5.989	1526	1539	1575	rBV	313131	657834	11.94%	3.147%
43	6.352	1650	1652	1653	rVB	496	149	0.00%	0.001%
44	6.365	1653	1656	1658	rBV2	630	453	0.01%	0.002%
45	6.432	1675	1677	1681	rBV3	638	396	0.01%	0.002%
46	6.554	1713	1715	1719	rVB2	383	208	0.00%	0.001%
47	6.616	1732	1734	1735	rBV	255	108	0.00%	0.001%
48	6.744	1771	1774	1778	rBV4	594	500	0.01%	0.002%
49	6.786	1785	1787	1788	rVB4	604	210	0.00%	0.001%
50	6.915	1817	1827	1857	rBV	160920	308034	5.59%	1.474%
51	7.243	1918	1929	1952	rBV	629236	1112245	20.18%	5.321%
52	7.554	2016	2026	2054	rBV	107107	202960	3.68%	0.971%
53	7.853	2117	2119	2122	rBV3	332	239	0.00%	0.001%
54	7.982	2154	2159	2163	rBV3	450	440	0.01%	0.002%
55	8.027	2163	2173	2226	rBV	288187	635873	11.54%	3.042%
56	8.423	2294	2296	2299	rBV	508	306	0.01%	0.001%
57	8.583	2343	2346	2349	rBV2	427	345	0.01%	0.002%
58	8.603	2349	2352	2354	rVB2	525	325	0.01%	0.002%
59	8.812	2397	2417	2462	rBV2	2782897	5511754	100.00%	26.370%
60	9.480	2621	2625	2627	rBV3	458	366	0.01%	0.002%
61	9.545	2643	2645	2648	rBV2	537	310	0.01%	0.001%
62	9.612	2664	2666	2667	rBV2	285	125	0.00%	0.001%
63	9.651	2676	2678	2682	rVB2	424	270	0.00%	0.001%
64	9.683	2686	2688	2689	rBV	389	123	0.00%	0.001%
65	9.799	2722	2724	2725	rBV	267	71	0.00%	0.000%
66	9.876	2746	2748	2758	rVB4	396	462	0.01%	0.002%
67	9.992	2779	2784	2789	rBV4	829	1033	0.02%	0.005%
68	10.152	2821	2834	2857	rBV	432808	683304	12.40%	3.269%
69	10.429	2918	2920	2921	rVB	251	79	0.00%	0.000%
70	10.451	2923	2927	2929	rVB	294	175	0.00%	0.001%
71	10.480	2929	2936	2939	rBV3	727	783	0.01%	0.004%
72	10.551	2955	2958	2961	rBV3	542	427	0.01%	0.002%
73	10.644	2983	2987	2990	rBV2	537	435	0.01%	0.002%
74	10.725	3010	3012	3014	rBV2	339	154	0.00%	0.001%
75	10.738	3014	3016	3019	rBV2	416	290	0.01%	0.001%
76	10.857	3051	3053	3058	rBV3	593	504	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
 Data File : VV034910.D
 Acq On : 29 Mar 2024 17:01
 Operator : SY/MD
 Sample : P1934-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.898	3063	3066	3069	rBV	244	215	0.00%	0.001%
78	10.934	3075	3077	3084	rVB2	451	312	0.01%	0.001%
79	11.001	3096	3098	3104	rBV	487	465	0.01%	0.002%
80	11.066	3116	3118	3119	rBV	358	130	0.00%	0.001%
81	11.117	3124	3134	3145	rBV	156386	247464	4.49%	1.184%
82	11.207	3146	3162	3187	rVB2	1468924	3138254	56.94%	15.015%
83	11.574	3260	3276	3299	rBV2	1811173	3620967	65.70%	17.324%
84	12.345	3510	3516	3517	rBV3	1168	1127	0.02%	0.005%
85	12.535	3570	3575	3578	rBV	500	646	0.01%	0.003%
86	12.590	3589	3592	3596	rBV3	888	981	0.02%	0.005%
87	12.696	3622	3625	3628	rBV5	970	766	0.01%	0.004%
88	12.815	3660	3662	3668	rVB3	427	311	0.01%	0.001%
89	12.892	3682	3686	3688	rBV2	430	296	0.01%	0.001%
90	13.197	3770	3781	3809	rBV	314460	495338	8.99%	2.370%
91	13.683	3921	3932	3953	rVB2	66004	109154	1.98%	0.522%
92	13.757	3953	3955	3959	rBV3	636	284	0.01%	0.001%


Sum of corrected areas: 20901322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034910.D
Acq On : 29 Mar 2024 17:01
Operator : SY/MD
Sample : P1934-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

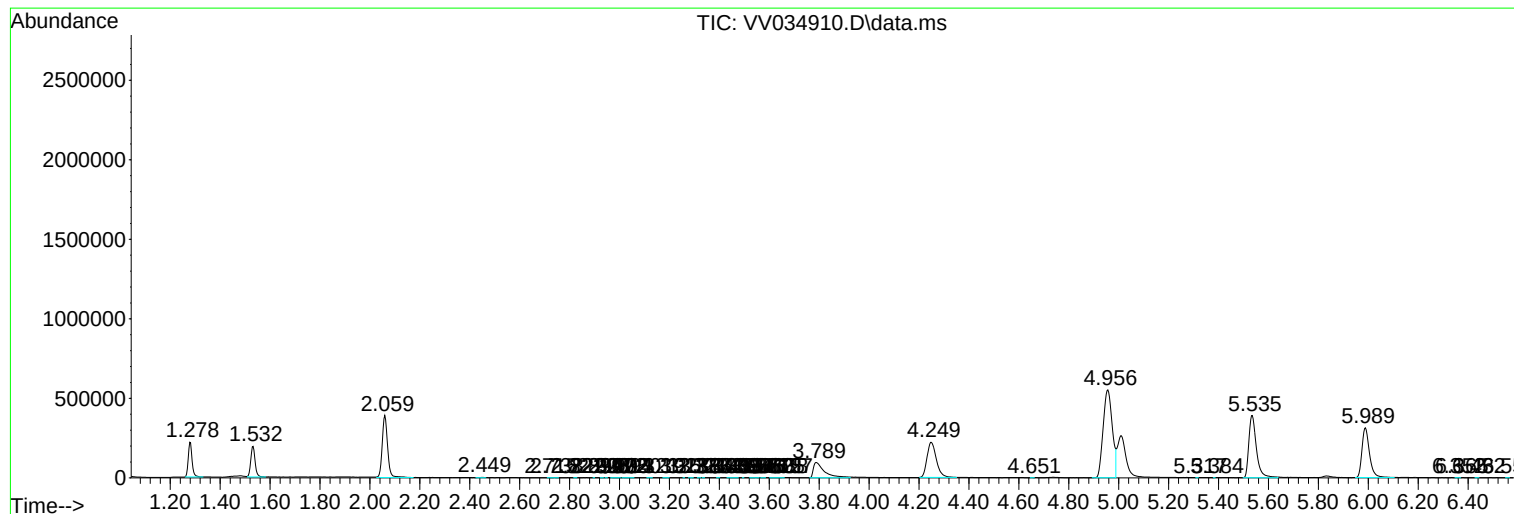

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034910.D
Acq On : 29 Mar 2024 17:01
Operator : SY/MD
Sample : P1934-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034910.D
Acq On : 29 Mar 2024 17:01
Operator : SY/MD
Sample : P1934-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------