


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032924\
Data File : VV034894.D
Acq On : 29 Mar 2024 08:15
Operator : SY/MD
Sample : BFB278
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB278

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Fri Mar 29 00:23:40 2024

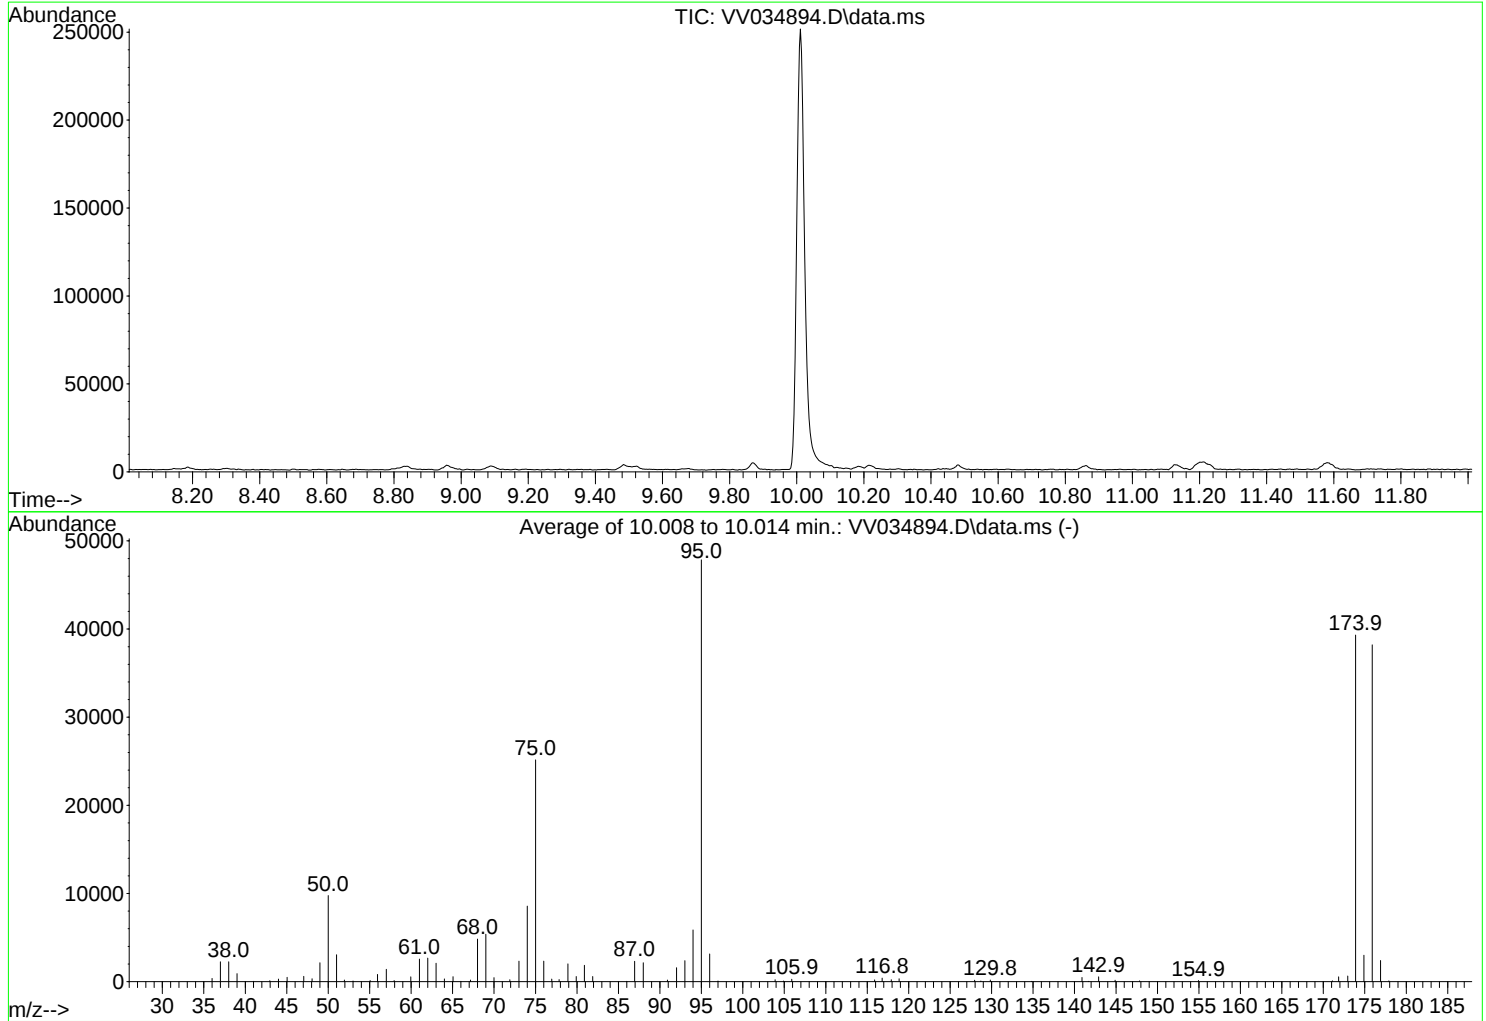

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	9768	PASS
75	95	30	80	52.6	25157	PASS
95	95	100	100	100.0	47851	PASS
96	95	5	9	6.6	3138	PASS
173	174	0.00	2	1.6	643	PASS
174	95	50	120	82.2	39320	PASS
175	174	5	9	7.6	3005	PASS
176	174	95	105	97.2	38203	PASS
177	176	5	10	6.3	2400	PASS

Scan 2778 (9.972 min): VV034894.D\data.ms
BFB278

m/z	Abundance
39.90	1012.0
44.00	375.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	399.0
37.00	2277.0
38.00	2404.0
39.00	930.0
39.90	956.0
41.00	101.0
42.90	107.0
44.00	617.0
45.10	474.0
47.00	599.0
48.00	366.0
49.00	2029.0
50.00	9941.0
51.00	2997.0
51.90	181.0
53.00	121.0
55.00	136.0
55.90	827.0
57.00	1415.0
58.00	153.0
60.00	517.0
61.00	2522.0
62.00	2648.0
63.00	2084.0
64.00	270.0
65.00	567.0
67.20	181.0
68.00	4838.0
69.00	5492.0
70.00	348.0
71.90	213.0
73.00	2265.0
74.00	8554.0
75.00	24920.0
76.00	2376.0
76.90	281.0
77.80	196.0
78.90	2035.0
79.90	586.0
80.90	1865.0
81.90	593.0
86.00	105.0
87.00	2356.0
88.00	2232.0
91.00	175.0
92.00	1508.0
93.00	2372.0
94.00	5779.0
95.00	47608.0
96.00	3163.0
97.00	111.0
103.90	203.0
104.90	119.0
105.90	260.0
115.90	210.0
116.80	383.0
117.90	210.0
118.80	307.0
127.90	178.0
128.70	118.0
129.90	211.0
140.90	485.0
141.70	109.0
142.90	540.0
144.90	162.0
147.80	159.0
154.90	133.0
171.80	597.0
173.00	547.0
173.90	38336.0
174.90	2806.0
175.90	37128.0
176.90	2552.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	362.0
37.00	2278.0
38.00	2318.0
39.00	950.0
39.90	984.0
42.90	122.0
44.00	670.0
45.10	531.0
47.00	620.0
48.10	338.0
49.00	2190.0
50.00	10153.0
51.00	3116.0
52.00	196.0
53.00	106.0
55.00	125.0
56.00	842.0
57.00	1390.0
58.00	129.0
59.90	571.0
61.00	2600.0
62.00	2790.0
63.00	2140.0
64.00	332.0
65.00	561.0
67.10	182.0
68.00	4970.0
69.00	5551.0
70.00	488.0
71.90	223.0
73.00	2391.0
74.00	8884.0
75.00	25984.0
76.00	2425.0
76.90	298.0
77.90	219.0
78.90	2067.0
79.90	580.0
80.90	1911.0
81.90	594.0
87.00	2351.0
88.00	2197.0
90.90	192.0
92.00	1660.0
93.00	2448.0
94.00	6050.0
95.00	49408.0
96.00	3218.0
97.00	118.0
103.90	240.0
104.90	120.0
105.90	285.0
115.90	221.0
116.80	428.0
117.90	223.0
118.90	335.0
128.00	155.0
128.70	116.0
129.90	196.0
140.90	471.0
142.90	558.0
144.90	183.0
147.90	131.0
155.00	122.0
171.10	123.0
171.90	565.0
172.90	662.0
173.90	40728.0
174.90	3085.0
175.90	39456.0
176.90	2434.0
177.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	342.0
37.00	2187.0
38.00	2040.0
39.00	868.0
39.90	934.0
43.00	104.0
44.00	731.0
45.00	475.0
47.10	602.0
48.00	299.0
49.00	2185.0
50.00	9210.0
51.00	3060.0
52.00	180.0
55.10	102.0
56.00	783.0
57.00	1372.0
57.90	102.0
60.00	576.0
61.00	2571.0
62.00	2577.0
63.00	2040.0
64.00	335.0
65.10	555.0
66.00	129.0
67.10	183.0
68.00	4677.0
69.00	5084.0
70.00	550.0
71.90	213.0
73.00	2313.0
74.00	8272.0
75.00	24568.0
76.00	2186.0
77.00	312.0
77.90	272.0
78.90	1923.0
79.90	561.0
80.90	1791.0
81.90	558.0
86.90	2233.0
88.00	1985.0
90.80	199.0
92.00	1559.0
93.00	2318.0
94.00	5773.0
95.00	46536.0
96.00	3033.0
103.90	231.0
105.90	264.0
115.90	193.0
116.80	412.0
117.90	236.0
118.90	369.0
128.00	148.0
129.80	152.0
134.80	101.0
140.90	454.0
142.90	560.0
144.90	175.0
155.00	116.0
171.10	141.0
171.90	503.0
173.00	720.0
173.90	38896.0
174.90	3123.0
175.90	38024.0
176.90	2214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278