

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033022\
 Data File : VW025309.D
 Acq On : 30 Mar 2022 12:02
 Operator : SY/MD
 Sample : N2165-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q8

Quant Time: Mar 31 01:27:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 31 01:26:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	148557	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	146812	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	61399	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	72320	5.212	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.200%
7) Chloroethane-d5	1.568	69	58104	4.989	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.111	63	102247	3.402	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.905	46	45736	33.088	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	66.180%
24) Chloroform-d	4.352	84	86926	4.800	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	5.034	65	39321	4.912	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.050	84	174430	4.696	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.069	67	50348	4.837	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.800%
41) Toluene-d8	7.317	98	147860	4.340	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%
43) trans-1,3-Dichloroprop...	7.625	79	14204	4.183	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.088	63	43679	35.615	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.220%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29701	4.279	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	49484	5.018	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	6426	0.547	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025309.D
Acq On : 30 Mar 2022 12:02
Operator : SY/MD
Sample : N2165-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

Quant Time: Mar 31 01:27:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 31 01:26:10 2022
Response via : Initial Calibration

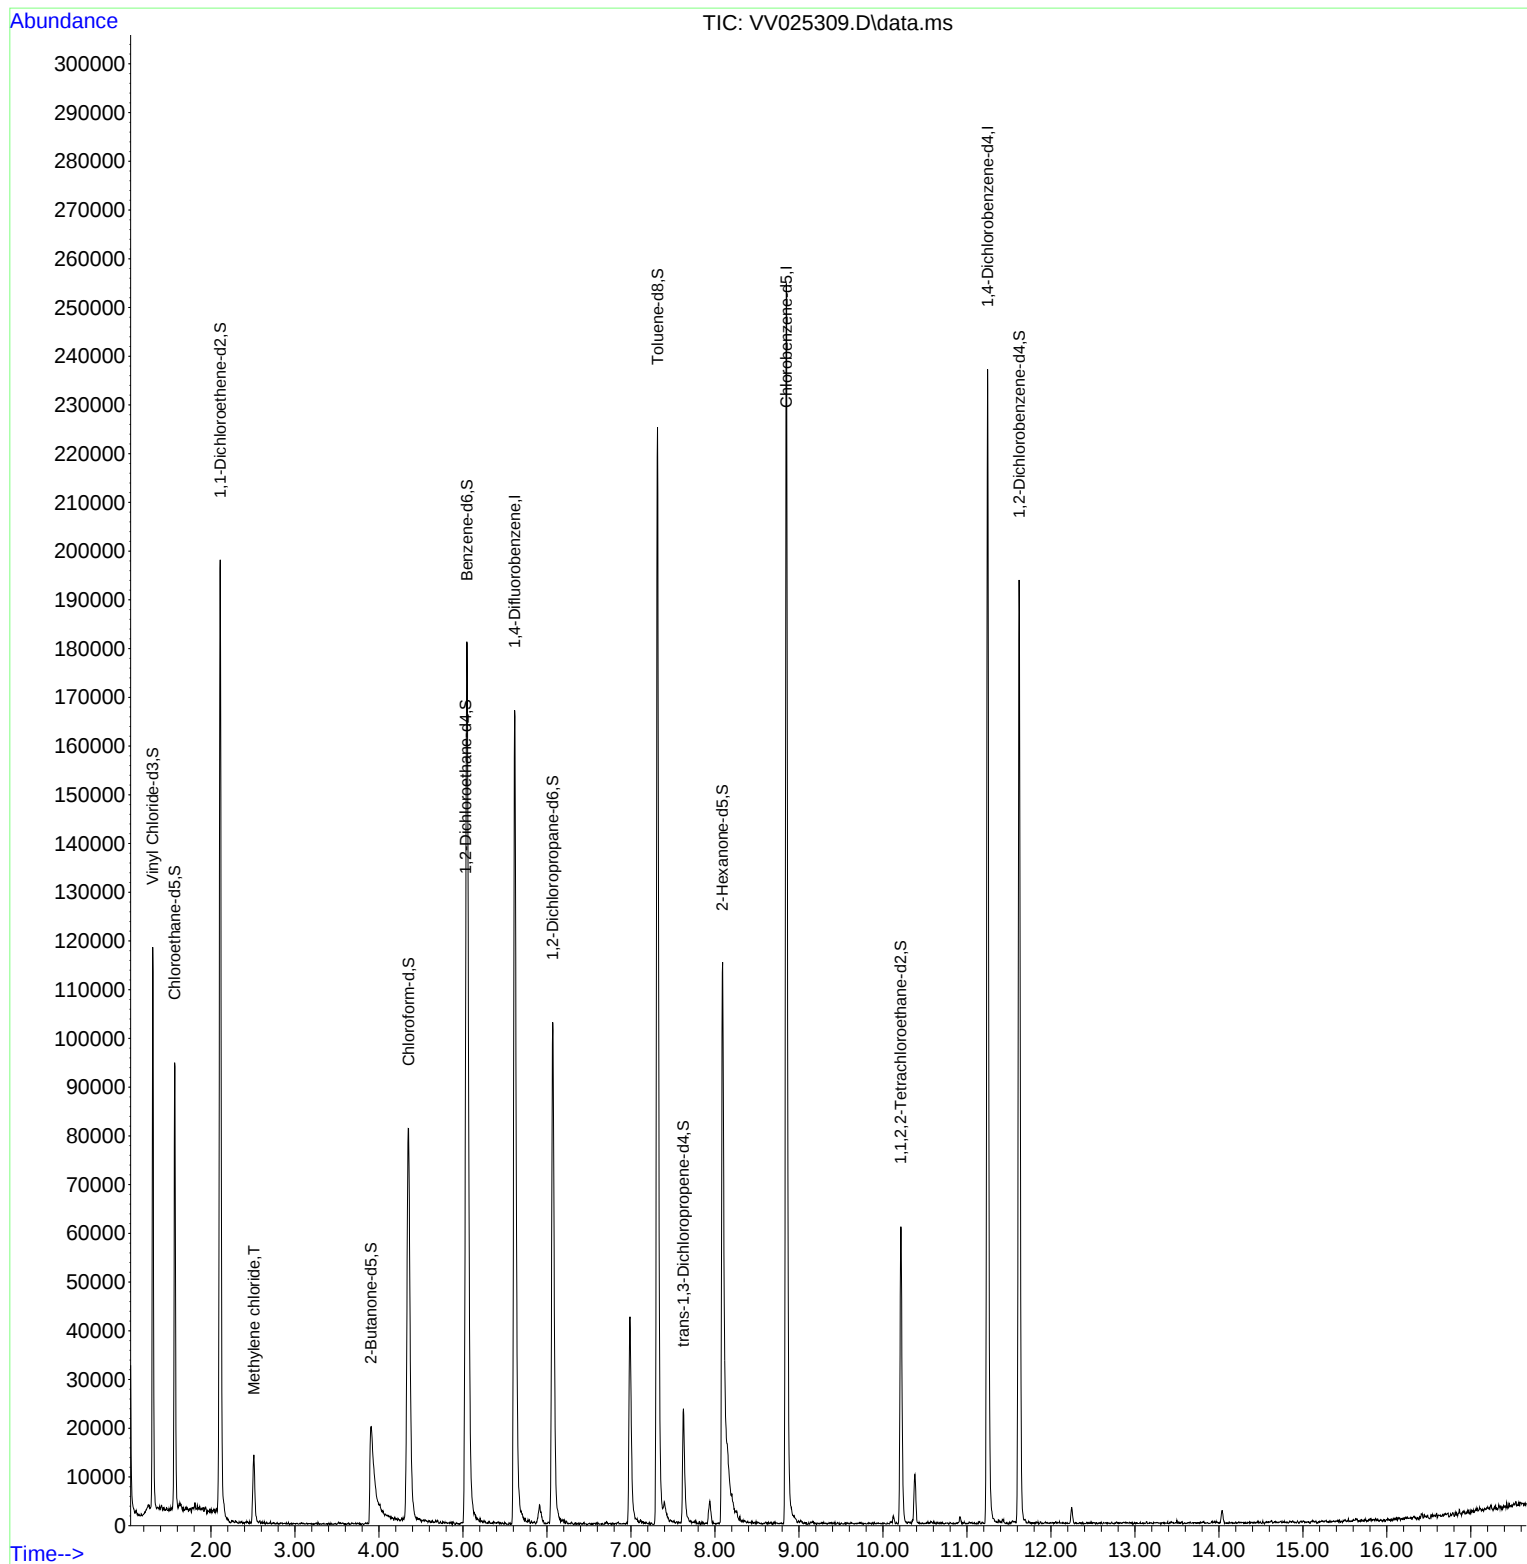

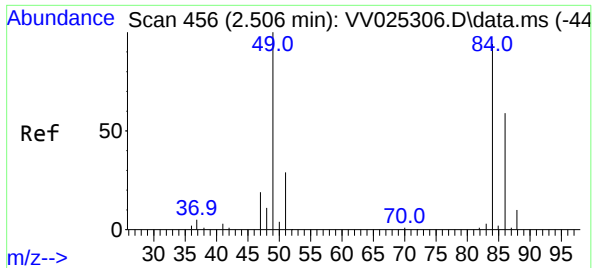

#16
Methylene chloride
Concen: 0.547 ug/L
RT: 2.513 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV025309.D
Acq: 30 Mar 2022 12:02

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

Tgt Ion:	84	Resp:	6426
Ion	Ratio	Lower	Upper
84	100		
86	49.0	43.5	80.7
49	91.0	74.5	138.3

