

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033022\
 Data File : VW025310.D
 Acq On : 30 Mar 2022 12:26
 Operator : SY/MD
 Sample : N2165-06DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6P3DL

Quant Time: Mar 31 01:27:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 31 01:26:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	140358	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	133687	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57654	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70245	5.358	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.200%
7) Chloroethane-d5	1.568	69	56945	5.175	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.600%
11) 1,1-Dichloroethene-d2	2.108	63	104806	3.690	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.800%
20) 2-Butanone-d5	3.918	46	56614	43.350	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.700%
24) Chloroform-d	4.349	84	85330	4.987	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	5.034	65	38036	5.029	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	5.050	84	173492	5.130	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
36) 1,2-Dichloropropane-d6	6.069	67	49641	5.237	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.800%
41) Toluene-d8	7.317	98	147186	4.745	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	7.625	79	13922	4.502	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.091	63	50212	44.961	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.920%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30948	4.897	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	48734	5.263	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.972	164	80068	10.084	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025310.D
Acq On : 30 Mar 2022 12:26
Operator : SY/MD
Sample : N2165-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P3DL


Quant Time: Mar 31 01:27:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 31 01:26:10 2022
Response via : Initial Calibration

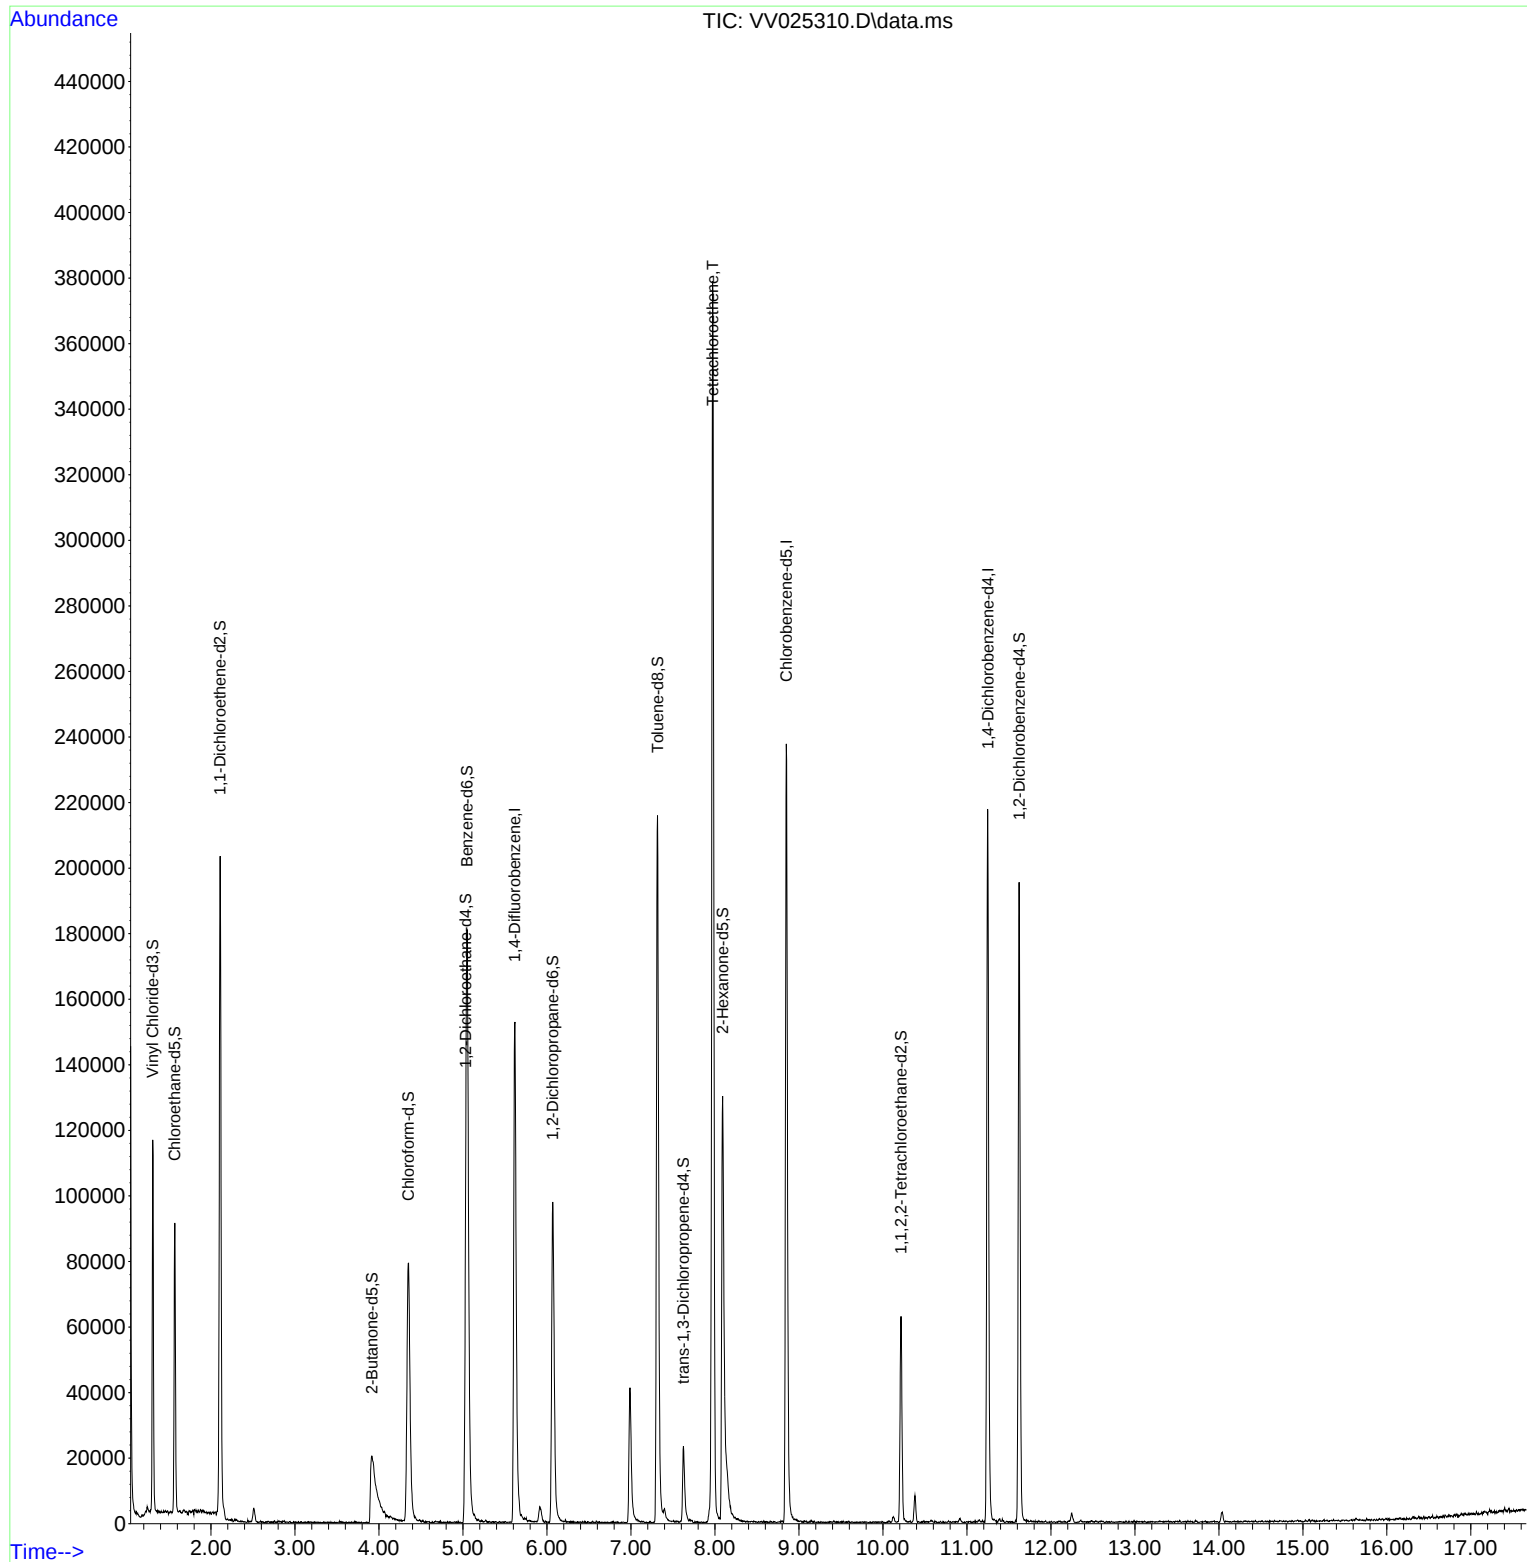

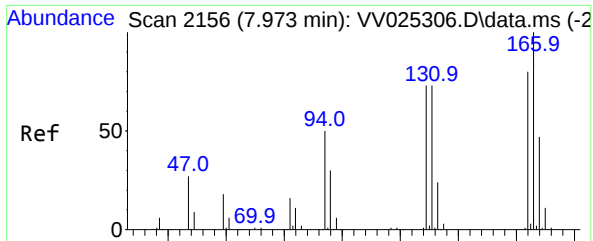

#47
Tetrachloroethene
Concen: 10.084 ug/L
RT: 7.972 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV025310.D
Acq: 30 Mar 2022 12:26

Instrument :
MSVOA_V
ClientSampleId :
EW6P3DL

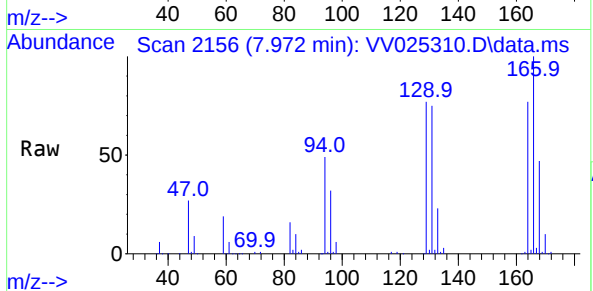

Tgt Ion:	164	Resp:	80068
Ion	Ratio	Lower	Upper
164	100		
129	99.6	67.5	125.4
131	97.3	68.0	126.4
166	129.0	86.2	160.2

