

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
 Data File : VV025308.D
 Acq On : 30 Mar 2022 11:39
 Operator : SY/MD
 Sample : N2165-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	116067	112782	26.00%	3.078%
2	1.564	154	163	175	rBV	88116	100881	23.26%	2.753%
3	2.105	320	331	346	rBV	185574	270867	62.45%	7.392%
4	2.503	445	455	468	rBV2	15195	24716	5.70%	0.675%
5	3.896	878	888	915	rBV	18438	69030	15.92%	1.884%
6	4.339	1010	1026	1049	rBV	77454	196832	45.38%	5.372%
7	5.040	1224	1244	1269	rBV3	171588	433741	100.00%	11.837%
8	5.609	1410	1421	1446	rBV	162459	335834	77.43%	9.165%
9	5.905	1504	1513	1526	rVB9	3713	8203	1.89%	0.224%
10	6.063	1550	1562	1587	rBV	95526	198744	45.82%	5.424%
11	6.982	1838	1848	1870	rBV2	39722	77158	17.79%	2.106%
12	7.310	1939	1950	1971	rBV	207158	370511	85.42%	10.112%
13	7.619	2037	2046	2067	rBV2	21567	41421	9.55%	1.130%
14	7.937	2134	2145	2156	rBV3	5571	10042	2.32%	0.274%
15	8.088	2182	2192	2229	rBV	103661	249382	57.50%	6.806%
16	8.850	2417	2429	2455	rBV	246102	412515	95.11%	11.258%
17	10.214	2840	2853	2866	rBV	55480	92169	21.25%	2.515%
18	10.381	2894	2905	2916	rBV	9222	15205	3.51%	0.415%
19	11.246	3163	3174	3192	rBV	225484	353309	81.46%	9.642%
20	11.622	3277	3291	3313	rBV	182704	290858	67.06%	7.938%




Sum of corrected areas: 3664200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025308.D
Acq On : 30 Mar 2022 11:39
Operator : SY/MD
Sample : N2165-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

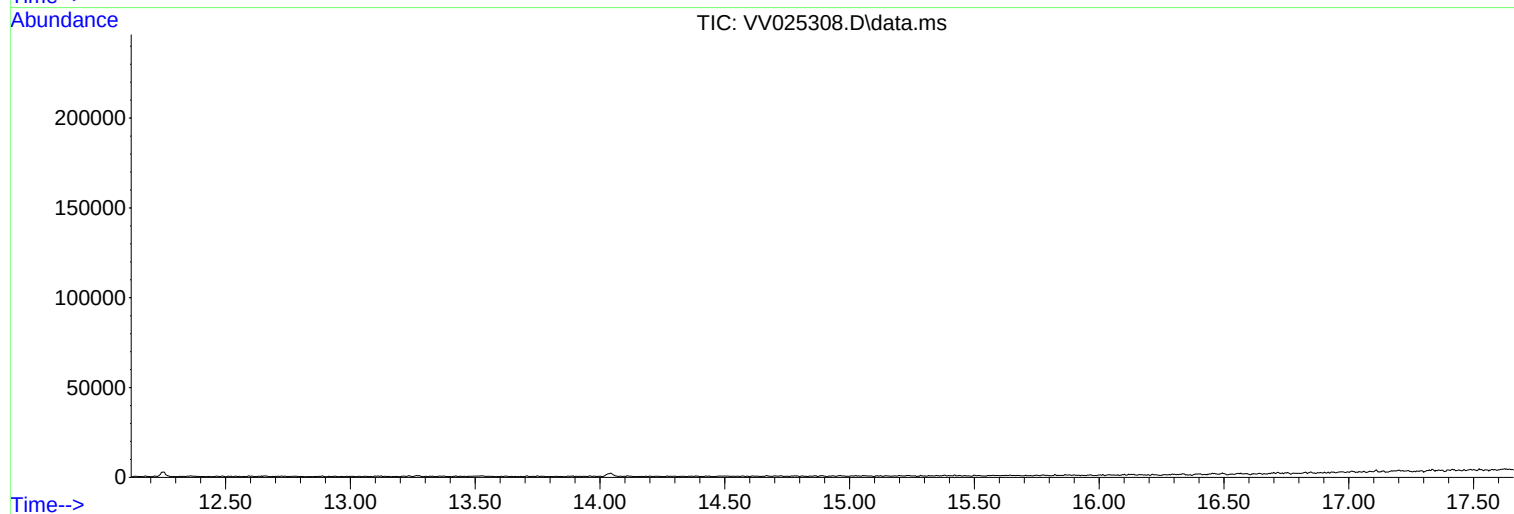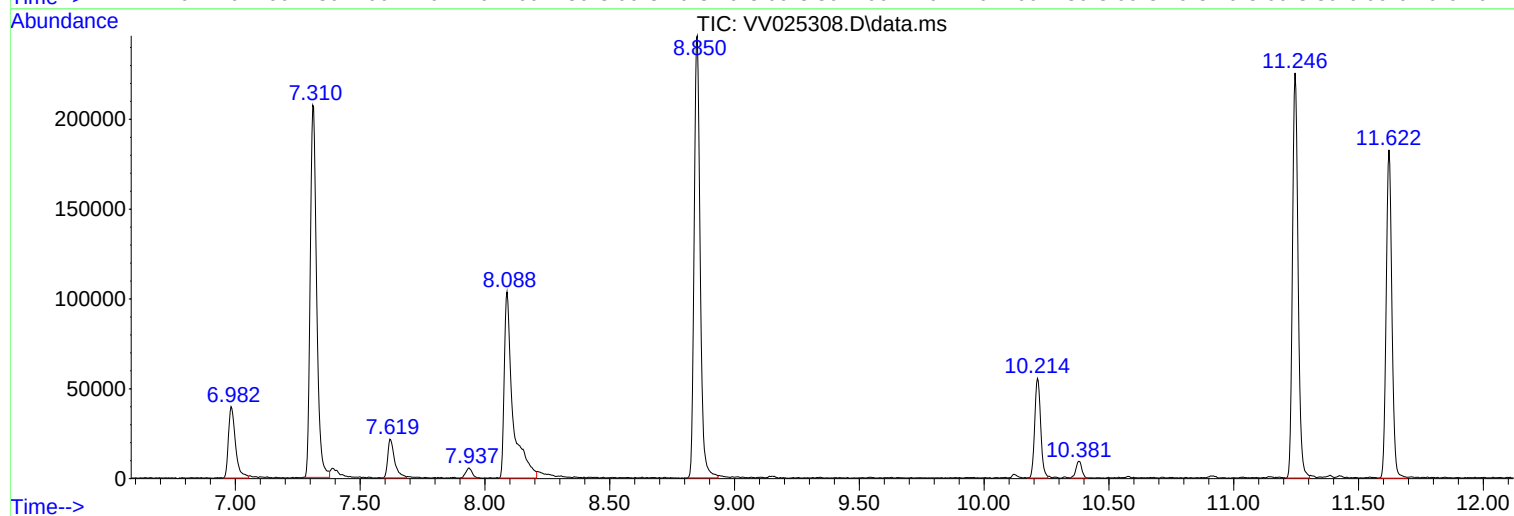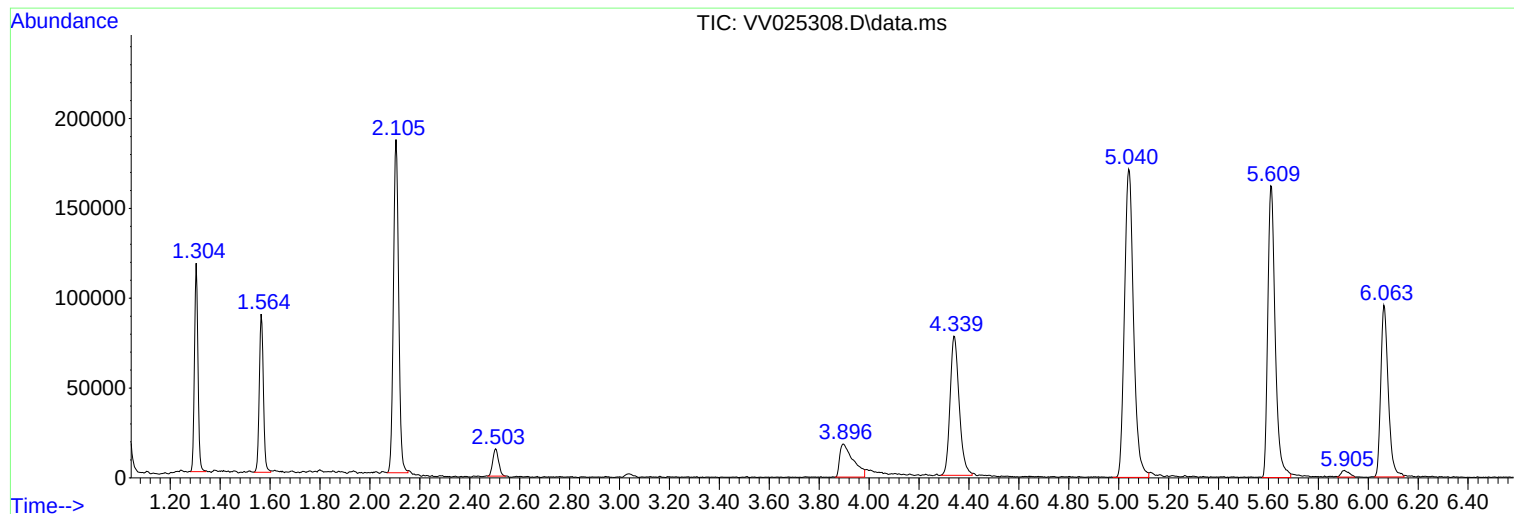

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025308.D
Acq On : 30 Mar 2022 11:39
Operator : SY/MD
Sample : N2165-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025308.D
Acq On : 30 Mar 2022 11:39
Operator : SY/MD
Sample : N2165-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc