

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
 Data File : VV025309.D
 Acq On : 30 Mar 2022 12:02
 Operator : SY/MD
 Sample : N2165-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	115283	116720	25.60%	3.024%
2	1.568	156	164	175	rBV	91523	105002	23.03%	2.721%
3	2.111	322	333	356	rVB	196764	295598	64.82%	7.659%
4	2.510	447	457	470	rBV2	14058	24004	5.26%	0.622%
5	3.908	882	892	919	rBV2	19988	73171	16.05%	1.896%
6	4.349	1013	1029	1059	rVB2	80282	208630	45.75%	5.406%
7	5.047	1230	1246	1271	rBV3	180873	455999	100.00%	11.816%
8	5.616	1411	1423	1446	rBV	167000	343746	75.38%	8.907%
9	5.911	1501	1515	1520	rBV6	3943	7221	1.58%	0.187%
10	6.069	1552	1564	1588	rBV	102826	213638	46.85%	5.536%
11	6.989	1840	1850	1869	rBV2	42462	81797	17.94%	2.119%
12	7.317	1936	1952	1971	rBV	225244	389760	85.47%	10.099%
13	7.625	2038	2048	2071	rBV	23503	42813	9.39%	1.109%
14	7.940	2136	2146	2155	rBV3	4634	8368	1.84%	0.217%
15	8.091	2183	2193	2225	rBV2	114950	265515	58.23%	6.880%
16	8.850	2419	2429	2453	rBV	254588	425823	93.38%	11.034%
17	10.214	2843	2853	2870	rBV	61050	101179	22.19%	2.622%
18	10.381	2896	2905	2915	rVB3	9875	15561	3.41%	0.403%
19	11.246	3163	3174	3195	rBV	236876	369003	80.92%	9.561%
20	11.622	3279	3291	3310	rBV	193566	310911	68.18%	8.056%
21	12.246	3477	3485	3496	rVB2	3370	4847	1.06%	0.126%




Sum of corrected areas: 3859306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025309.D
Acq On : 30 Mar 2022 12:02
Operator : SY/MD
Sample : N2165-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

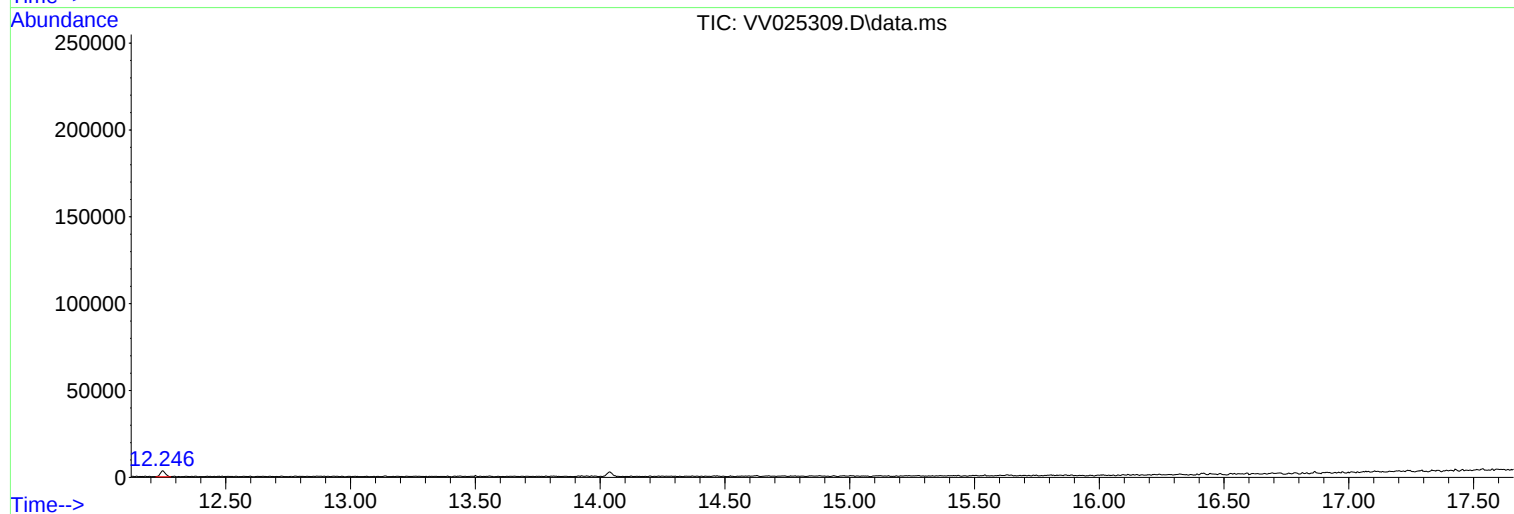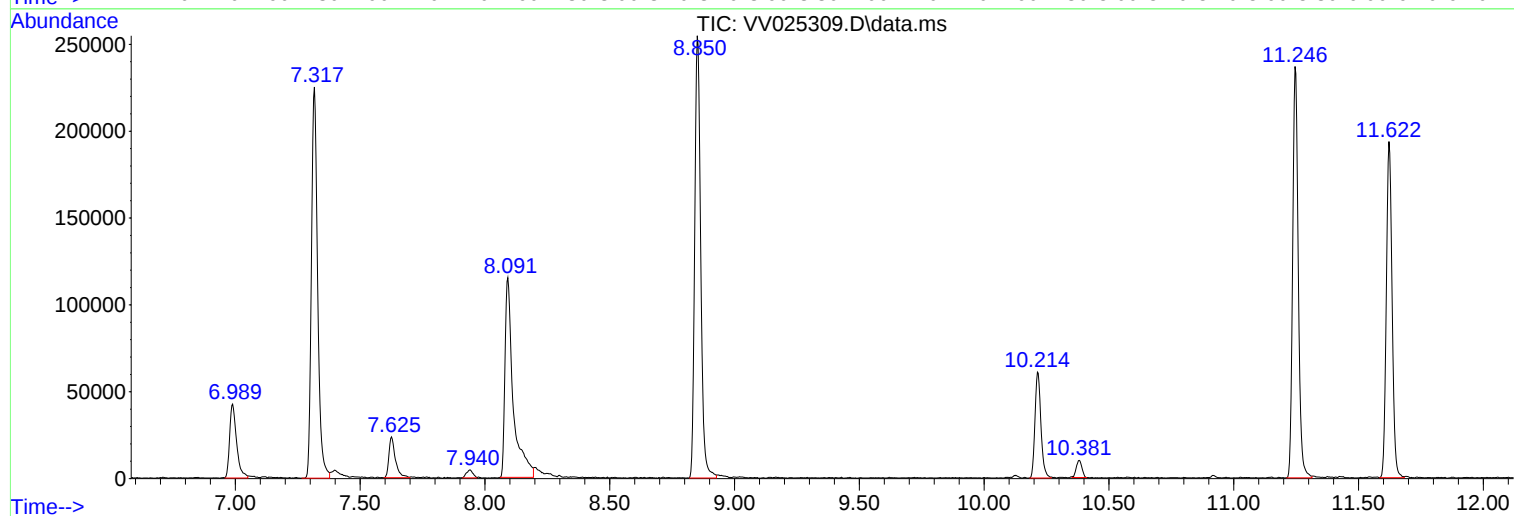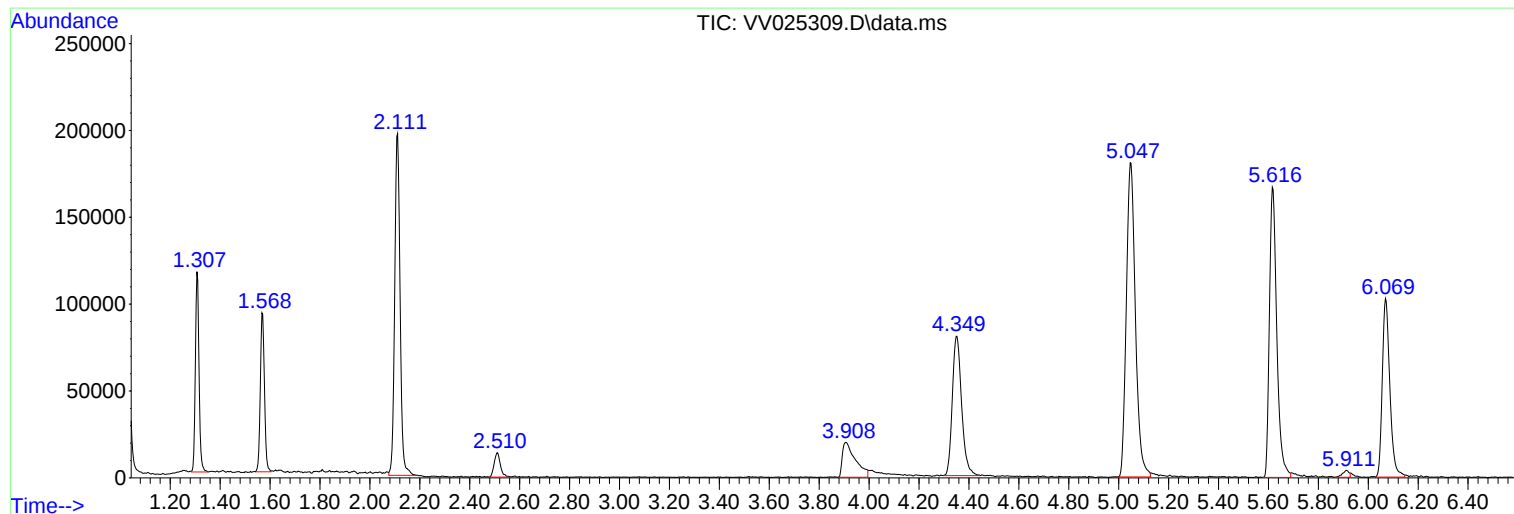

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025309.D
Acq On : 30 Mar 2022 12:02
Operator : SY/MD
Sample : N2165-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025309.D
Acq On : 30 Mar 2022 12:02
Operator : SY/MD
Sample : N2165-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc