

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
 Data File : VV025310.D
 Acq On : 30 Mar 2022 12:26
 Operator : SY/MD
 Sample : N2165-06DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6P3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	113284	113663	17.43%	2.581%
2	1.568	156	164	179	rVB	88086	101984	15.64%	2.316%
3	2.111	322	333	356	rVB	202487	303226	46.49%	6.886%
4	2.510	449	457	471	rVB3	4276	7450	1.14%	0.169%
5	3.915	884	894	928	rBV2	20363	96433	14.79%	2.190%
6	4.352	1014	1030	1052	rBV	78546	201775	30.94%	4.582%
7	5.050	1231	1247	1272	rBV2	181085	453569	69.54%	10.299%
8	5.619	1410	1424	1444	rBV	152703	317260	48.64%	7.204%
9	5.915	1505	1516	1529	rBV	4694	10111	1.55%	0.230%
10	6.069	1551	1564	1594	rBV	97841	210712	32.31%	4.785%
11	6.989	1838	1850	1873	rBV2	41147	81113	12.44%	1.842%
12	7.317	1939	1952	1971	rBV	215668	382325	58.62%	8.682%
13	7.625	2039	2048	2067	rBV	22947	40370	6.19%	0.917%
14	7.972	2132	2156	2178	rBV	378579	652223	100.00%	14.810%
15	8.091	2184	2193	2222	rBV	129158	279671	42.88%	6.351%
16	8.850	2419	2429	2448	rBV	237427	392768	60.22%	8.919%
17	10.217	2843	2854	2865	rBV2	62640	99456	15.25%	2.258%
18	10.381	2892	2905	2916	rBV2	8249	12791	1.96%	0.290%
19	11.246	3164	3174	3194	rBV	217644	341617	52.38%	7.757%
20	11.622	3279	3291	3309	rBV	195197	305299	46.81%	6.933%




Sum of corrected areas: 4403816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025310.D
Acq On : 30 Mar 2022 12:26
Operator : SY/MD
Sample : N2165-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

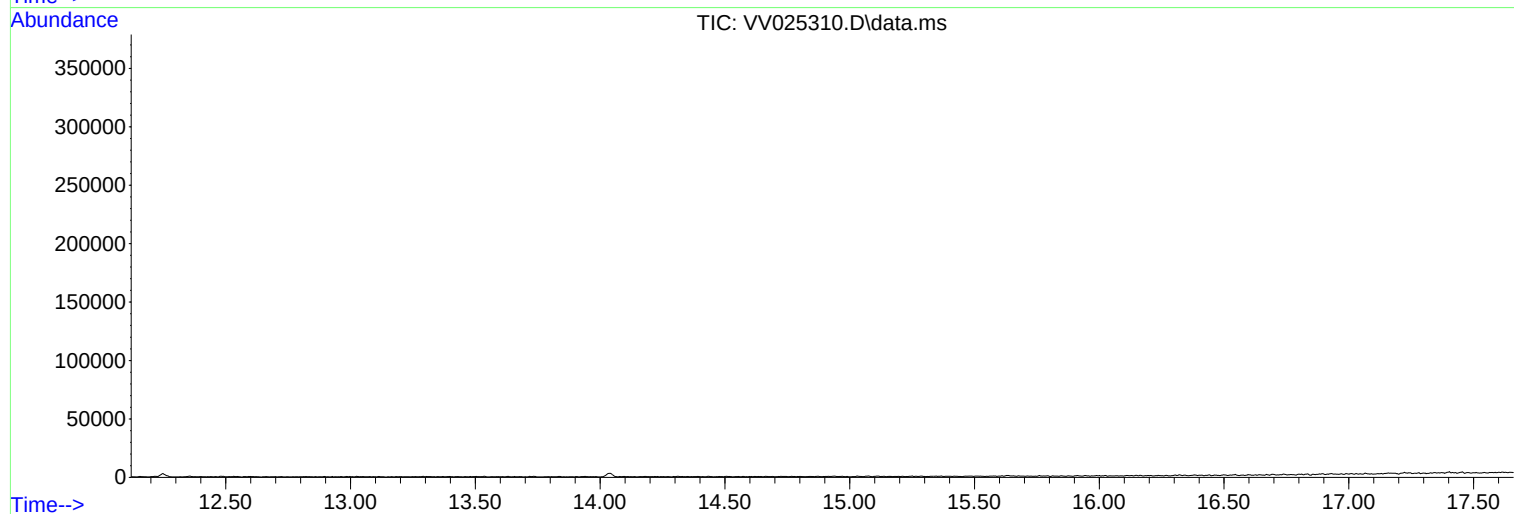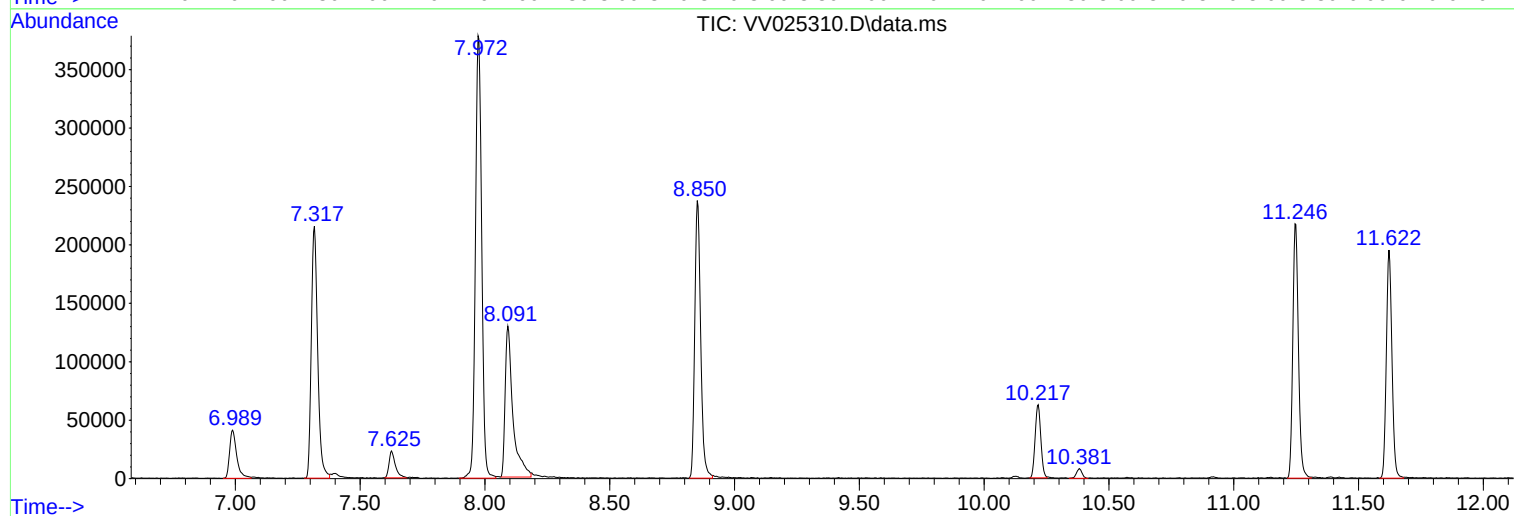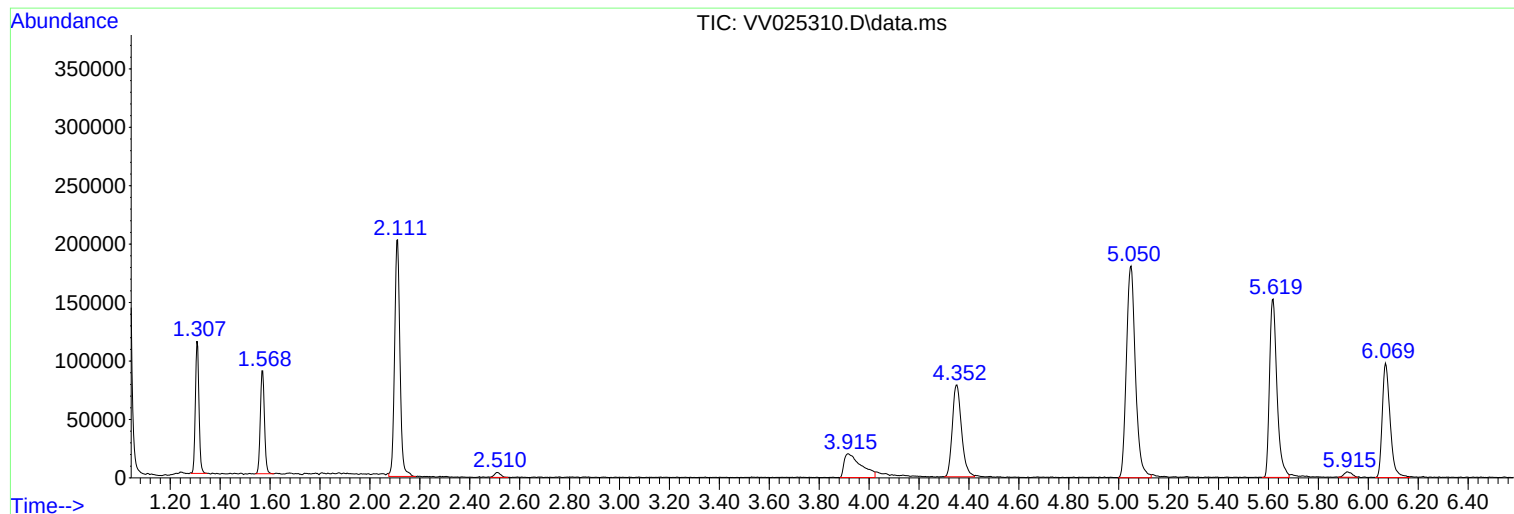

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025310.D
Acq On : 30 Mar 2022 12:26
Operator : SY/MD
Sample : N2165-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
Data File : VV025310.D
Acq On : 30 Mar 2022 12:26
Operator : SY/MD
Sample : N2165-06DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc