


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033022\
 Data File : VV025305.D
 Acq On : 30 Mar 2022 09:35
 Operator : SY/MD
 Sample : BFB291
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB291

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 02 00:37:35 2022

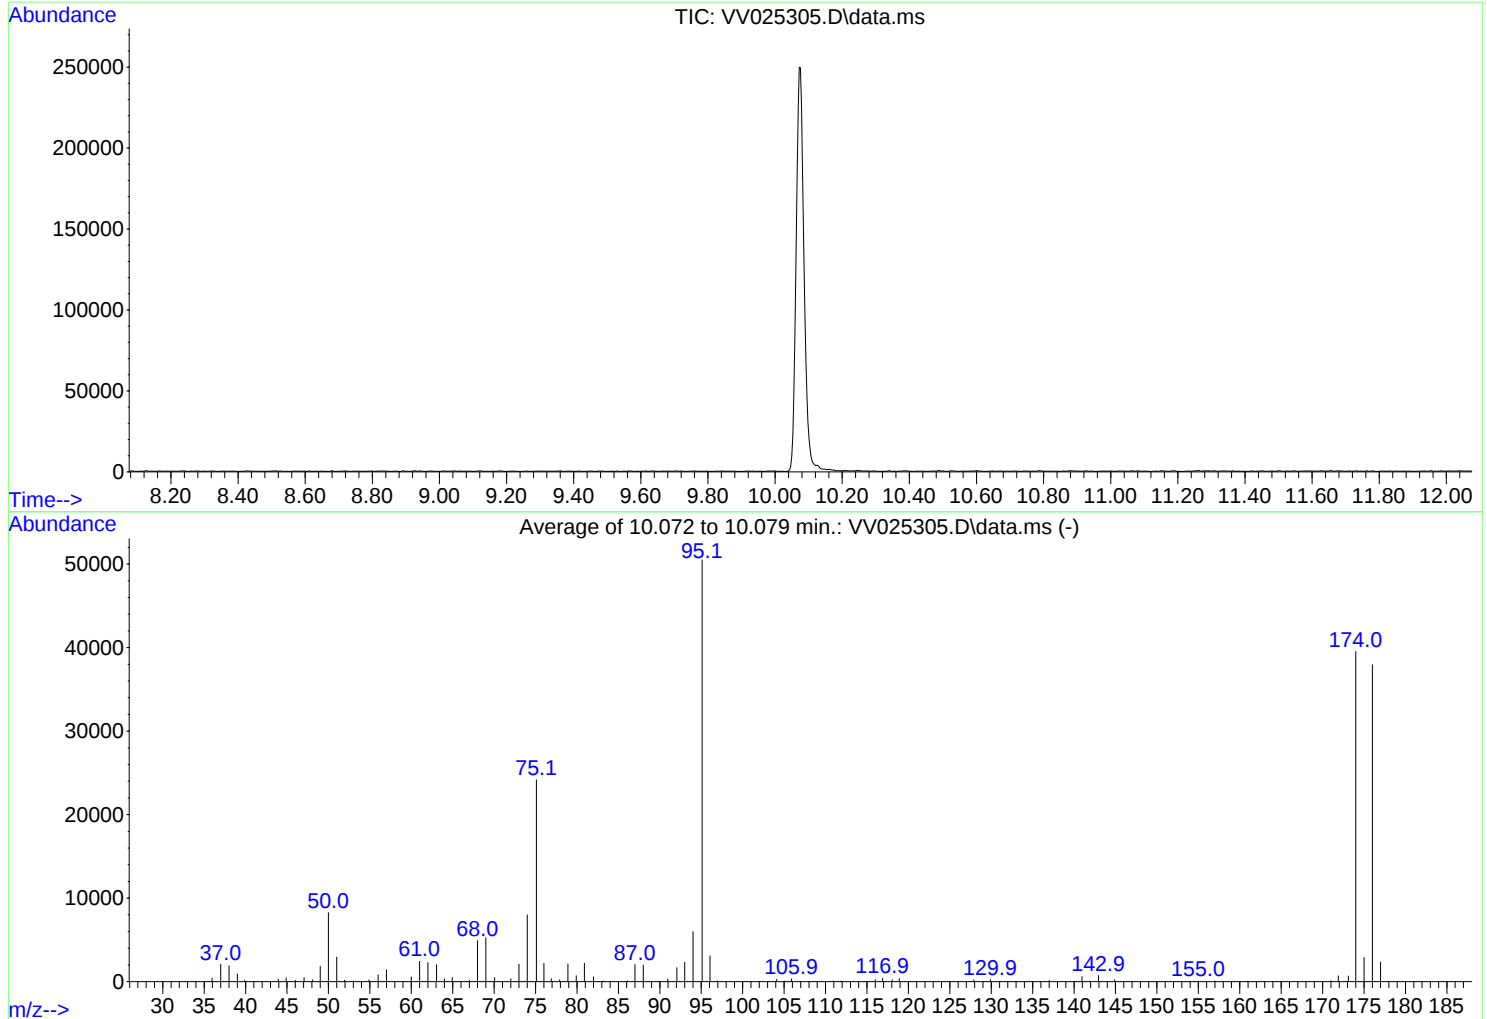

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8257	PASS
75	95	30	80	47.8	24163	PASS
95	95	100	100	100.0	50507	PASS
96	95	5	9	6.1	3087	PASS
173	174	0.00	2	1.7	667	PASS
174	95	50	120	78.2	39517	PASS
175	174	5	9	7.3	2893	PASS
176	174	95	105	96.0	37952	PASS
177	176	5	10	6.2	2338	PASS

m/z	Abundance
43.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
36.00	417.0
37.00	1970.0
38.00	1940.0
39.00	956.0
39.90	193.0
44.00	504.0
44.90	440.0
46.10	146.0
47.00	497.0
48.00	305.0
49.00	1936.0
50.00	8649.0
51.00	3014.0
52.00	193.0
53.00	134.0
54.90	231.0
56.00	903.0
57.00	1443.0
60.00	671.0
61.00	2538.0
62.00	2302.0
63.10	2284.0
64.00	298.0
65.10	484.0
67.10	158.0
68.00	5043.0
69.00	5508.0
70.00	545.0
72.00	307.0
73.00	2228.0
74.00	8406.0
75.10	25480.0
76.00	2260.0
76.90	373.0
77.90	199.0
78.90	2239.0
79.90	703.0
80.90	2282.0
82.00	577.0
86.90	2117.0
88.00	2041.0
91.00	356.0
92.00	1767.0
93.00	2562.0
94.00	6317.0
95.10	51696.0
96.00	3147.0
96.90	148.0
104.10	281.0
105.90	347.0
116.00	247.0
116.90	483.0
118.00	223.0
118.90	367.0
127.90	228.0
129.90	255.0
130.90	132.0
137.00	149.0
141.00	586.0
141.90	114.0
142.90	758.0
144.90	215.0
148.10	124.0
154.50	106.0
155.00	145.0
157.00	107.0
161.00	100.0
171.00	114.0
171.90	694.0
173.10	696.0
174.00	40216.0
175.00	3080.0
176.00	38776.0
177.00	2400.0
178.00	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	402.0
37.00	2075.0
38.00	1785.0
39.00	846.0
39.90	156.0
44.00	433.0
44.90	430.0
45.90	173.0
47.10	476.0
48.20	174.0
49.00	1684.0
50.00	7675.0
51.00	2760.0
51.90	161.0
54.90	164.0
56.00	712.0
57.00	1317.0
60.00	429.0
61.00	2272.0
62.00	2241.0
63.00	1724.0
64.00	326.0
64.90	498.0
67.00	147.0
68.00	4533.0
69.00	4796.0
70.10	417.0
72.00	343.0
73.00	1881.0
74.00	7365.0
75.10	22256.0
76.00	2024.0
76.90	321.0
77.90	214.0
78.90	1987.0
79.90	675.0
80.90	2071.0
82.00	533.0
83.20	130.0
86.10	162.0
87.10	2005.0
88.00	1879.0
90.90	241.0
92.10	1485.0
93.00	2026.0
94.00	5491.0
95.10	47320.0
96.10	2967.0
104.10	270.0
105.10	118.0
105.90	301.0
110.90	115.0
111.80	120.0
116.00	212.0
116.90	288.0
118.00	193.0
118.90	344.0
127.90	190.0
129.90	190.0
137.00	115.0
140.90	622.0
143.00	683.0
144.90	253.0
171.00	120.0
171.90	672.0
173.10	617.0
174.00	37448.0
175.00	2659.0
176.00	36096.0
177.00	2194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	415.0
37.00	2146.0
38.00	1952.0
39.00	937.0
39.90	158.0
44.00	454.0
44.90	468.0
46.00	164.0
47.00	485.0
48.10	229.0
49.00	1892.0
50.00	8446.0
51.00	3022.0
52.00	195.0
53.00	128.0
54.90	219.0
56.00	847.0
57.00	1482.0
60.00	597.0
61.00	2514.0
62.00	2323.0
63.10	2087.0
64.00	332.0
64.90	481.0
67.10	144.0
68.00	5155.0
69.00	5431.0
70.00	478.0
72.00	372.0
73.00	2138.0
74.00	8215.0
75.10	24752.0
76.00	2276.0
76.90	346.0
77.90	225.0
78.90	2159.0
79.90	757.0
80.90	2276.0
82.00	609.0
83.10	113.0
86.10	146.0
87.00	2058.0
88.00	1982.0
91.00	324.0
92.00	1725.0
93.00	2361.0
94.00	6184.0
95.10	52504.0
96.00	3147.0
96.90	136.0
104.10	321.0
105.10	119.0
105.90	354.0
110.90	105.0
111.90	105.0
116.00	247.0
116.90	394.0
118.10	213.0
118.90	402.0
127.90	226.0
129.90	255.0
137.00	137.0
141.00	612.0
141.90	104.0
142.90	728.0
144.90	247.0
155.00	111.0
157.00	103.0
160.90	102.0
171.00	129.0
171.90	694.0
173.10	689.0
174.00	40888.0
175.00	2940.0
176.00	38984.0
177.00	2419.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291