

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
 Data File : VV025326.D
 Acq On : 31 Mar 2022 10:58
 Operator : SY/MD
 Sample : VV0331WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Quant Time: Apr 01 01:32:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 01 01:30:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	138461	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	129741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	54353	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	68362	5.286	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	105.800%	
7) Chloroethane-d5	1.568	69	54847	5.053	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.000%	
11) 1,1-Dichloroethene-d2	2.105	63	102941	3.674	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.400%	
20) 2-Butanone-d5	3.912	46	58060	45.066	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.140%	
24) Chloroform-d	4.346	84	82423	4.883	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.030	65	37886	5.078	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.600%	
32) Benzene-d6	5.043	84	162041	4.937	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6	6.066	67	46421	5.046	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.000%	
41) Toluene-d8	7.313	98	136186	4.524	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	7.622	79	14169	4.722	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.088	63	47032	43.395	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	86.780%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29416	4.796	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	45182	5.176	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	2793	0.255	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025326.D
Acq On : 31 Mar 2022 10:58
Operator : SY/MD
Sample : VV0331WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331


Quant Time: Apr 01 01:32:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 01 01:30:42 2022
Response via : Initial Calibration

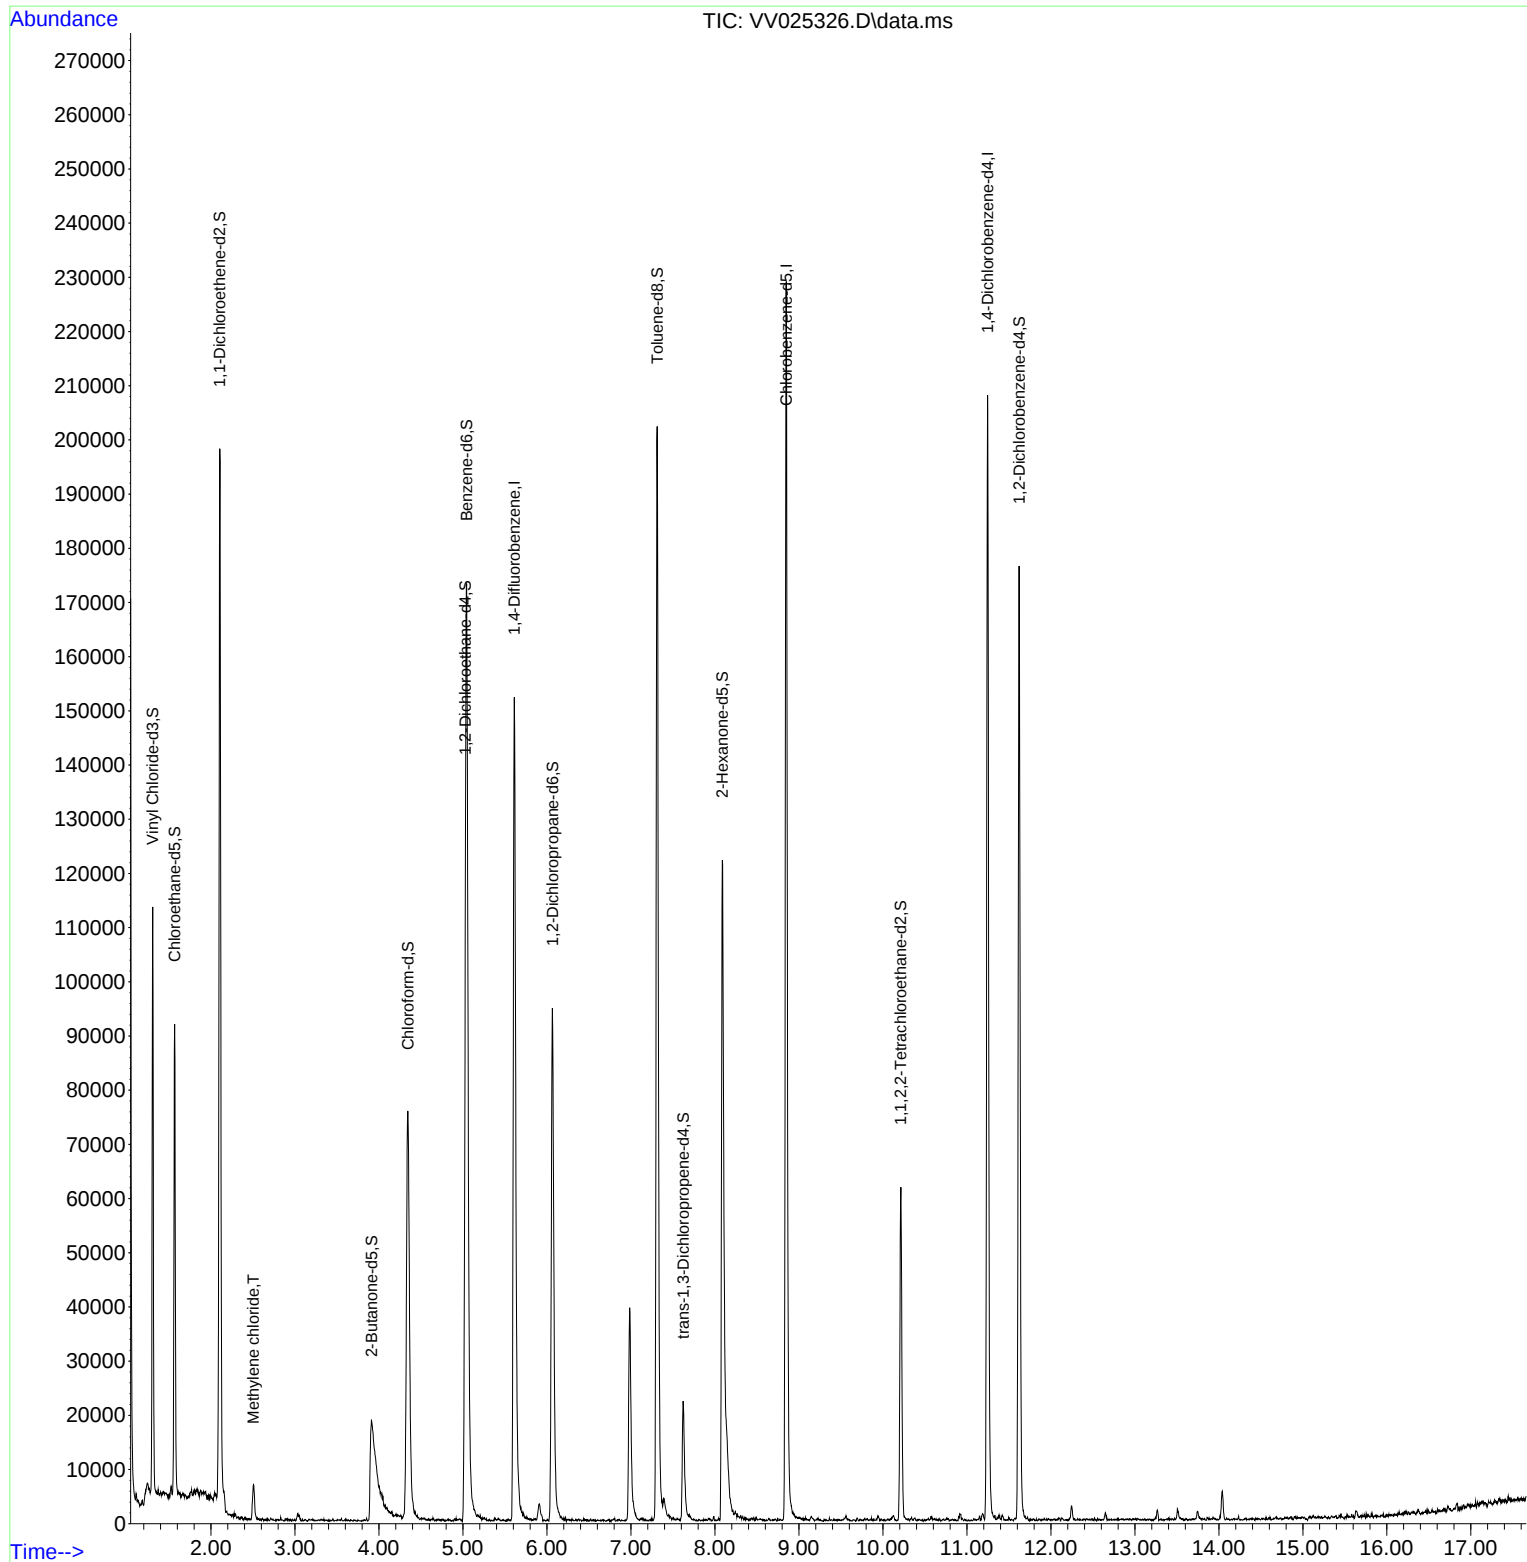

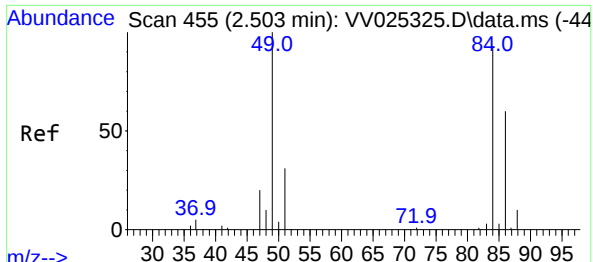

#16
Methylene chloride
Concen: 0.255 ug/L
RT: 2.503 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV025326.D
Acq: 31 Mar 2022 10:58

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

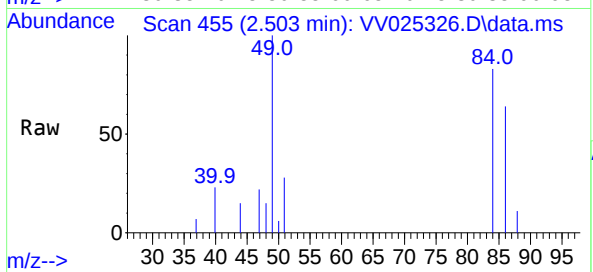

Tgt Ion: 84 Resp: 2793

Ion	Ratio	Lower	Upper
84	100		
86	76.3	43.5	80.7
49	119.8	74.5	138.3

