

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033122\
 Data File : VW025331.D
 Acq On : 31 Mar 2022 14:25
 Operator : SY/MD
 Sample : N2179-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

Quant Time: Apr 01 01:33:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 01 01:30:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	130821	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125810	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	53831	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57310	4.690	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.800%	
7) Chloroethane-d5	1.568	69	50961	4.969	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.108	63	83074	3.139	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.800%	
20) 2-Butanone-d5	3.892	46	54239	44.559	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.120%	
24) Chloroform-d	4.349	84	75904	4.760	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	5.034	65	34489	4.893	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
32) Benzene-d6	5.050	84	151314	4.754	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.000%	
36) 1,2-Dichloropropane-d6	6.072	67	43487	4.875	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.600%	
41) Toluene-d8	7.317	98	128312	4.395	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.000%	
43) trans-1,3-Dichloroprop...	7.628	79	12452	4.279	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.600%	
46) 2-Hexanone-d5	8.088	63	44144	42.003	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.000%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27188	4.571	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	42032	4.862	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.200%	
Target Compounds						Qvalue
3) Chloromethane	1.240	50	3645	0.237	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025331.D
Acq On : 31 Mar 2022 14:25
Operator : SY/MD
Sample : N2179-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R42


Quant Time: Apr 01 01:33:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 01 01:30:42 2022
Response via : Initial Calibration

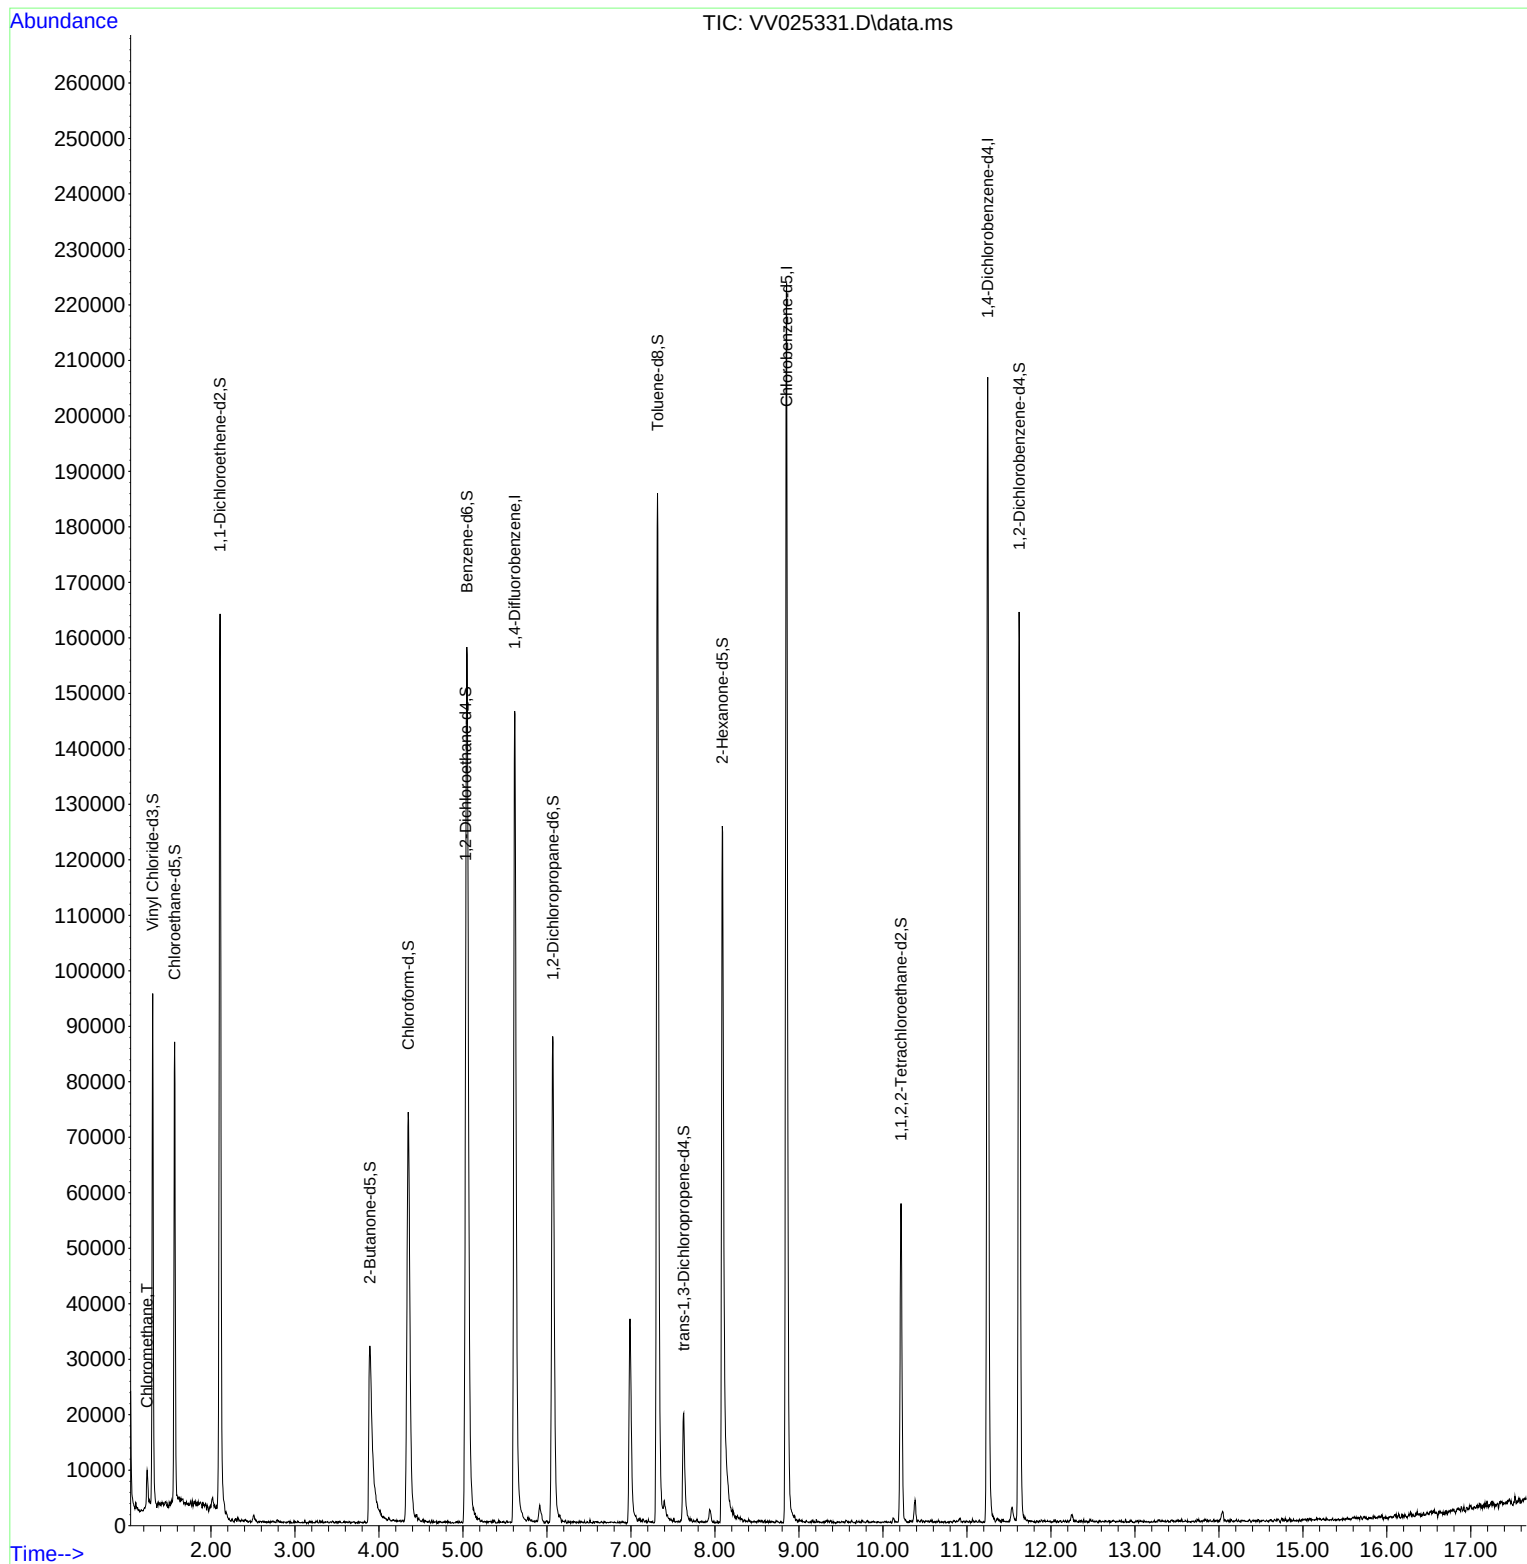

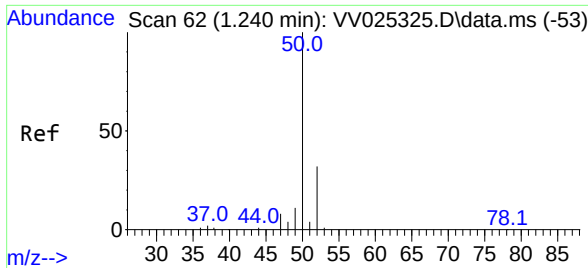

#3
 Chloromethane
 Concen: 0.237 ug/L
 RT: 1.240 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: VV025331.D
 Acq: 31 Mar 2022 14:25

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R42

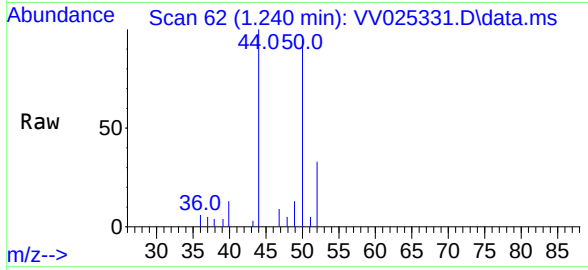

Tgt Ion: 50 Resp: 3645

Ion	Ratio	Lower	Upper
50	100		
52	34.6	22.9	42.5

