

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW033122\
 Data File : VW025334.D
 Acq On : 31 Mar 2022 15:35
 Operator : SY/MD
 Sample : N2179-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R41

Quant Time: Apr 01 01:33:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 01 01:30:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122290	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	121043	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49264	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59634	5.221	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.400%
7) Chloroethane-d5	1.568	69	53851	5.617	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.400%
11) 1,1-Dichloroethene-d2	2.111	63	88262	3.567	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.400%
20) 2-Butanone-d5	3.889	46	60429	53.108	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.220%
24) Chloroform-d	4.349	84	81280	5.452	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.000%
26) 1,2-Dichloroethane-d4	5.034	65	36874	5.596	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	5.050	84	158306	5.170	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	6.069	67	45760	5.332	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%
41) Toluene-d8	7.316	98	133049	4.737	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	7.625	79	13172	4.705	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.000%
46) 2-Hexanone-d5	8.088	63	47770	47.243	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.480%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29869	5.220	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	46439	5.869	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.400%
Target Compounds					Qvalue	
13) Acetone	2.178	43	5783	6.660	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025334.D
Acq On : 31 Mar 2022 15:35
Operator : SY/MD
Sample : N2179-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0R41

Quant Time: Apr 01 01:33:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 01 01:30:42 2022
Response via : Initial Calibration

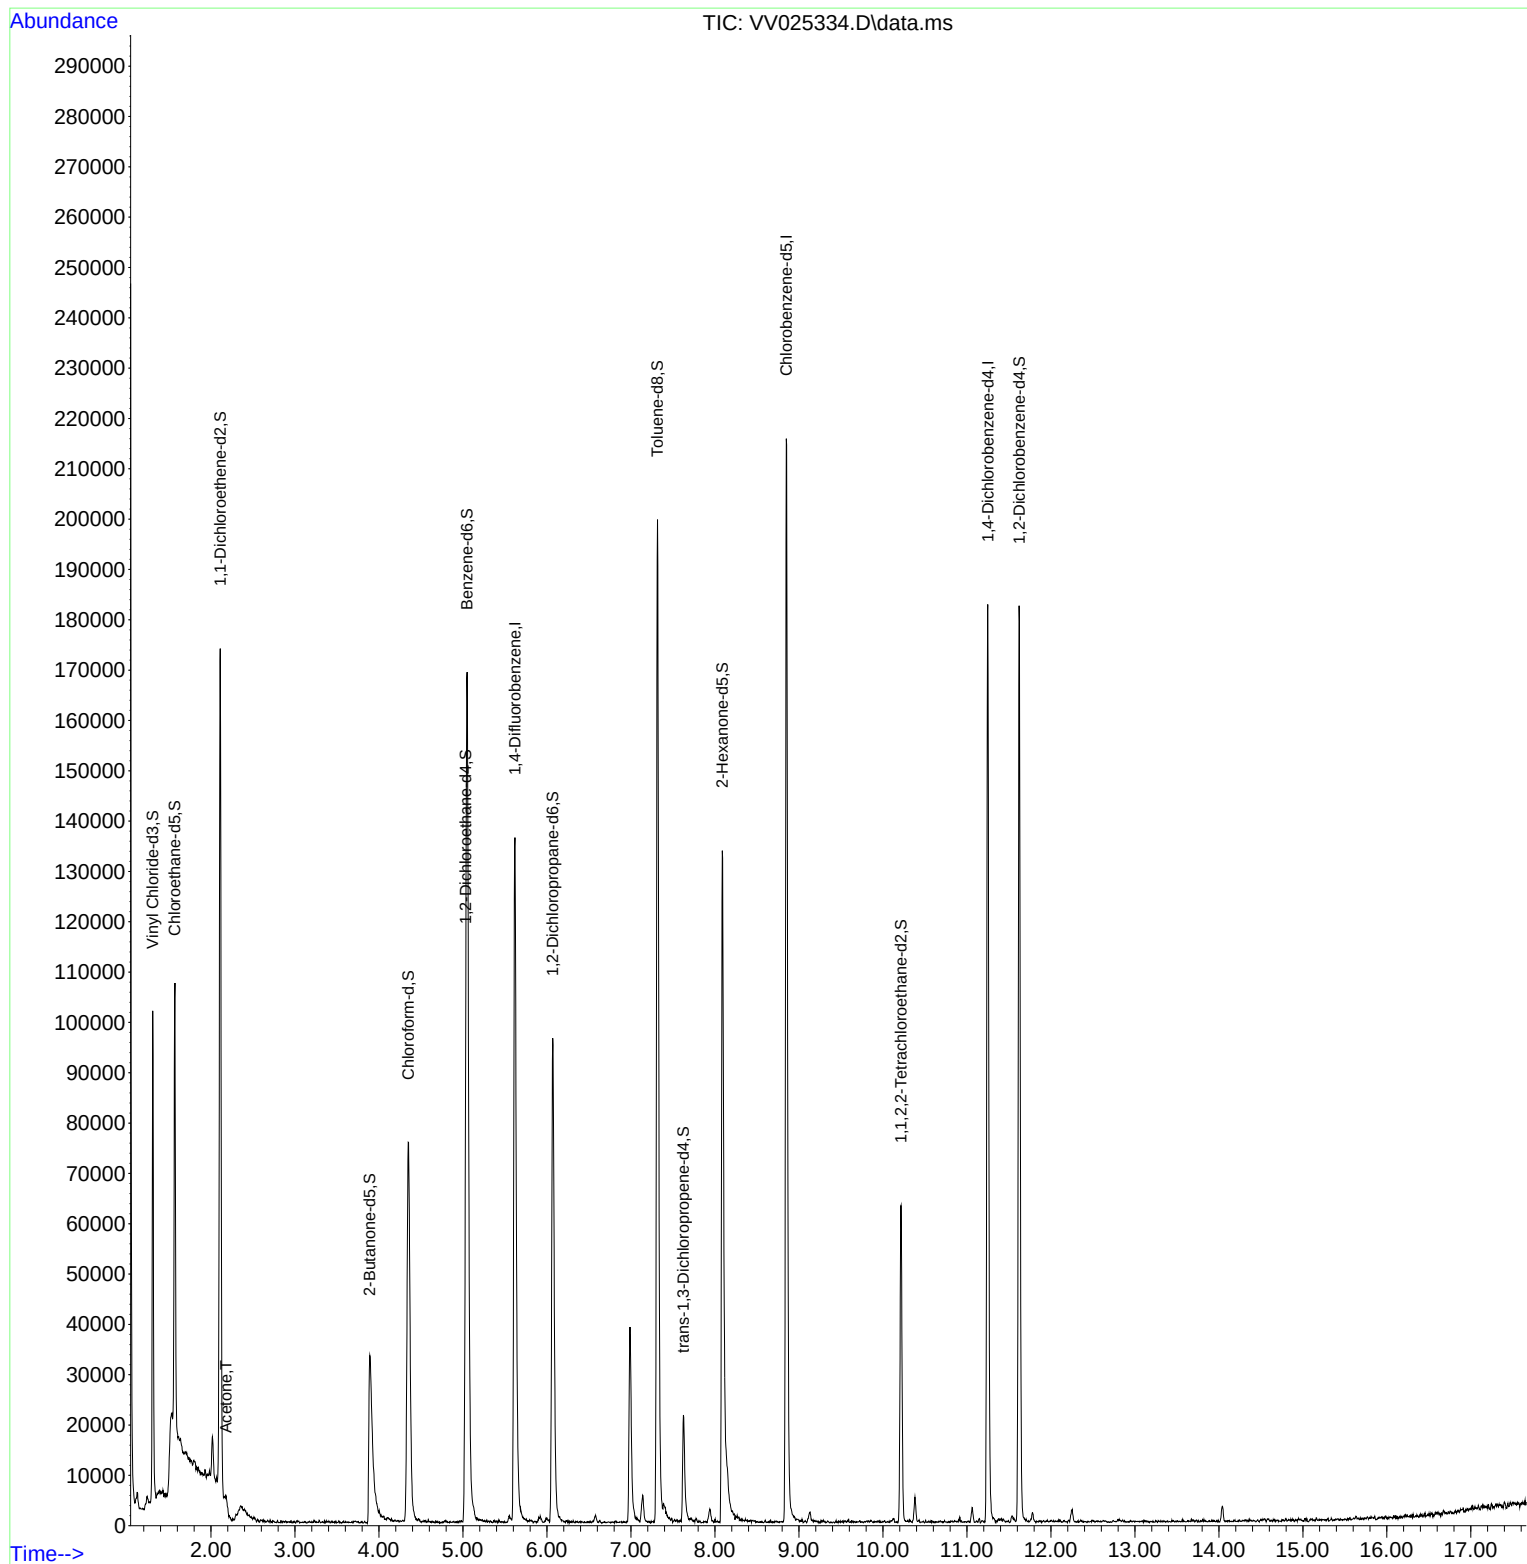

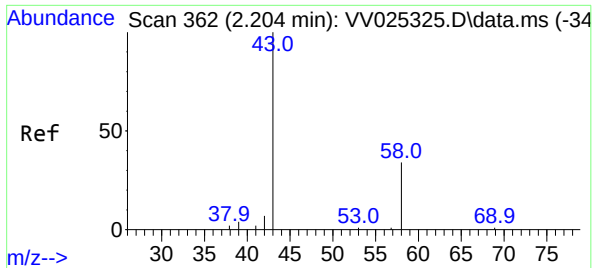

#13
 Acetone
 Concen: 6.660 ug/L
 RT: 2.178 min Scan# 31
 Delta R.T. -0.026 min
 Lab File: VV025334.D
 Acq: 31 Mar 2022 15:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0R41

Tgt Ion: 43 Resp: 5783
 Ion Ratio Lower Upper
 43 100
 58 39.5 0.0 51.2

