

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
 Data File : VV025326.D
 Acq On : 31 Mar 2022 10:58
 Operator : SY/MD
 Sample : VV0331WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	50	63	67	rBV7	3968	8834	2.05%	0.245%
2	1.307	76	83	101	rVB	108362	111235	25.78%	3.085%
3	1.568	156	164	175	rVB	86693	99510	23.06%	2.760%
4	2.105	320	331	345	rBV	193584	280400	64.98%	7.777%
5	2.506	447	456	469	rBV2	6509	11462	2.66%	0.318%
6	3.912	879	893	925	rBV2	18727	89603	20.76%	2.485%
7	4.342	1009	1027	1052	rBV	75019	193687	44.88%	5.372%
8	5.043	1230	1245	1274	rBV2	172988	431519	100.00%	11.968%
9	5.612	1409	1422	1445	rBV2	151991	317220	73.51%	8.798%
10	5.908	1504	1514	1528	rVB8	3212	7425	1.72%	0.206%
11	6.066	1549	1563	1585	rBV2	94722	200342	46.43%	5.556%
12	6.985	1834	1849	1870	rBV2	39346	78094	18.10%	2.166%
13	7.313	1935	1951	1971	rBV	201925	357454	82.84%	9.914%
14	7.390	1971	1975	1990	rVB3	3380	6501	1.51%	0.180%
15	7.622	2036	2047	2067	rBV2	21981	42586	9.87%	1.181%
16	8.088	2183	2192	2229	rBV	121701	273283	63.33%	7.579%
17	8.850	2414	2429	2452	rBV	228640	381289	88.36%	10.575%
18	10.214	2842	2853	2872	rBV2	61491	98932	22.93%	2.744%
19	11.246	3163	3174	3199	rBV	207515	327980	76.01%	9.096%
20	11.622	3280	3291	3306	rBV	175806	280017	64.89%	7.766%
21	14.040	4036	4043	4054	rVB3	5315	8227	1.91%	0.228%




Sum of corrected areas: 3605600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025326.D
Acq On : 31 Mar 2022 10:58
Operator : SY/MD
Sample : VV0331WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

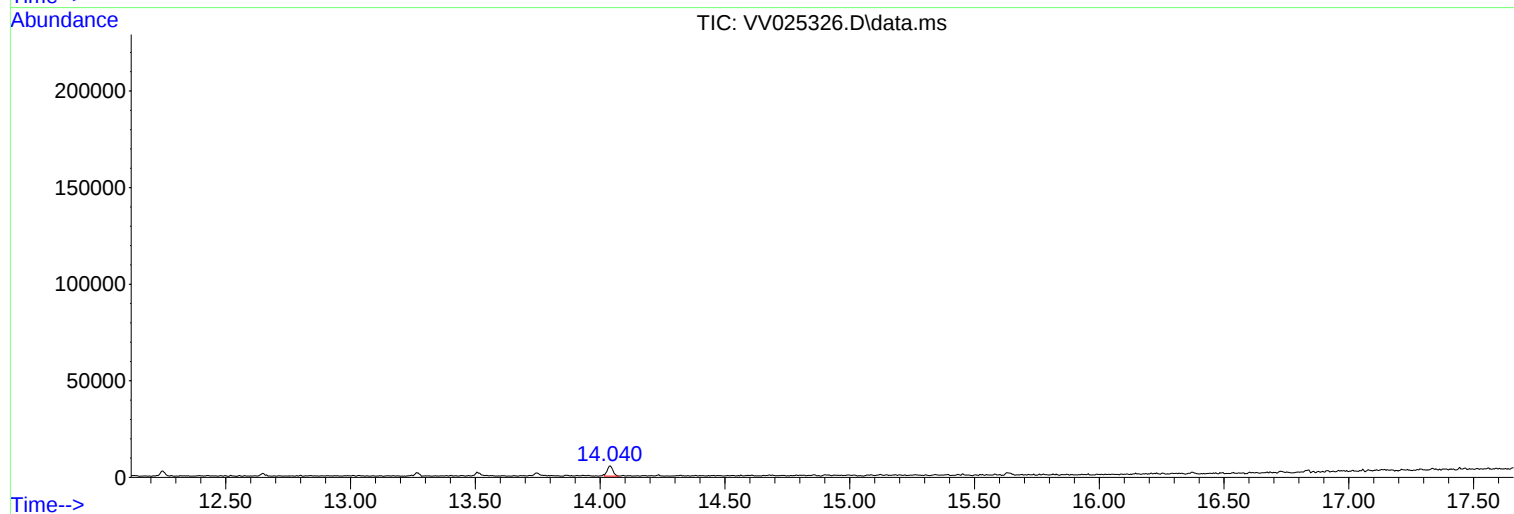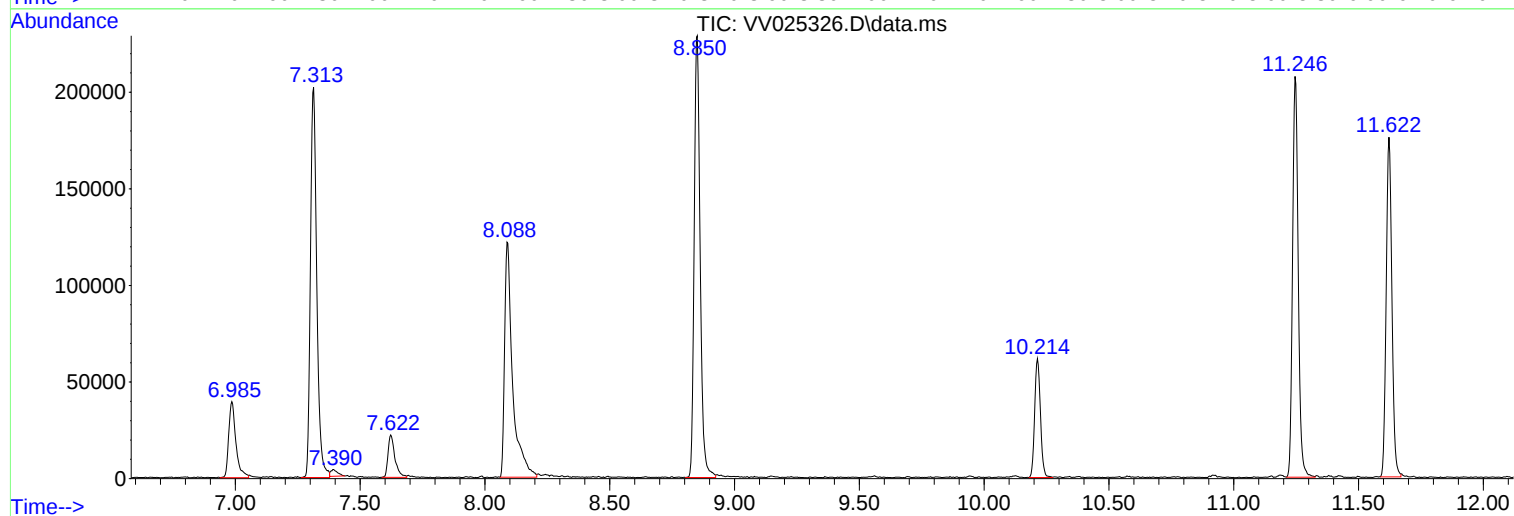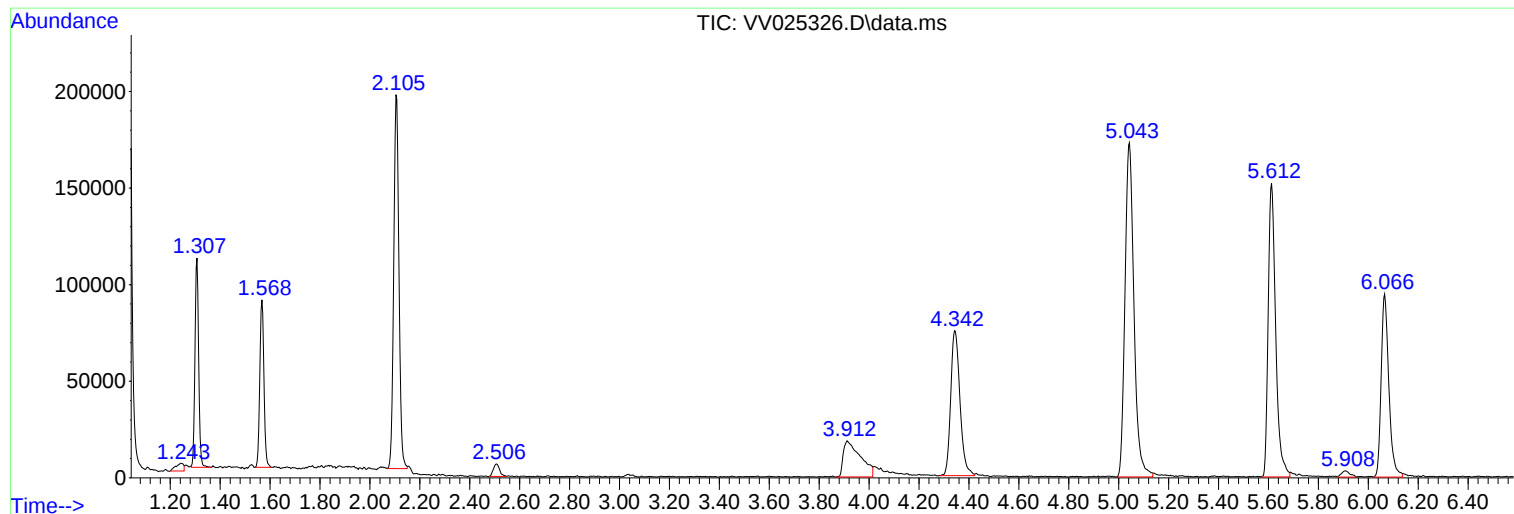

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025326.D
Acq On : 31 Mar 2022 10:58
Operator : SY/MD
Sample : VV0331WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV033122\
Data File : VV025326.D
Acq On : 31 Mar 2022 10:58
Operator : SY/MD
Sample : VV0331WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc