

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040122\
 Data File : VV025340.D
 Acq On : 01 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2179-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	92	rBV	91763	90801	23.16%	2.711%
2	1.568	157	164	176	rVB	75632	85391	21.78%	2.549%
3	2.108	322	332	350	rVB	155916	234420	59.80%	6.998%
4	2.507	445	456	471	rVB3	6429	11429	2.92%	0.341%
5	3.908	882	892	925	rBV2	20245	88142	22.49%	2.631%
6	4.349	1014	1029	1055	rBV2	70430	181239	46.24%	5.410%
7	5.047	1227	1246	1272	rBV3	156867	391992	100.00%	11.702%
8	5.616	1411	1423	1445	rBV	148061	305370	77.90%	9.116%
9	6.069	1551	1564	1590	rBV2	89230	188682	48.13%	5.632%
10	6.989	1840	1850	1870	rBV2	36348	70049	17.87%	2.091%
11	7.317	1939	1952	1970	rBV	176462	315967	80.61%	9.432%
12	7.625	2038	2048	2062	rBV3	20391	37391	9.54%	1.116%
13	8.092	2180	2193	2231	rBV2	118381	261512	66.71%	7.807%
14	8.850	2417	2429	2452	rBV	227198	380493	97.07%	11.358%
15	10.214	2843	2853	2868	rBV	58273	94841	24.19%	2.831%
16	11.246	3163	3174	3196	rBV	214557	334010	85.21%	9.971%
17	11.622	3280	3291	3312	rBV	168022	267612	68.27%	7.989%
18	12.249	3475	3486	3494	rBV2	3165	5128	1.31%	0.153%
19	14.040	4036	4043	4051	rVB3	3919	5440	1.39%	0.162%




Sum of corrected areas: 3349909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040122\
Data File : VV025340.D
Acq On : 01 Apr 2022 15:15
Operator : SY/MD
Sample : N2179-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

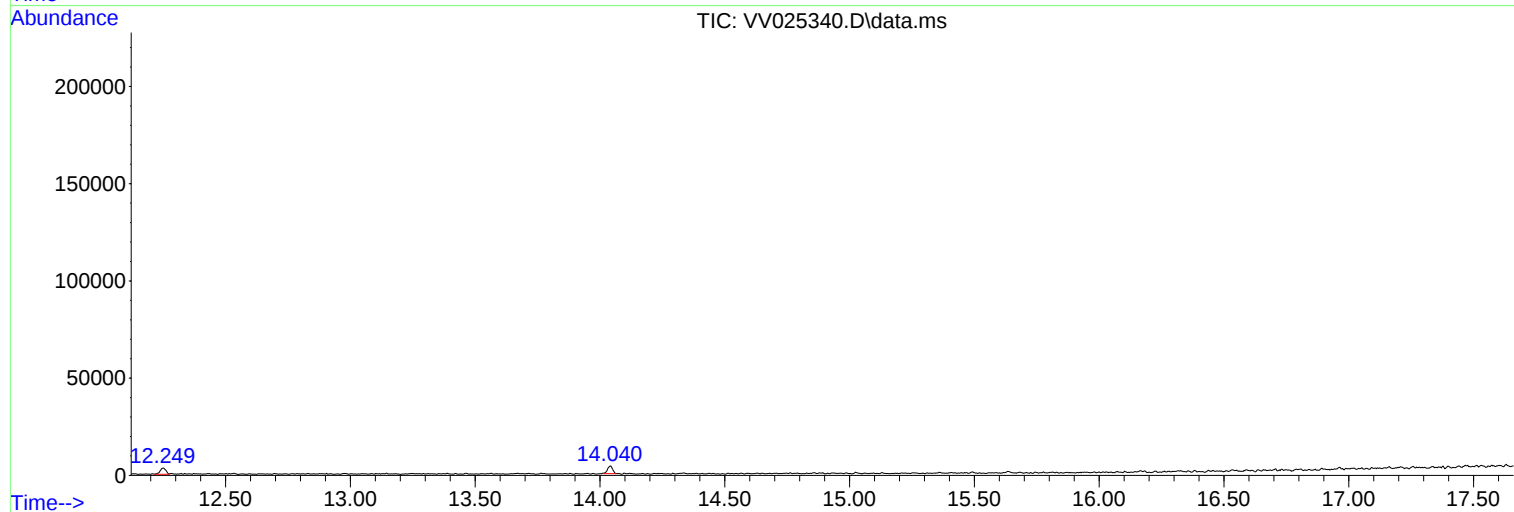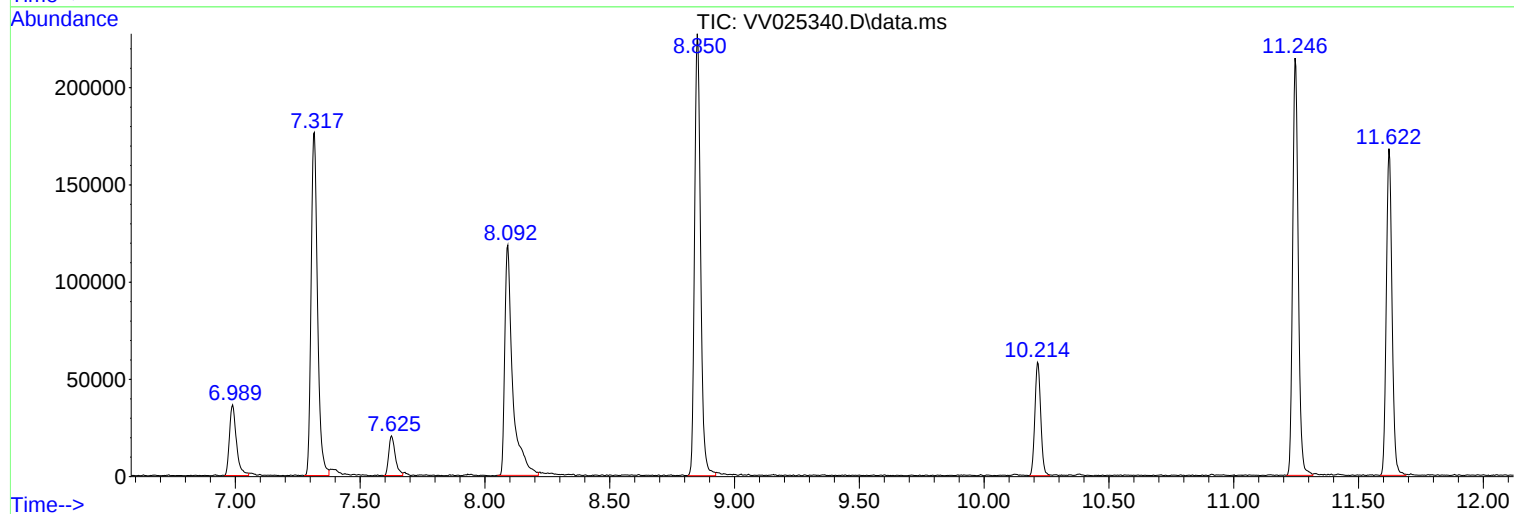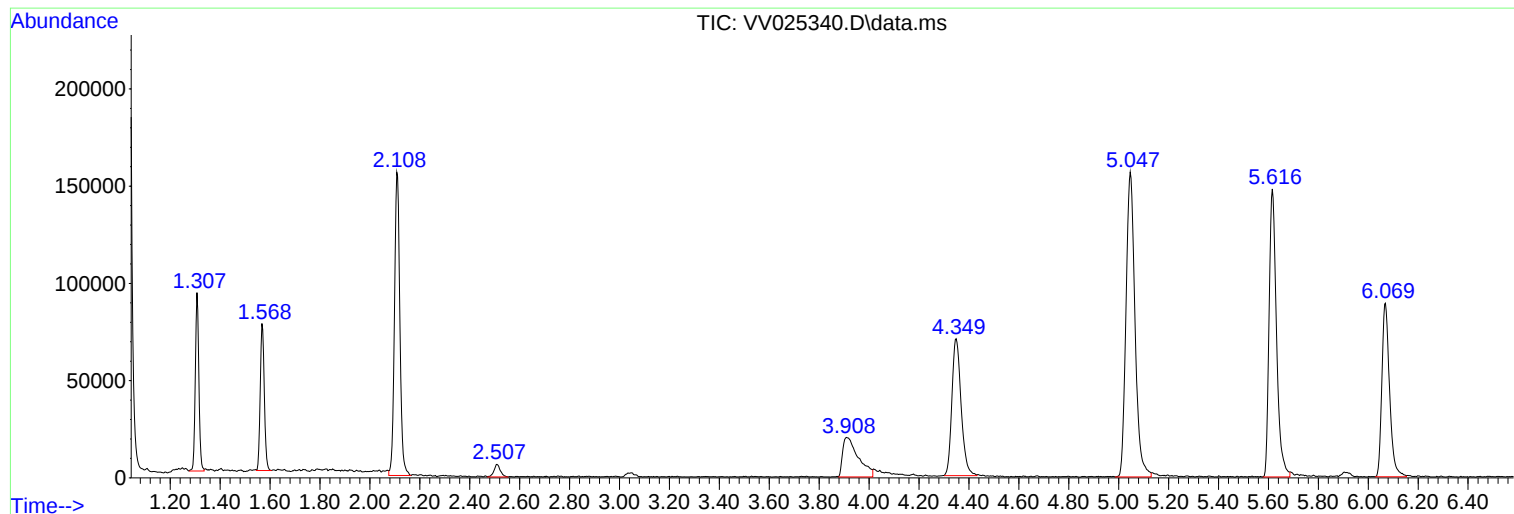

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040122\
Data File : VV025340.D
Acq On : 01 Apr 2022 15:15
Operator : SY/MD
Sample : N2179-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040122\
Data File : VV025340.D
Acq On : 01 Apr 2022 15:15
Operator : SY/MD
Sample : N2179-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc