
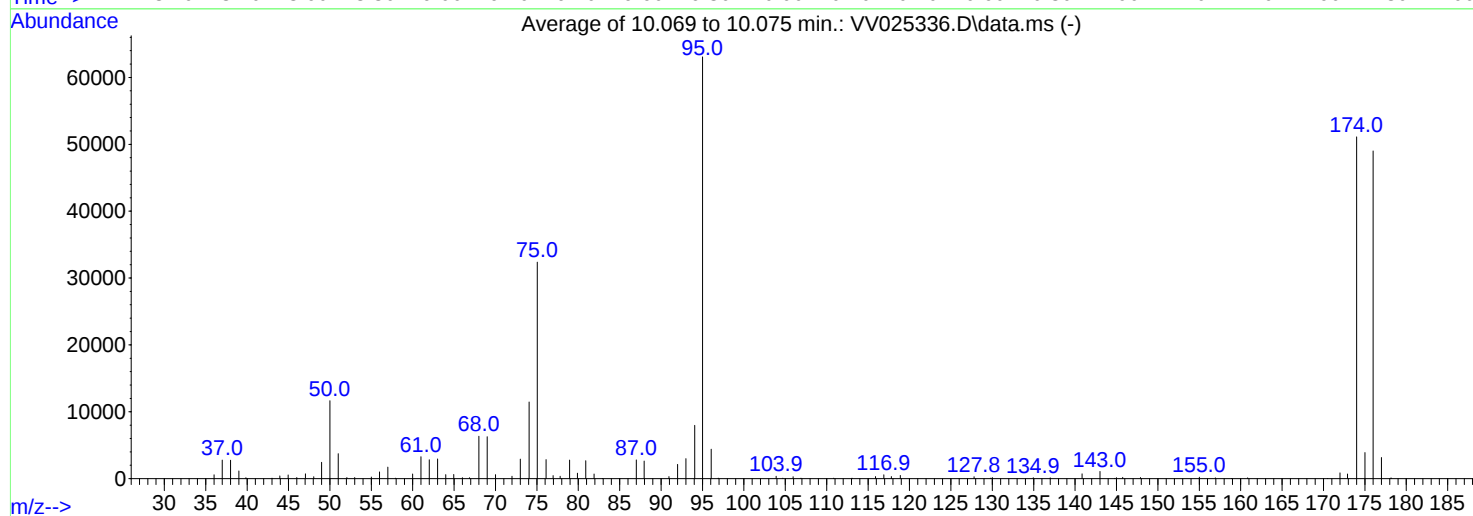


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040122\
 Data File : VV025336.D
 Acq On : 01 Apr 2022 08:53
 Operator : SY/MD
 Sample : BFB293
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB293

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 02 00:37:35 2022

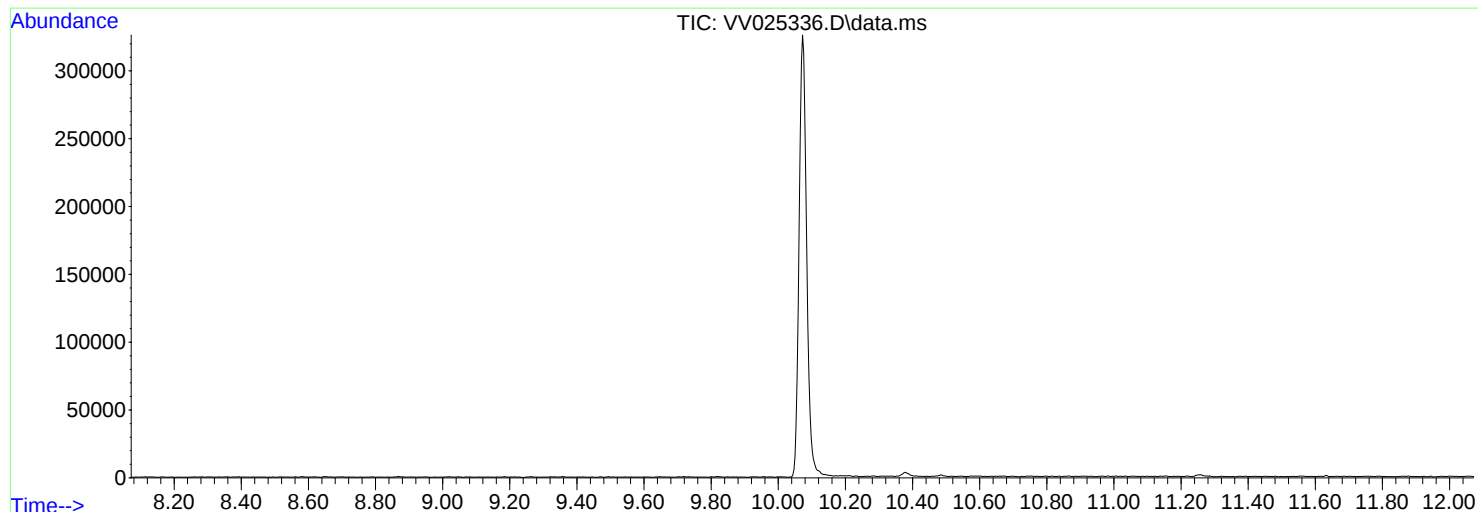

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	11646	PASS
75	95	30	80	51.3	32373	PASS
95	95	100	100	100.0	63085	PASS
96	95	5	9	7.0	4396	PASS
173	174	0.00	2	1.4	696	PASS
174	95	50	120	81.0	51117	PASS
175	174	5	9	7.7	3912	PASS
176	174	95	105	95.9	49011	PASS
177	176	5	10	6.4	3153	PASS

m/z	Abundance
39.80	267.0
44.10	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	573.0
37.00	2676.0
38.00	2683.0
39.00	1169.0
40.00	332.0
43.90	578.0
45.00	564.0
46.10	153.0
47.00	746.0
48.00	295.0
49.00	2587.0
50.00	11726.0
51.00	3745.0
52.10	174.0
53.00	140.0
55.00	243.0
56.00	1114.0
57.00	1710.0
60.00	832.0
61.00	3269.0
62.00	2791.0
63.00	3034.0
64.00	483.0
65.00	560.0
66.00	176.0
66.80	181.0
68.00	6045.0
69.00	6069.0
70.00	604.0
72.00	343.0
73.00	2888.0
74.00	11427.0
75.00	31320.0
76.10	2824.0
77.00	467.0
77.80	308.0
79.00	2836.0
79.90	757.0
80.90	2676.0
81.90	712.0
87.00	2772.0
88.00	2758.0
90.90	302.0
92.00	2241.0
93.00	3036.0
94.10	7854.0
95.00	61528.0
96.00	4443.0
103.90	353.0
104.70	132.0
105.90	282.0
110.90	117.0
115.90	264.0
116.90	531.0
117.80	301.0
118.90	421.0
127.80	313.0
129.80	239.0
134.90	159.0
137.00	138.0
140.80	672.0
143.00	961.0
144.80	159.0
145.80	174.0
147.90	164.0
155.00	190.0
157.00	102.0
160.90	109.0
172.00	882.0
172.90	712.0
174.00	48792.0
175.00	3798.0
176.00	46160.0
177.00	2961.0
178.10	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	623.0
37.00	2849.0
38.00	2893.0
39.00	1200.0
39.90	415.0
43.00	110.0
43.90	644.0
45.00	554.0
46.00	205.0
47.00	746.0
48.10	278.0
49.00	2492.0
50.00	12070.0
51.00	3899.0
52.00	169.0
53.00	183.0
55.00	250.0
56.00	1008.0
57.00	1761.0
57.90	116.0
60.00	698.0
61.00	3437.0
62.00	2835.0
63.00	3097.0
64.00	632.0
64.90	658.0
66.00	154.0
66.80	146.0
68.00	6523.0
69.00	6505.0
70.00	638.0
72.00	381.0
73.00	2957.0
74.00	11701.0
75.10	33496.0
76.10	2923.0
76.90	463.0
77.80	365.0
79.00	2901.0
79.90	843.0
80.90	2775.0
81.90	734.0
87.00	2892.0
88.00	2683.0
91.00	334.0
92.00	2153.0
93.00	3104.0
94.00	8310.0
95.00	65424.0
96.00	4468.0
96.90	112.0
103.90	358.0
104.70	126.0
105.90	301.0
106.90	111.0
110.80	109.0
113.10	103.0
115.90	343.0
116.90	597.0
117.80	323.0
118.90	477.0
127.80	302.0
130.00	250.0
134.90	155.0
137.00	139.0
140.90	758.0
143.00	1116.0
145.00	200.0
145.80	209.0
147.90	172.0
155.00	228.0
156.90	120.0
158.90	108.0
160.90	141.0
170.50	103.0
172.00	916.0
172.90	722.0
174.00	52928.0
175.00	4110.0
176.00	50752.0
177.00	3233.0
178.10	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	555.0
37.00	2829.0
38.00	2680.0
39.00	1113.0
39.90	525.0
43.00	139.0
44.00	688.0
44.90	532.0
45.90	184.0
47.10	700.0
48.00	324.0
49.00	2243.0
50.00	11142.0
51.00	3570.0
52.10	160.0
53.00	173.0
55.00	231.0
56.00	908.0
57.00	1699.0
58.00	108.0
60.00	558.0
61.00	3135.0
62.00	2881.0
63.00	2725.0
64.00	665.0
65.00	645.0
66.10	109.0
66.90	128.0
68.00	6480.0
69.00	6216.0
70.00	557.0
72.00	369.0
73.00	2937.0
74.10	11282.0
75.10	32304.0
76.10	2786.0
76.90	402.0
77.80	377.0
78.90	2631.0
79.90	856.0
80.90	2614.0
81.90	659.0
82.90	116.0
87.00	2777.0
87.90	2467.0
90.90	334.0
92.00	2008.0
93.00	2854.0
94.00	7758.0
95.00	62304.0
96.10	4277.0
96.90	125.0
103.90	333.0
106.00	280.0
106.90	113.0
113.00	126.0
115.90	359.0
116.90	615.0
117.80	305.0
118.90	505.0
127.80	230.0
130.00	234.0
135.00	142.0
137.00	113.0
140.90	744.0
143.00	1131.0
145.00	236.0
145.70	225.0
147.90	146.0
155.00	219.0
156.90	117.0
160.80	147.0
172.00	820.0
172.90	653.0
174.00	51632.0
175.00	3827.0
176.00	50120.0
177.00	3265.0
178.20	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293