

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020873.D
 Acq On : 02 Apr 2021 13:20
 Operator : SY/MD
 Sample : VV0402WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Quant Time: Apr 03 00:37:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 03 00:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	671111	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	653911	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	325041	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	172474	36.20	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.40%		
7) Chloroethane-d5	1.571	69	145003	40.25	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.50%		
11) 1,1-Dichloroethene-d2	2.108	63	282171	31.39	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.78%		
21) 2-Butanone-d5	3.902	46	269695	87.01	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.01%		
24) Chloroform-d	4.352	84	464546	49.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.10%		
26) 1,2-Dichloroethane-d4	5.034	65	319663	51.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.48%		
32) Benzene-d6	5.053	84	873175	50.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.20%		
36) 1,2-Dichloropropane-d6	6.072	67	255995	47.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.68%		
41) Toluene-d8	7.317	98	839471	51.74	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.48%		
43) trans-1,3-Dichloroprop...	7.625	79	141984	49.87	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.74%		
47) 2-Hexanone-d5	8.091	63	194145	86.54	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.54%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	351070	45.04	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.08%		
64) 1,2-Dichlorobenzene-d4	11.632	152	359001	56.91	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	113.82%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.985	75	8852	1.21	ug/L	# 55
59) 1,2,3-Trichloropropane	11.255	75	29294	4.74	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020873.D
Acq On : 02 Apr 2021 13:20
Operator : SY/MD
Sample : VV0402WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Time: Apr 03 00:37:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 03 00:36:16 2021
Response via : Initial Calibration




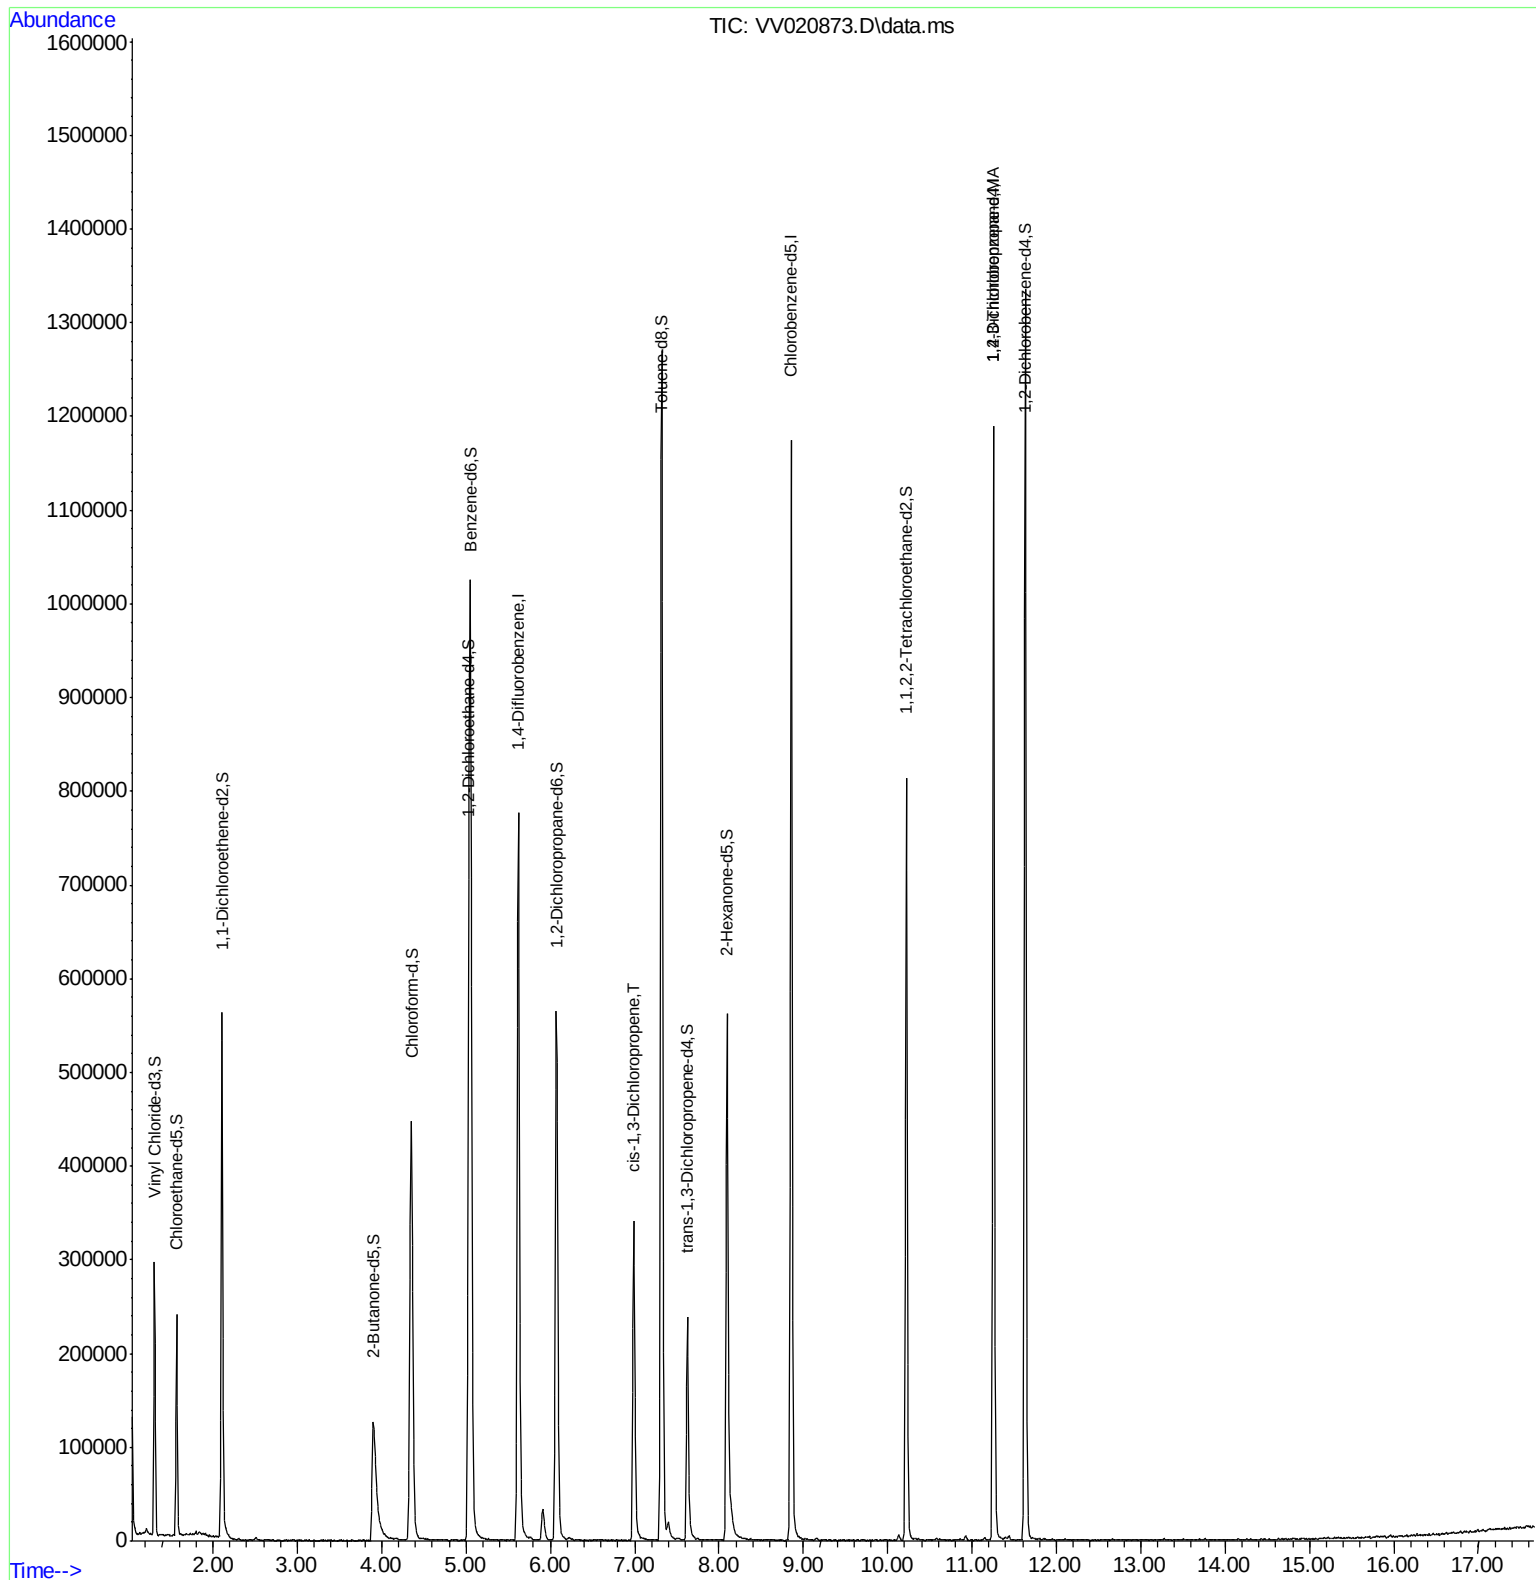


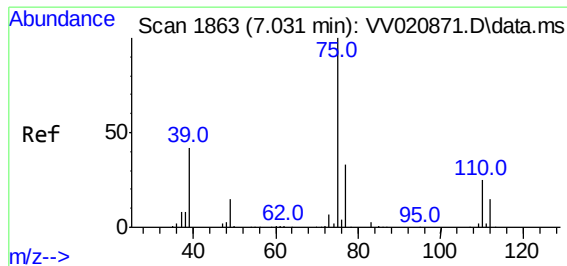

#39
cis-1,3-Dichloropropene
Concen: 1.21 ug/L
RT: 6.985 min Scan# 1849
Delta R.T. -0.045 min
Lab File: VV020873.D
Acq: 02 Apr 2021 13:20

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Tgt Ion: 75 Resp: 8852
Ion Ratio Lower Upper
75 100
77 56.0 21.7 40.3#

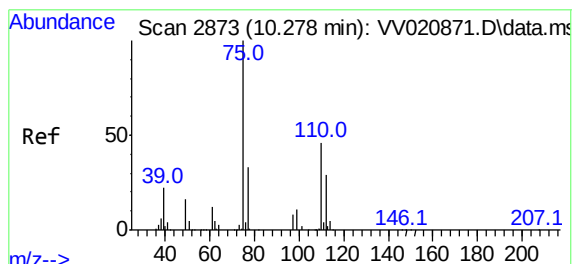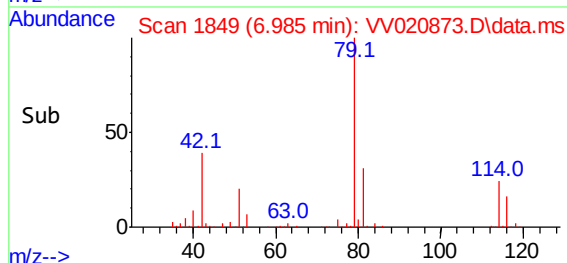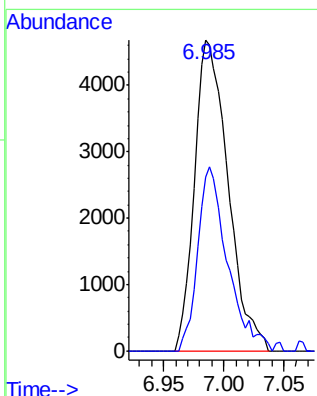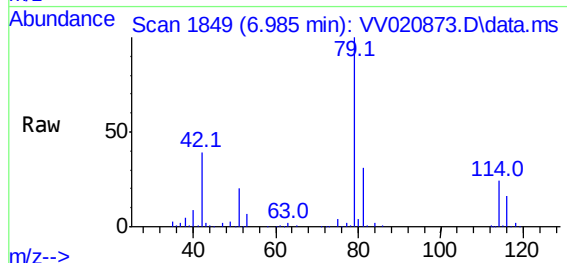

#59
1,2,3-Trichloropropane
Concen: 4.74 ug/L
RT: 11.255 min Scan# 3177
Delta R.T. 0.977 min
Lab File: VV020873.D
Acq: 02 Apr 2021 13:20

Tgt Ion: 75 Resp: 29294
Ion Ratio Lower Upper
75 100
77 33.9 25.3 37.9

