

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020875.D
 Acq On : 02 Apr 2021 14:16
 Operator : SY/MD
 Sample : M1880-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Apr 03 00:37:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 03 00:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	647084	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	620730	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	308544	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	162161	35.30	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.60%		
7) Chloroethane-d5	1.568	69	140872	40.56	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.12%		
11) 1,1-Dichloroethene-d2	2.108	63	268839	31.02	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.04%		
21) 2-Butanone-d5	3.899	46	286411	95.83	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.83%		
24) Chloroform-d	4.352	84	450110	49.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.58%		
26) 1,2-Dichloroethane-d4	5.034	65	316867	52.68	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.36%		
32) Benzene-d6	5.053	84	829445	50.13	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.26%		
36) 1,2-Dichloropropane-d6	6.072	67	255923	50.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.76%		
41) Toluene-d8	7.320	98	802357	52.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.20%		
43) trans-1,3-Dichloroprop...	7.625	79	136817	50.62	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	101.24%		
47) 2-Hexanone-d5	8.091	63	205085	96.30	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.30%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	352796	47.68	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.36%		
64) 1,2-Dichlorobenzene-d4	11.631	152	341850	57.09	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	114.18%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.152	43	10597	2.31	ug/L #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020875.D
Acq On : 02 Apr 2021 14:16
Operator : SY/MD
Sample : M1880-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Apr 03 00:37:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 03 00:36:16 2021
Response via : Initial Calibration

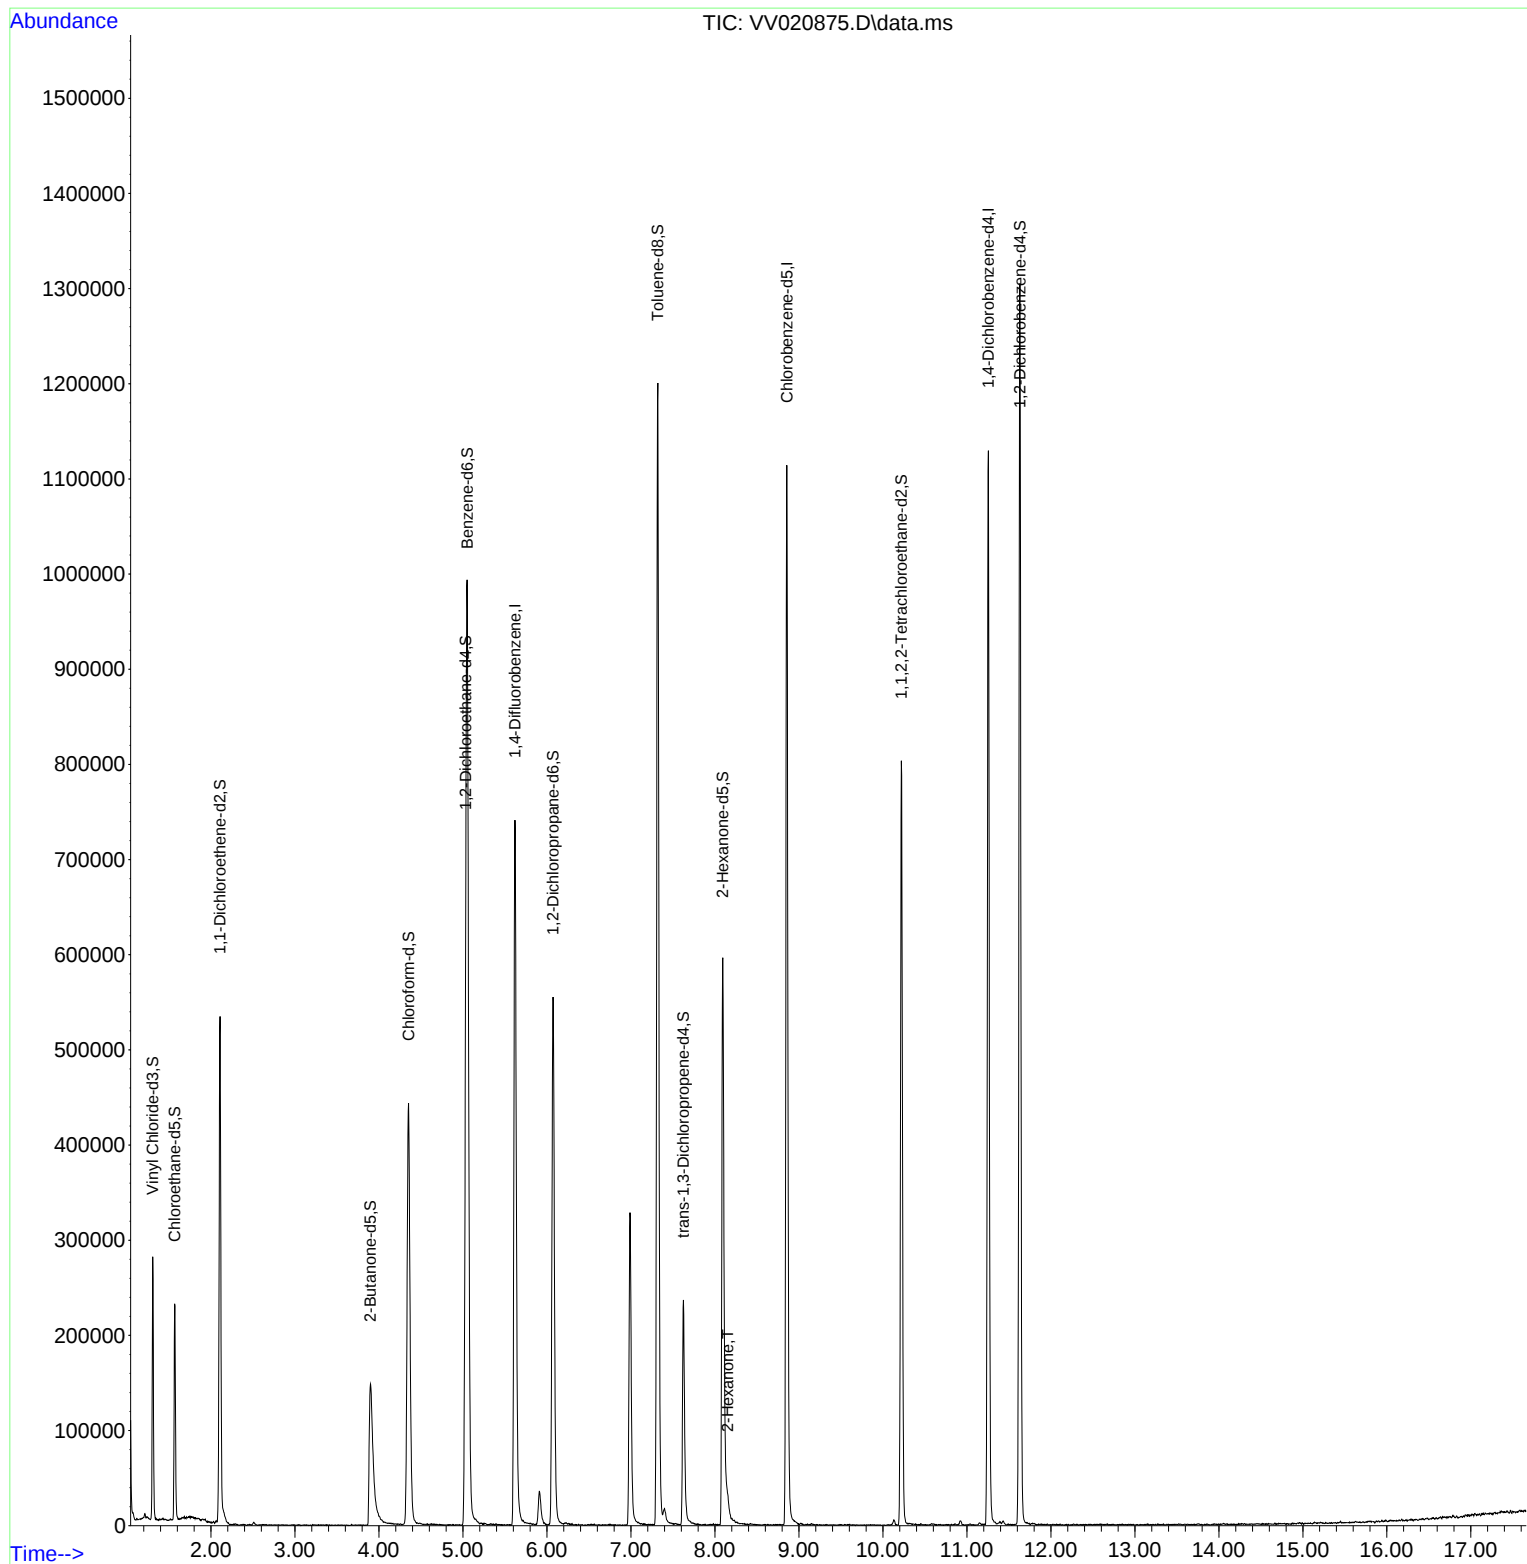

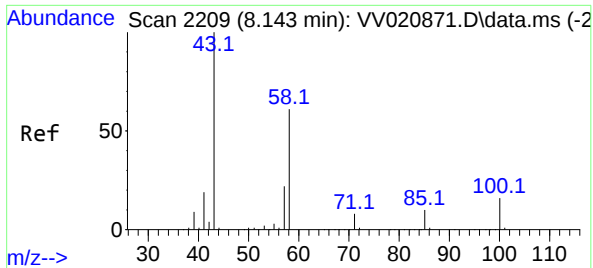

#48
2-Hexanone
Concen: 2.31 ug/L
RT: 8.152 min Scan# 2212
Delta R.T. 0.009 min
Lab File: VV020875.D
Acq: 02 Apr 2021 14:16

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tgt Ion: 43	Resp: 10597
Ion Ratio	Lower Upper
43 100	
58 34.5	45.8 68.8#
57 3.8	15.4 23.2#
100 4.2	10.2 15.4#

