

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020889.D
 Acq On : 02 Apr 2021 19:51
 Operator : SY/MD
 Sample : M1896-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J0

Quant Time: Apr 03 01:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 03 00:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	620636	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	594368	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	290556	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153576	34.85	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 69.70%			
7) Chloroethane-d5	1.571	69	132045	39.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 79.28%			
11) 1,1-Dichloroethene-d2	2.108	63	250842	30.17	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 60.34%			
21) 2-Butanone-d5	3.899	46	248897	86.83	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 86.83%			
24) Chloroform-d	4.352	84	430049	49.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.20%			
26) 1,2-Dichloroethane-d4	5.037	65	293868	50.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.88%			
32) Benzene-d6	5.053	84	794782	50.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.34%			
36) 1,2-Dichloropropane-d6	6.072	67	234185	48.15	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 96.30%			
41) Toluene-d8	7.320	98	754916	51.19	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.38%			
43) trans-1,3-Dichloroprop...	7.625	79	127514	49.27	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 98.54%			
47) 2-Hexanone-d5	8.095	63	174543	85.59	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 85.59%			
57) 1,1,2,2-Tetrachloroeth...	10.223	84	315353	44.51	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 89.02%			
64) 1,2-Dichlorobenzene-d4	11.631	152	325387	57.70	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 115.40%			
Target Compounds					Qvalue	
13) Acetone	2.198	43	15565	7.61	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020889.D
Acq On : 02 Apr 2021 19:51
Operator : SY/MD
Sample : M1896-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J0


Quant Time: Apr 03 01:59:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 03 00:36:16 2021
Response via : Initial Calibration

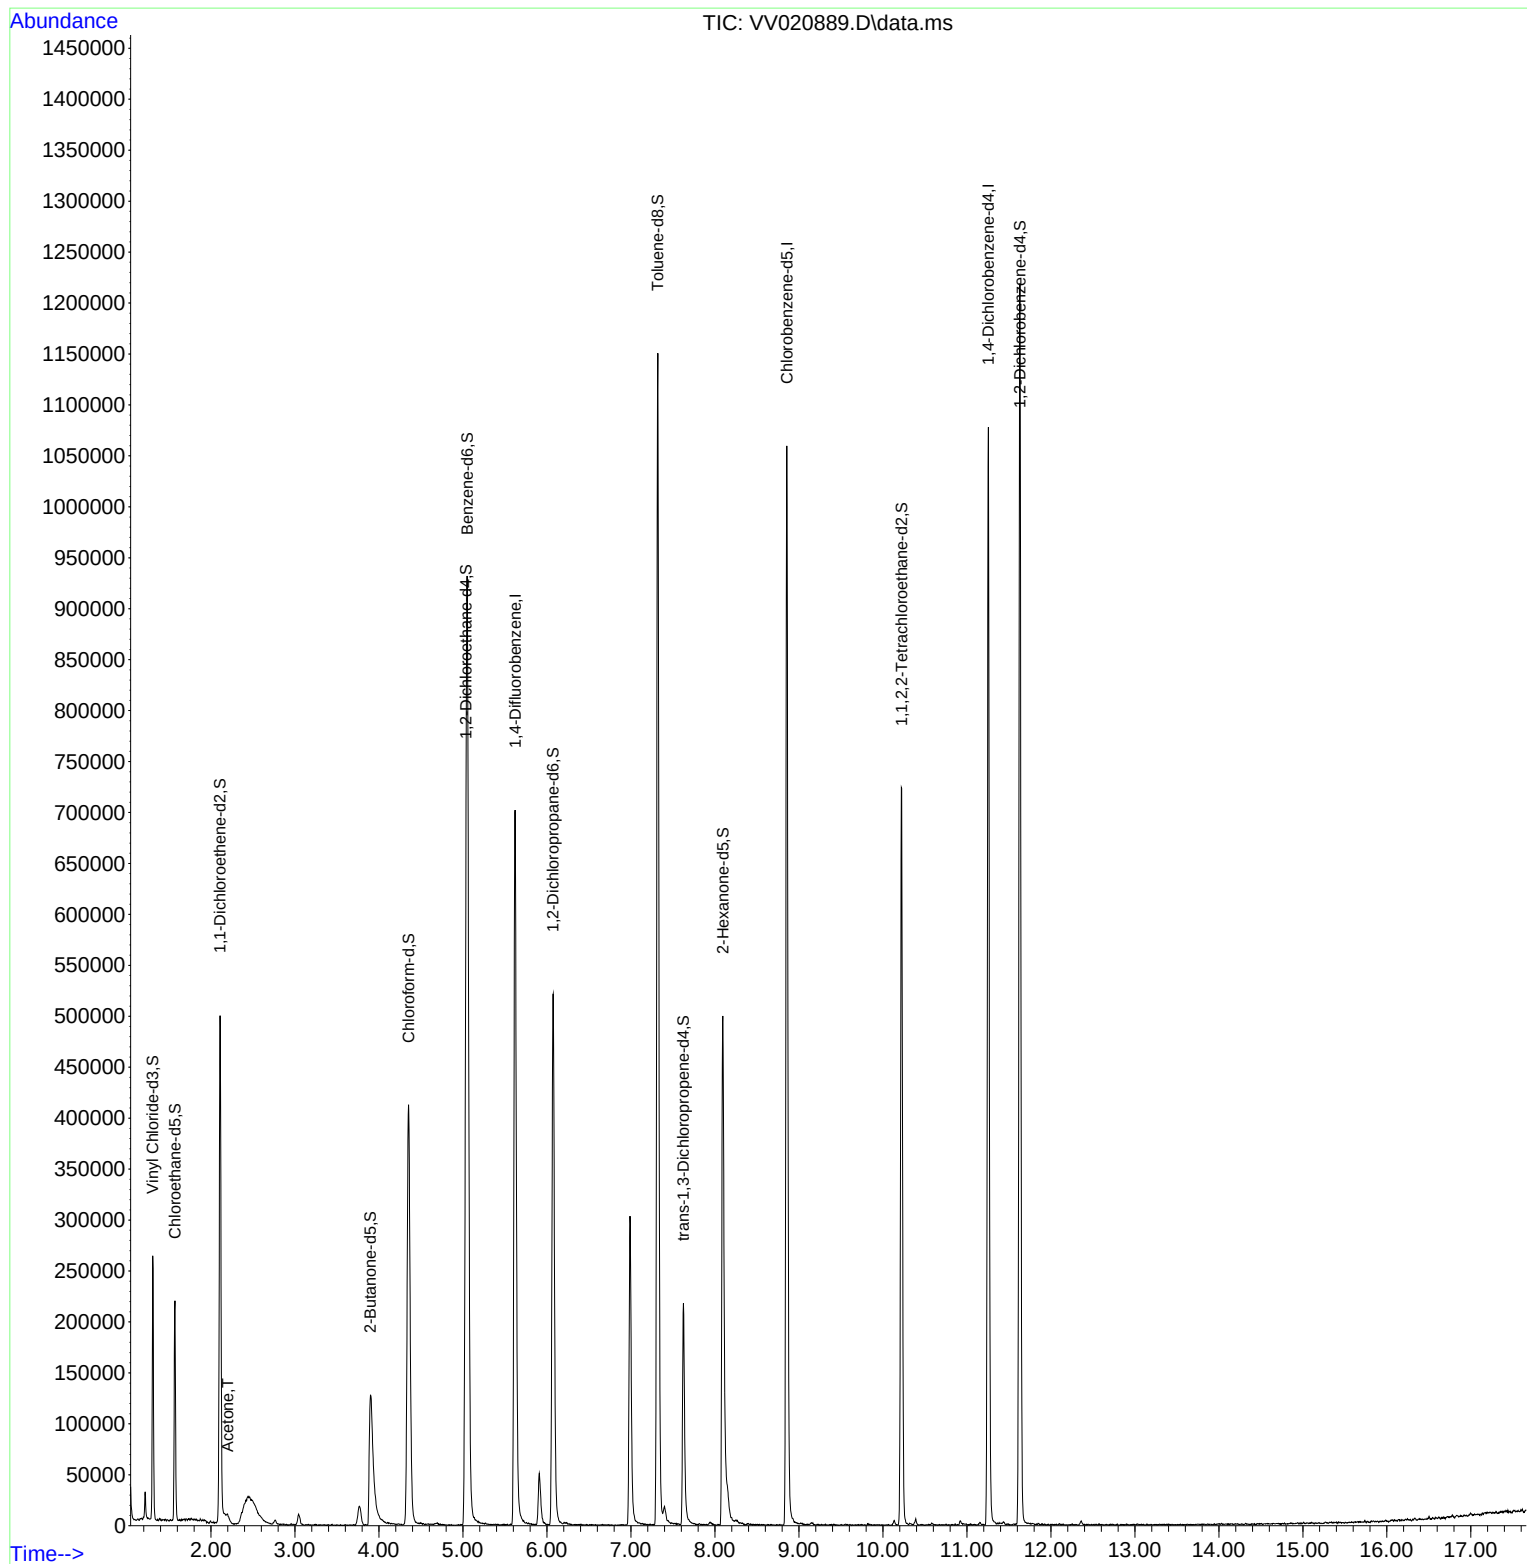

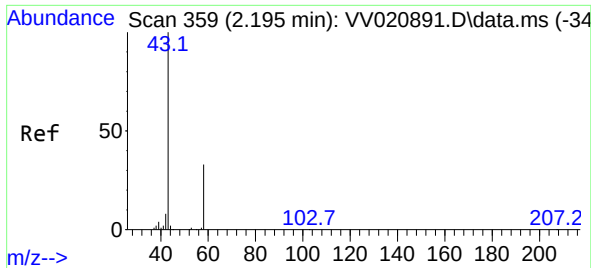

#13
Acetone
Concen: 7.61 ug/L
RT: 2.198 min Scan# 360
Delta R.T. 0.006 min
Lab File: VV020889.D
Acq: 02 Apr 2021 19:51

Instrument :
MSVOA_V
ClientSampleId :
BG3J0

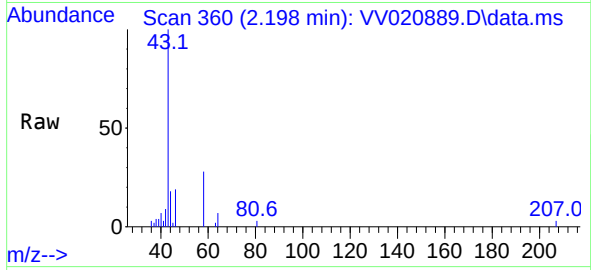

Tgt Ion: 43 Resp: 15565
Ion Ratio Lower Upper
43 100
58 16.1 0.0 60.8

