

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040221\
 Data File : VW020890.D
 Acq On : 02 Apr 2021 20:15
 Operator : SY/MD
 Sample : M1879-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B5

Quant Time: Apr 03 00:41:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 03 00:36:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	614374	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	593620	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.256	152	284849	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	150548	34.52	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.04%		
7) Chloroethane-d5	1.571	69	128137	38.86	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.72%		
11) 1,1-Dichloroethene-d2	2.108	63	249566	30.33	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.66%		
21) 2-Butanone-d5	3.899	46	230205	81.12	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.12%		
24) Chloroform-d	4.352	84	432216	49.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.70%		
26) 1,2-Dichloroethane-d4	5.034	65	291781	51.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.18%		
32) Benzene-d6	5.053	84	776157	49.05	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.10%		
36) 1,2-Dichloropropane-d6	6.072	67	232504	47.86	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.72%		
41) Toluene-d8	7.320	98	746350	50.67	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.34%		
43) trans-1,3-Dichloroprop...	7.625	79	122277	47.31	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.62%		
47) 2-Hexanone-d5	8.095	63	167062	82.03	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.03%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	313287	44.27	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.54%		
64) 1,2-Dichlorobenzene-d4	11.632	152	315648	57.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	114.20%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.150	43	12338	2.81	ug/L #	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020890.D
Acq On : 02 Apr 2021 20:15
Operator : SY/MD
Sample : M1879-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B5

Quant Time: Apr 03 00:41:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 03 00:36:16 2021
Response via : Initial Calibration

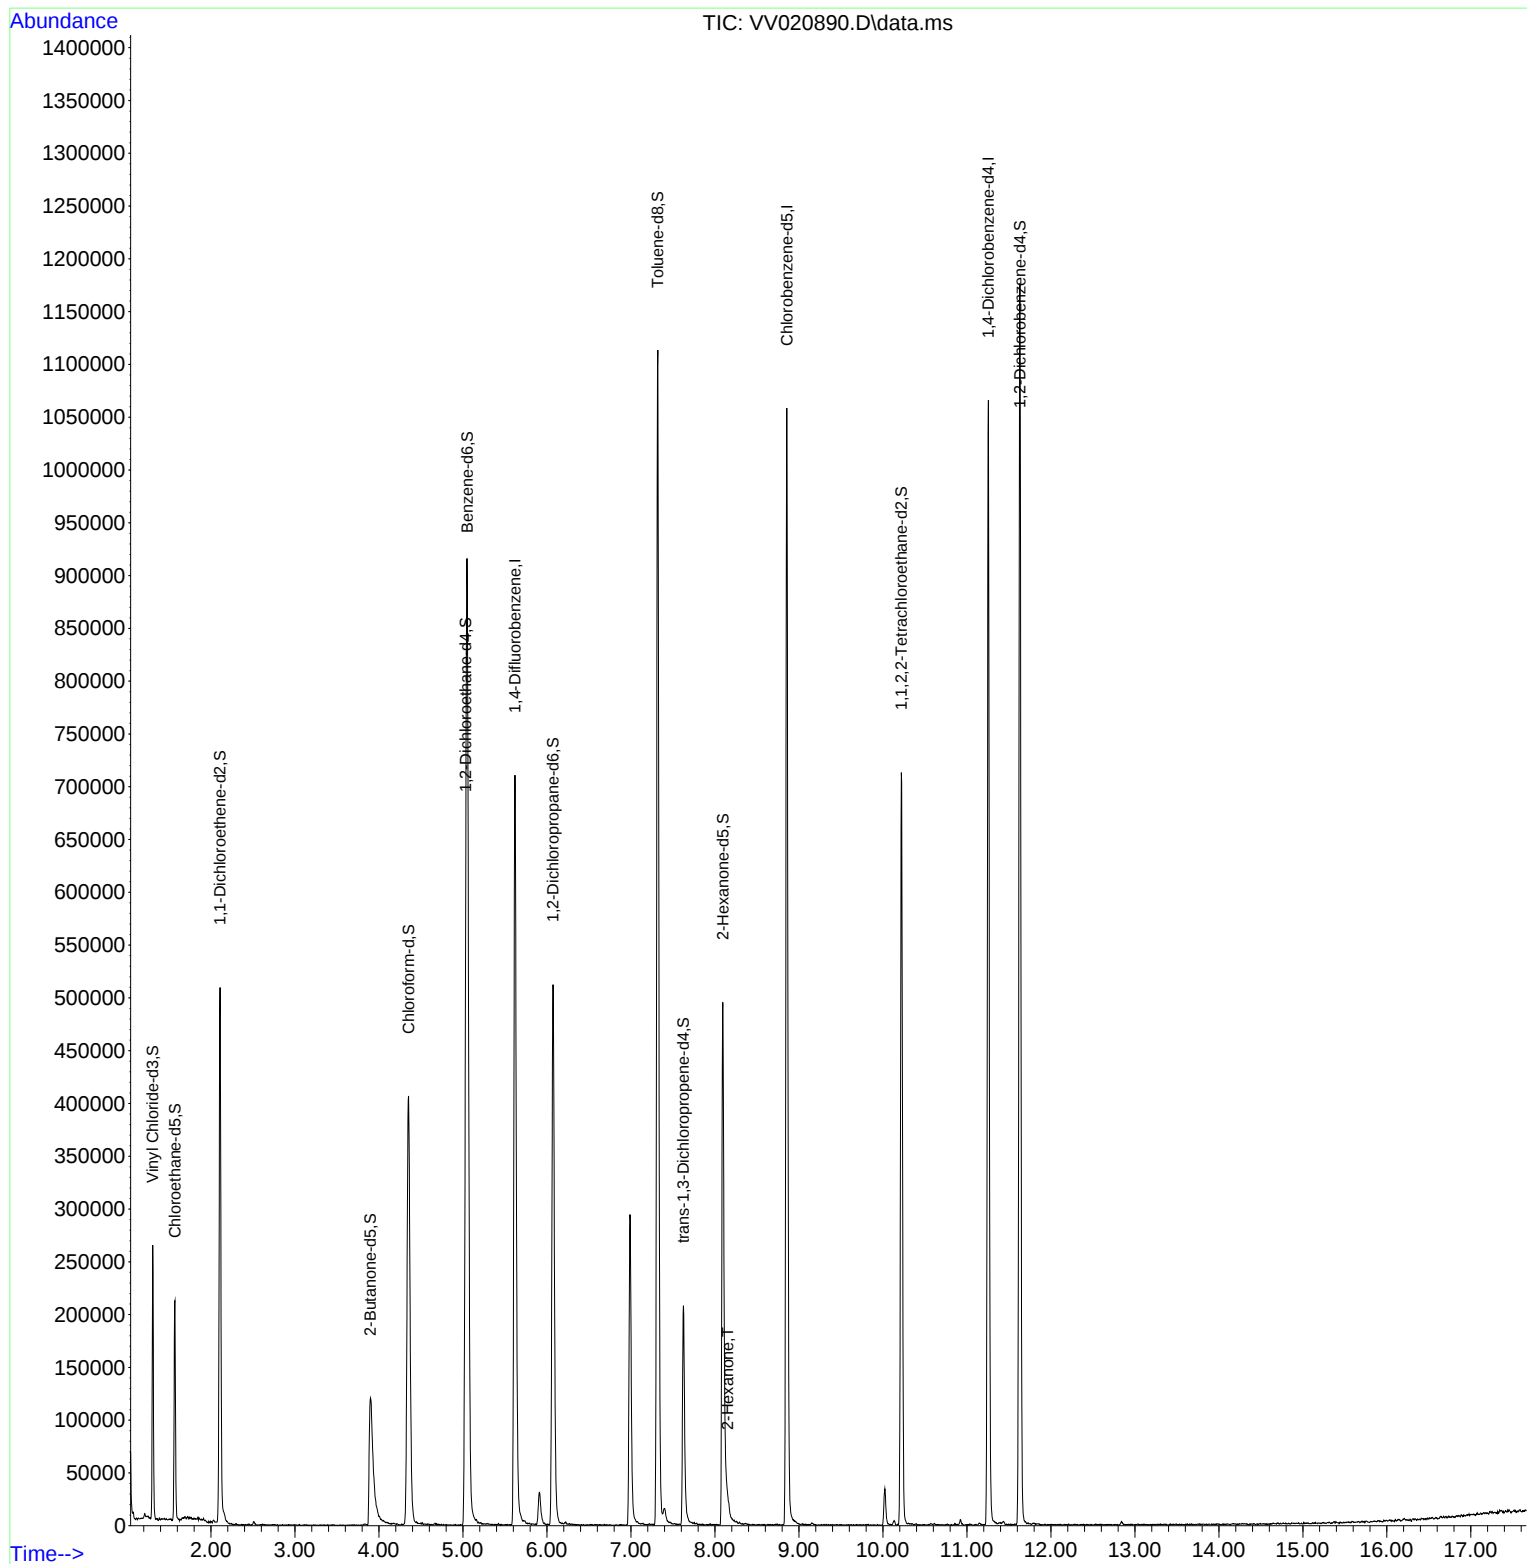

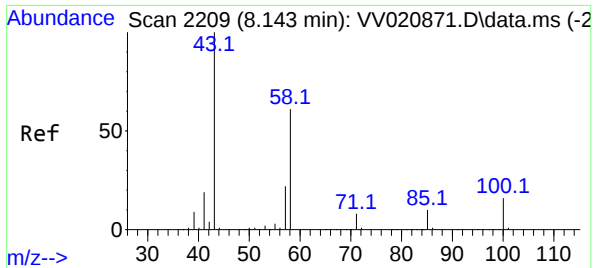

#48
2-Hexanone
Concen: 2.81 ug/L
RT: 8.150 min Scan# 2211
Delta R.T. 0.007 min
Lab File: VV020890.D
Acq: 02 Apr 2021 20:15

Instrument :
MSVOA_V
ClientSampleId :
EW1B5

Tgt Ion: 43 Resp: 12338

Ion	Ratio	Lower	Upper
43	100		
58	2.5	45.8	68.8#
57	0.0	15.4	23.2#
100	3.5	10.2	15.4#

