

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020873.D
 Acq On : 02 Apr 2021 13:20
 Operator : SY/MD
 Sample : VV0402WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	292835	291834	11.17%	1.473%
2	1.571	157	165	175	rBV	236280	266029	10.18%	1.342%
3	2.108	322	332	365	rVB	561463	826511	31.64%	4.171%
4	2.426	426	431	432	rBV2	490	411	0.02%	0.002%
5	2.510	450	457	466	rBV6	2968	4592	0.18%	0.023%
6	2.580	477	479	483	rVB2	559	301	0.01%	0.002%
7	2.606	483	487	488	rBV2	768	395	0.02%	0.002%
8	2.703	514	517	519	rVV2	768	459	0.02%	0.002%
9	2.761	529	535	537	rBV2	658	591	0.02%	0.003%
10	2.847	559	562	564	rVV	721	347	0.01%	0.002%
11	2.873	564	570	573	rVV2	538	529	0.02%	0.003%
12	2.995	606	608	611	rVV3	484	287	0.01%	0.001%
13	3.015	611	614	615	rVV2	748	457	0.02%	0.002%
14	3.053	624	626	633	rVB2	414	474	0.02%	0.002%
15	3.085	633	636	638	rBV2	516	309	0.01%	0.002%
16	3.137	648	652	654	rBV	507	341	0.01%	0.002%
17	3.285	693	698	700	rVV2	549	412	0.02%	0.002%
18	3.397	730	733	736	rBV3	493	337	0.01%	0.002%
19	3.436	742	745	752	rBV	781	775	0.03%	0.004%
20	3.519	767	771	773	rBV2	581	453	0.02%	0.002%
21	3.764	844	847	848	rBV	618	411	0.02%	0.002%
22	3.902	879	890	930	rBV2	126736	471046	18.03%	2.377%
23	4.352	1014	1030	1057	rBV	445584	1098596	42.06%	5.544%
24	4.825	1171	1177	1179	rBV3	1016	885	0.03%	0.004%
25	4.886	1194	1196	1202	rVB4	1009	967	0.04%	0.005%
26	4.944	1212	1214	1218	rBV3	793	490	0.02%	0.002%
27	4.963	1218	1220	1223	rBV2	643	367	0.01%	0.002%
28	4.979	1223	1225	1229	rVB3	761	338	0.01%	0.002%
29	5.050	1229	1247	1279	rBV2	1024866	2612277	100.00%	13.183%
30	5.378	1346	1349	1352	rVB3	929	512	0.02%	0.003%
31	5.400	1353	1356	1358	rBV2	918	582	0.02%	0.003%
32	5.468	1374	1377	1380	rBV2	500	266	0.01%	0.001%
33	5.494	1383	1385	1387	rVV3	868	508	0.02%	0.003%
34	5.519	1391	1393	1394	rBV2	585	280	0.01%	0.001%
35	5.619	1411	1424	1446	rBV	776223	1541899	59.03%	7.781%
36	5.908	1504	1514	1535	rBV3	32896	74319	2.84%	0.375%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020873.D
 Acq On : 02 Apr 2021 13:20
 Operator : SY/MD
 Sample : VV0402WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.072	1552	1565	1590	rBV	564031	1144493	43.81%	5.776%
38	6.297	1630	1635	1637	rBV3	900	803	0.03%	0.004%
39	6.394	1661	1665	1666	rBV3	877	576	0.02%	0.003%
40	6.436	1675	1678	1680	rVB2	597	341	0.01%	0.002%
41	6.487	1692	1694	1698	rVB2	782	558	0.02%	0.003%
42	6.506	1698	1700	1702	rBV	604	299	0.01%	0.002%
43	6.699	1758	1760	1763	rVB2	493	251	0.01%	0.001%
44	6.722	1763	1767	1770	rBV2	488	352	0.01%	0.002%
45	6.741	1770	1773	1774	rBV2	525	293	0.01%	0.001%
46	6.773	1780	1783	1785	rBV	428	266	0.01%	0.001%
47	6.863	1808	1811	1816	rBV2	535	576	0.02%	0.003%
48	6.937	1832	1834	1837	rBV2	445	258	0.01%	0.001%
49	6.989	1839	1850	1866	rBV	341047	609105	23.32%	3.074%
50	7.320	1940	1953	1971	rBV	1269215	2180409	83.47%	11.003%
51	7.625	2038	2048	2073	rBV2	238102	419753	16.07%	2.118%
52	7.924	2139	2141	2144	rBV2	850	432	0.02%	0.002%
53	8.046	2177	2179	2183	rVB2	749	380	0.01%	0.002%
54	8.095	2183	2194	2232	rBV	562714	1084201	41.50%	5.471%
55	8.374	2278	2281	2282	rBV3	1253	558	0.02%	0.003%
56	8.506	2317	2322	2326	rVB5	612	574	0.02%	0.003%
57	8.706	2381	2384	2387	rVB2	857	488	0.02%	0.002%
58	8.857	2418	2431	2456	rBV	1173347	1893801	72.50%	9.557%
59	9.204	2536	2539	2540	rBV2	739	317	0.01%	0.002%
60	9.304	2567	2570	2572	rVB	1004	489	0.02%	0.002%
61	9.378	2591	2593	2598	rBV3	793	522	0.02%	0.003%
62	9.432	2608	2610	2613	rBV3	764	422	0.02%	0.002%
63	9.448	2613	2615	2617	rBV2	512	291	0.01%	0.001%
64	9.548	2643	2646	2647	rBV	932	471	0.02%	0.002%
65	9.574	2652	2654	2657	rVV3	509	267	0.01%	0.001%
66	9.593	2657	2660	2663	rVV3	830	553	0.02%	0.003%
67	9.609	2663	2665	2669	rVB	849	385	0.01%	0.002%
68	9.686	2685	2689	2693	rBV3	683	832	0.03%	0.004%
69	9.709	2694	2696	2703	rVB4	1017	923	0.04%	0.005%
70	9.786	2714	2720	2723	rVV4	650	646	0.02%	0.003%
71	9.815	2726	2729	2731	rBV2	886	448	0.02%	0.002%
72	9.902	2754	2756	2758	rBV	697	297	0.01%	0.001%
73	10.066	2804	2807	2809	rBV2	753	472	0.02%	0.002%
74	10.091	2812	2815	2817	rBV2	520	290	0.01%	0.001%
75	10.130	2820	2827	2837	rVB5	5898	9409	0.36%	0.047%
76	10.220	2841	2855	2874	rBV	813768	1270825	48.65%	6.413%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020873.D
 Acq On : 02 Apr 2021 13:20
 Operator : SY/MD
 Sample : VV0402WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.535	2949	2953	2955	rBV3	958	867	0.03%	0.004%
78	10.738	3012	3016	3017	rBV2	482	376	0.01%	0.002%
79	10.767	3022	3025	3029	rBV3	460	451	0.02%	0.002%
80	10.824	3040	3043	3045	rBV	958	588	0.02%	0.003%
81	10.924	3067	3074	3082	rVB8	5137	8028	0.31%	0.041%
82	11.033	3101	3108	3112	rBV5	1309	1870	0.07%	0.009%
83	11.255	3165	3177	3198	rBV	1188669	1842599	70.54%	9.298%
84	11.535	3258	3264	3266	rBV4	830	894	0.03%	0.005%
85	11.628	3281	3293	3316	rBV	1335147	2124078	81.31%	10.719%
86	11.786	3339	3342	3343	rBV3	1491	765	0.03%	0.004%
87	11.853	3357	3363	3365	rBV6	2415	2228	0.09%	0.011%
88	11.921	3382	3384	3387	rVB3	638	293	0.01%	0.001%
89	11.947	3390	3392	3397	rVB3	1179	736	0.03%	0.004%
90	11.995	3405	3407	3413	rBV5	1134	1007	0.04%	0.005%
91	12.021	3413	3415	3417	rBV	625	267	0.01%	0.001%
92	12.062	3426	3428	3431	rBV2	887	614	0.02%	0.003%
93	12.429	3538	3542	3545	rBV2	778	605	0.02%	0.003%
94	12.487	3557	3560	3561	rBV	759	380	0.01%	0.002%
95	12.648	3606	3610	3611	rBV	864	721	0.03%	0.004%
96	12.898	3686	3688	3690	rBV3	767	434	0.02%	0.002%
97	13.114	3752	3755	3758	rBV4	736	381	0.01%	0.002%
98	13.175	3772	3774	3778	rVB	979	542	0.02%	0.003%
99	13.381	3835	3838	3841	rBV	676	563	0.02%	0.003%
100	14.149	4074	4077	4079	rBV2	1156	698	0.03%	0.004%




Sum of corrected areas: 19816198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020873.D
Acq On : 02 Apr 2021 13:20
Operator : SY/MD
Sample : VV0402WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

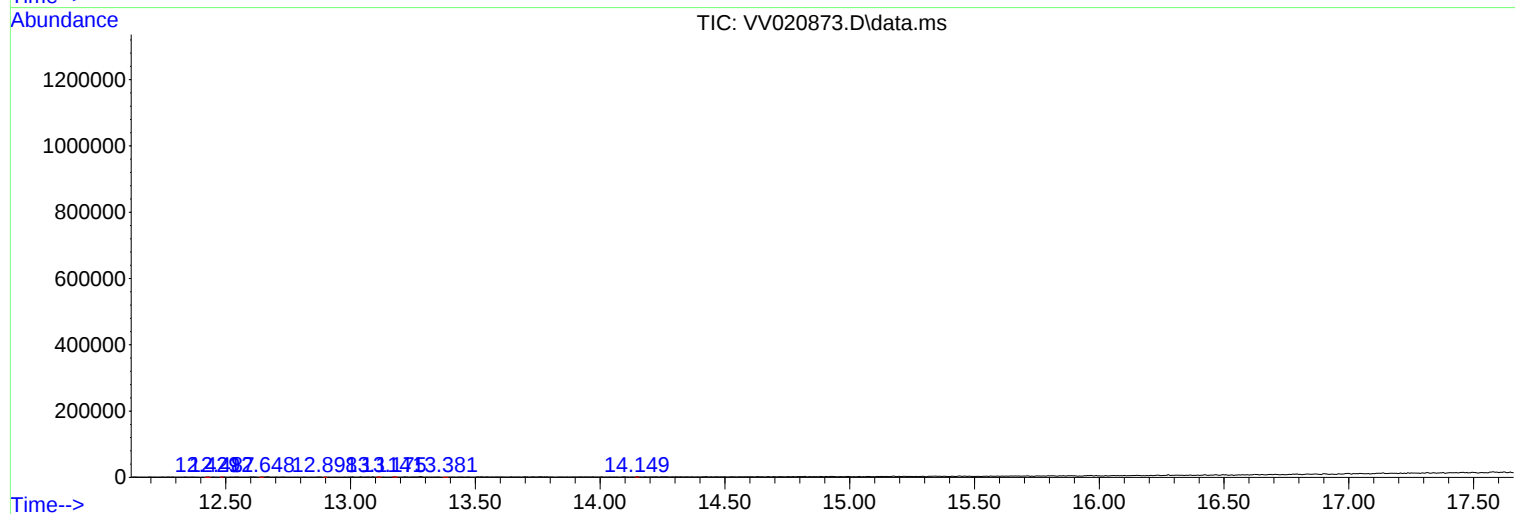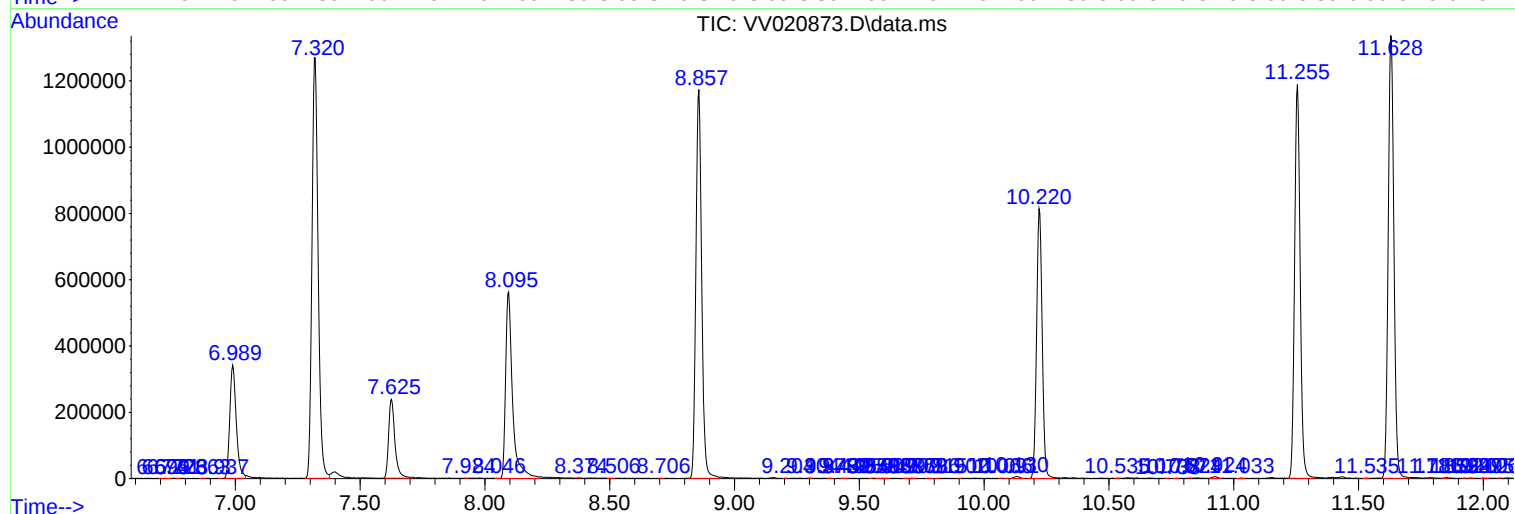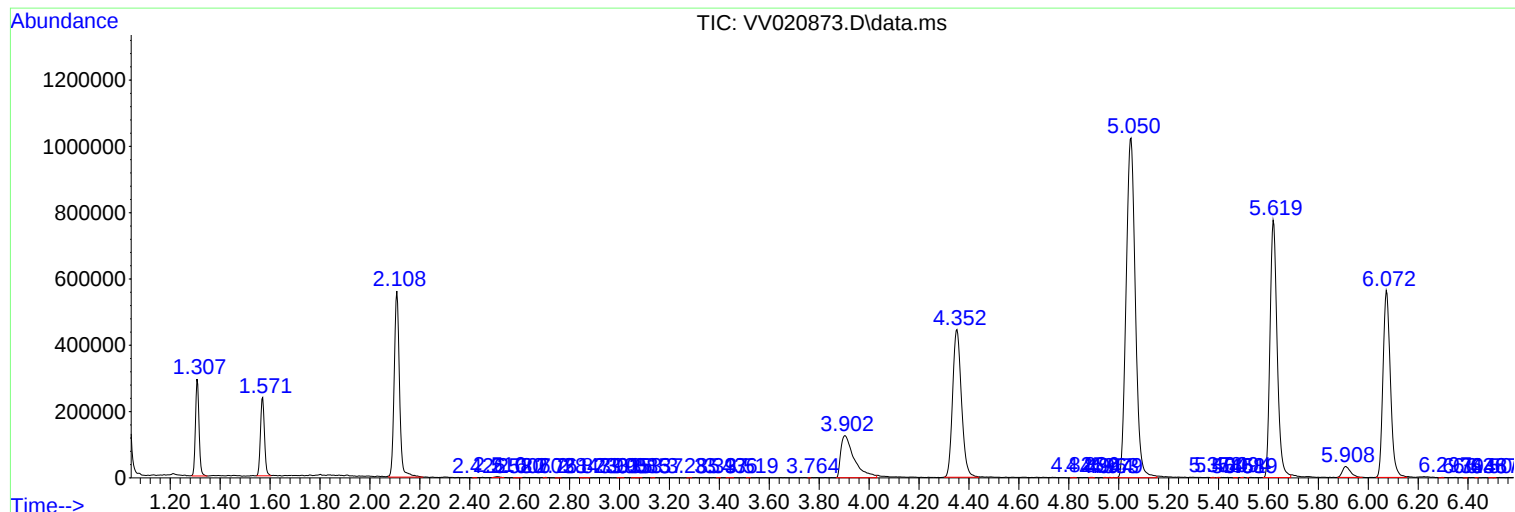

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020873.D
Acq On : 02 Apr 2021 13:20
Operator : SY/MD
Sample : VV0402WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020873.D
Acq On : 02 Apr 2021 13:20
Operator : SY/MD
Sample : VV0402WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------