

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020882.D
 Acq On : 02 Apr 2021 17:04
 Operator : SY/MD
 Sample : M1845-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	103	rVB2	909081	950101	39.80%	4.527%
2	1.571	157	165	176	rBV	215718	245887	10.30%	1.172%
3	2.108	322	332	353	rBV	502768	753938	31.58%	3.593%
4	2.339	401	404	407	rVB3	963	566	0.02%	0.003%
5	2.375	413	415	416	rBV	681	299	0.01%	0.001%
6	2.416	424	428	429	rBV3	961	535	0.02%	0.003%
7	2.497	450	453	454	rBV2	1879	1008	0.04%	0.005%
8	2.548	466	469	471	rBV	507	313	0.01%	0.001%
9	2.590	477	482	484	rBV	641	580	0.02%	0.003%
10	2.728	523	525	527	rBV3	878	416	0.02%	0.002%
11	2.767	530	537	550	rVB3	6043	11142	0.47%	0.053%
12	2.873	566	570	571	rBV3	577	392	0.02%	0.002%
13	2.892	574	576	580	rVV2	411	330	0.01%	0.002%
14	2.944	588	592	594	rBV2	429	300	0.01%	0.001%
15	3.063	626	629	630	rBV2	431	264	0.01%	0.001%
16	3.114	642	645	647	rBV2	561	261	0.01%	0.001%
17	3.127	647	649	652	rVB3	734	329	0.01%	0.002%
18	3.150	654	656	660	rBV3	467	326	0.01%	0.002%
19	3.195	660	670	681	rVV3	7886	16154	0.68%	0.077%
20	3.249	685	687	690	rVB2	681	391	0.02%	0.002%
21	3.275	690	695	698	rBV3	526	455	0.02%	0.002%
22	3.400	731	734	736	rBV3	563	380	0.02%	0.002%
23	3.432	741	744	746	rBV2	759	333	0.01%	0.002%
24	3.497	761	764	766	rVB3	856	473	0.02%	0.002%
25	3.510	766	768	771	rBV2	552	354	0.01%	0.002%
26	3.577	787	789	794	rBV3	427	398	0.02%	0.002%
27	3.600	794	796	799	rVB	723	312	0.01%	0.001%
28	3.677	817	820	825	rVB2	621	445	0.02%	0.002%
29	3.786	850	854	857	rBV3	527	393	0.02%	0.002%
30	3.912	875	893	923	rBV2	836684	2261430	94.73%	10.776%
31	4.352	1014	1030	1060	rBV	413077	1010584	42.33%	4.816%
32	4.577	1098	1100	1104	rBV	689	519	0.02%	0.002%
33	4.863	1186	1189	1192	rBV3	798	488	0.02%	0.002%
34	4.883	1192	1195	1198	rBV3	797	629	0.03%	0.003%
35	4.940	1209	1213	1216	rVB2	666	519	0.02%	0.002%
36	4.973	1219	1223	1226	rBV3	439	413	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020882.D
 Acq On : 02 Apr 2021 17:04
 Operator : SY/MD
 Sample : M1845-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.050	1229	1247	1278	rBV2	930667	2387148	100.00%	11.375%
38	5.323	1328	1332	1334	rBV3	1214	810	0.03%	0.004%
39	5.548	1399	1402	1405	rVB4	608	414	0.02%	0.002%
40	5.619	1412	1424	1447	rBV	715484	1444754	60.52%	6.884%
41	5.918	1502	1517	1544	rBV4	195551	412429	17.28%	1.965%
42	6.072	1552	1565	1589	rBV	515482	1049811	43.98%	5.002%
43	6.275	1626	1628	1635	rVB6	1191	807	0.03%	0.004%
44	6.391	1662	1664	1666	rBV	499	252	0.01%	0.001%
45	6.436	1675	1678	1681	rVB2	635	383	0.02%	0.002%
46	6.461	1684	1686	1689	rBV2	407	266	0.01%	0.001%
47	6.510	1696	1701	1703	rBV5	702	688	0.03%	0.003%
48	6.625	1735	1737	1739	rBV	534	264	0.01%	0.001%
49	6.654	1744	1746	1747	rBV	643	284	0.01%	0.001%
50	6.725	1766	1768	1772	rBV2	667	300	0.01%	0.001%
51	6.757	1776	1778	1779	rBV2	609	252	0.01%	0.001%
52	6.879	1814	1816	1819	rVB3	1028	551	0.02%	0.003%
53	6.895	1819	1821	1823	rBV2	561	353	0.01%	0.002%
54	6.989	1838	1850	1878	rBV	301388	557637	23.36%	2.657%
55	7.320	1940	1953	1971	rBV	1149446	1948942	81.64%	9.287%
56	7.625	2036	2048	2069	rBV2	215995	378083	15.84%	1.802%
57	7.812	2104	2106	2111	rVB3	1263	891	0.04%	0.004%
58	7.882	2126	2128	2130	rVB2	691	275	0.01%	0.001%
59	7.902	2130	2134	2136	rBV3	945	643	0.03%	0.003%
60	8.030	2171	2174	2177	rBV4	887	568	0.02%	0.003%
61	8.091	2183	2193	2237	rBV	502652	973720	40.79%	4.640%
62	8.554	2334	2337	2338	rBV2	746	321	0.01%	0.002%
63	8.751	2396	2398	2401	rBV2	952	425	0.02%	0.002%
64	8.857	2419	2431	2456	rBV	1098793	1769810	74.14%	8.433%
65	9.133	2515	2517	2519	rBV2	702	445	0.02%	0.002%
66	9.262	2554	2557	2559	rBV2	674	479	0.02%	0.002%
67	9.403	2599	2601	2605	rBV4	708	478	0.02%	0.002%
68	9.490	2624	2628	2630	rBV4	826	548	0.02%	0.003%
69	9.516	2634	2636	2640	rVB2	415	245	0.01%	0.001%
70	9.542	2640	2644	2648	rBV3	600	728	0.03%	0.003%
71	9.628	2669	2671	2676	rVB	602	323	0.01%	0.002%
72	9.834	2733	2735	2737	rBV	613	283	0.01%	0.001%
73	9.937	2763	2767	2771	rBV3	591	493	0.02%	0.002%
74	10.133	2819	2828	2839	rVB8	4968	8465	0.35%	0.040%
75	10.220	2843	2855	2873	rBV	746990	1165293	48.82%	5.553%
76	10.451	2923	2927	2928	rBV2	750	583	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020882.D
 Acq On : 02 Apr 2021 17:04
 Operator : SY/MD
 Sample : M1845-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.529	2947	2951	2953	rBV3	691	415	0.02%	0.002%
78	10.738	3013	3016	3018	rBV	1270	725	0.03%	0.003%
79	10.844	3044	3049	3051	rBV3	1381	1132	0.05%	0.005%
80	10.924	3066	3074	3082	rVB8	4691	7721	0.32%	0.037%
81	11.111	3126	3132	3134	rBV3	679	590	0.02%	0.003%
82	11.130	3136	3138	3140	rVV2	661	308	0.01%	0.001%
83	11.156	3140	3146	3153	rVB5	2494	3563	0.15%	0.017%
84	11.255	3164	3177	3195	rBV	1102825	1689992	70.80%	8.053%
85	11.541	3259	3266	3280	rBV7	8458	18076	0.76%	0.086%
86	11.631	3282	3294	3311	rVV	1197008	1882799	78.87%	8.972%
87	12.136	3448	3451	3455	rBV3	778	494	0.02%	0.002%
88	12.258	3486	3489	3494	rBV4	999	850	0.04%	0.004%
89	12.445	3543	3547	3551	rVB3	805	779	0.03%	0.004%
90	12.467	3551	3554	3557	rBV4	657	647	0.03%	0.003%
91	12.532	3570	3574	3579	rBV5	1046	1188	0.05%	0.006%
92	12.567	3582	3585	3589	rVV4	940	721	0.03%	0.003%
93	12.754	3641	3643	3646	rBV2	577	356	0.01%	0.002%
94	12.918	3691	3694	3699	rBV3	1590	1342	0.06%	0.006%
95	13.056	3733	3737	3740	rBV2	817	678	0.03%	0.003%
96	13.091	3744	3748	3751	rBV5	808	775	0.03%	0.004%
97	13.445	3856	3858	3860	rBV2	707	349	0.01%	0.002%
98	13.696	3934	3936	3938	rBV3	707	325	0.01%	0.002%
99	13.766	3956	3958	3960	rVB	1173	435	0.02%	0.002%
100	13.934	4008	4010	4014	rBV4	844	576	0.02%	0.003%




Sum of corrected areas: 20985937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020882.D
Acq On : 02 Apr 2021 17:04
Operator : SY/MD
Sample : M1845-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

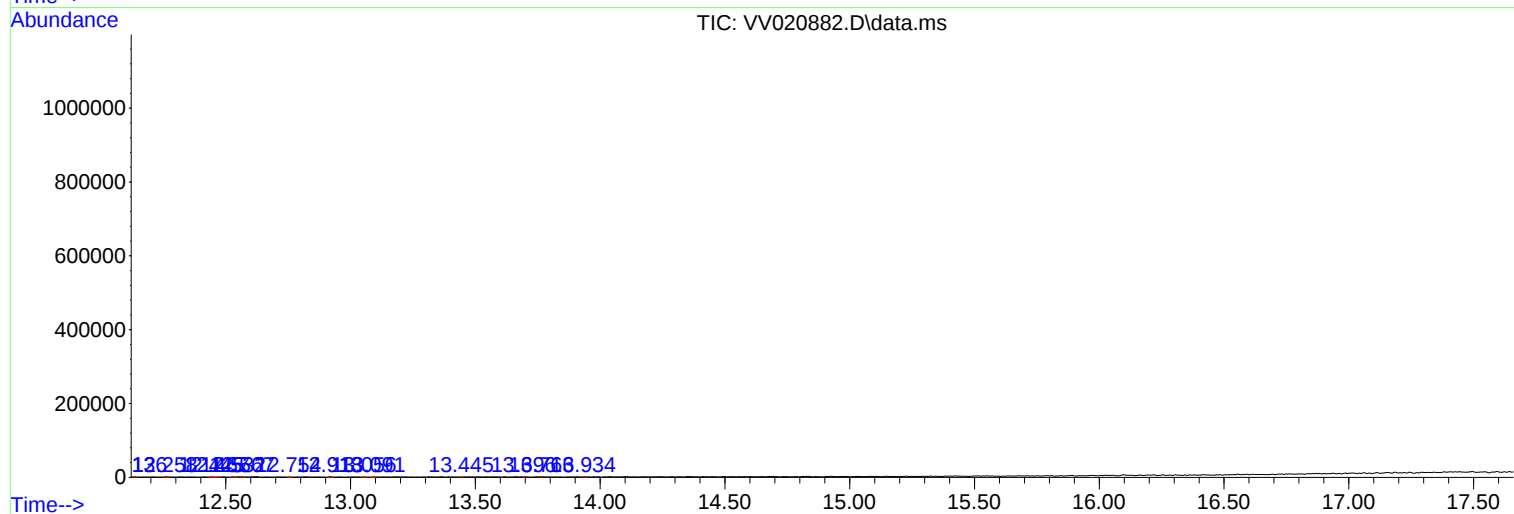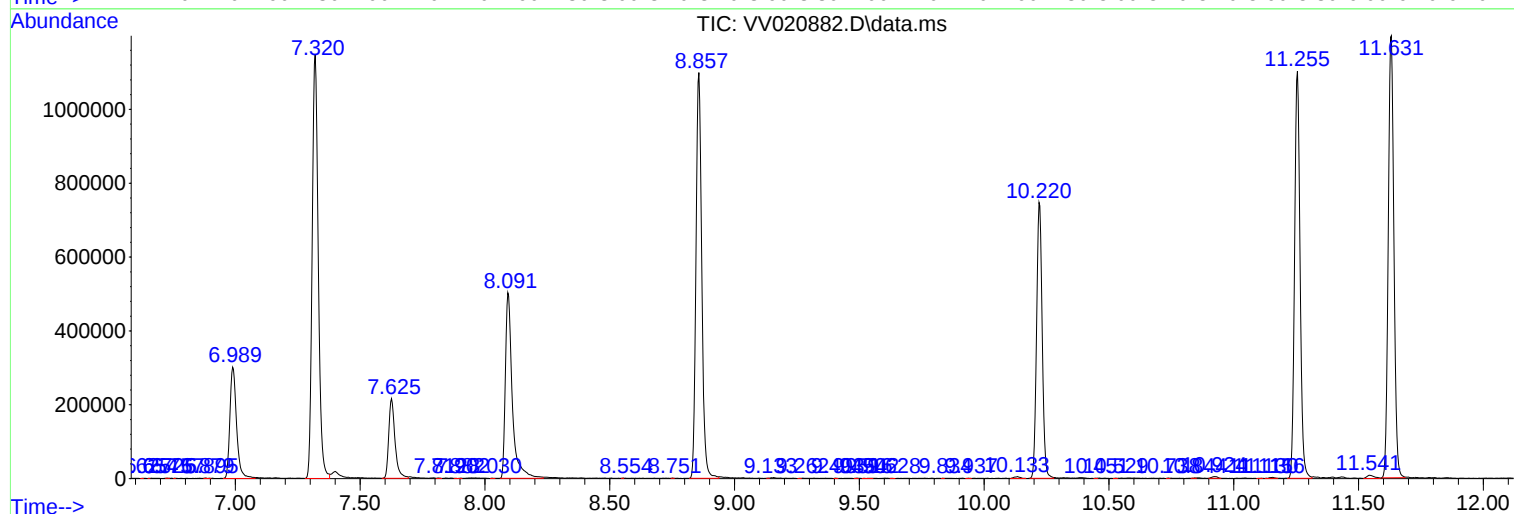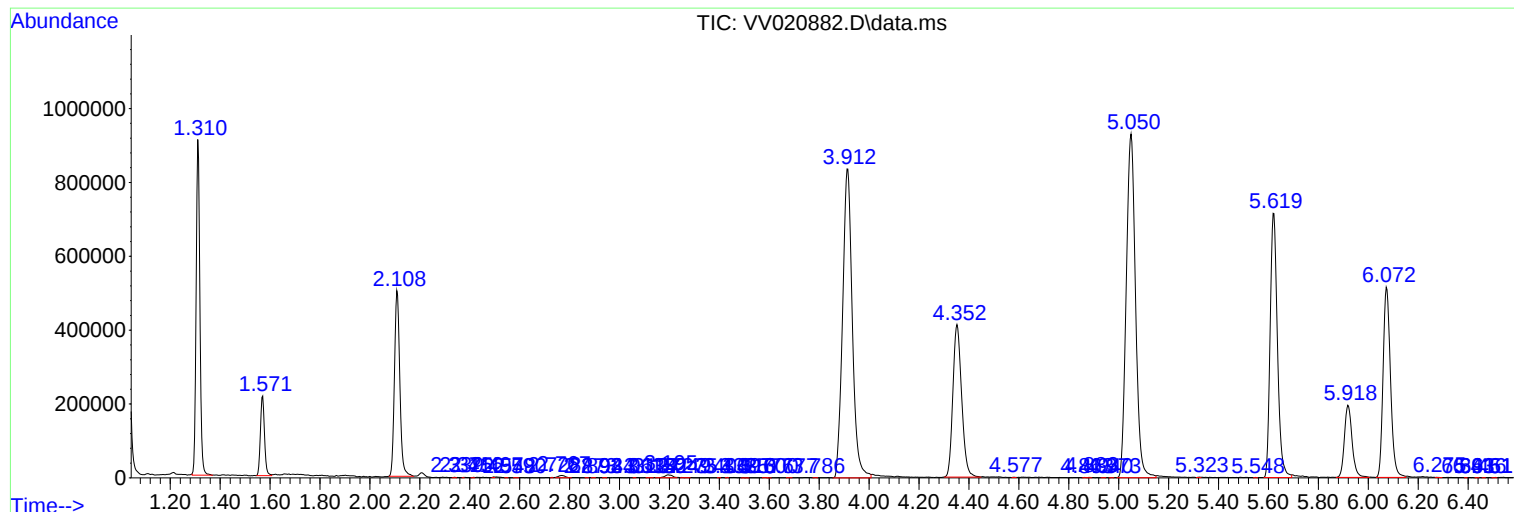

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020882.D
Acq On : 02 Apr 2021 17:04
Operator : SY/MD
Sample : M1845-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020882.D
Acq On : 02 Apr 2021 17:04
Operator : SY/MD
Sample : M1845-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
