

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040221\
 Data File : VV020890.D
 Acq On : 02 Apr 2021 20:15
 Operator : SY/MD
 Sample : M1879-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	259994	253990	10.80%	1.430%
2	1.571	157	165	174	rBV	207473	237068	10.08%	1.334%
3	2.108	322	332	356	rVB	505791	731573	31.10%	4.118%
4	2.359	405	410	411	rBV2	523	345	0.01%	0.002%
5	2.410	424	426	430	rBV3	522	420	0.02%	0.002%
6	2.510	449	457	462	rBV6	3549	4842	0.21%	0.027%
7	2.558	468	472	475	rBV	522	478	0.02%	0.003%
8	2.613	487	489	497	rVB4	765	657	0.03%	0.004%
9	2.790	542	544	549	rVB3	887	630	0.03%	0.004%
10	2.819	549	553	555	rBV2	561	442	0.02%	0.002%
11	2.921	583	585	586	rBV	403	188	0.01%	0.001%
12	2.944	590	592	594	rBV2	401	212	0.01%	0.001%
13	2.999	604	609	612	rBV3	606	599	0.03%	0.003%
14	3.053	621	626	631	rVB3	817	783	0.03%	0.004%
15	3.098	639	640	642	rBV	425	213	0.01%	0.001%
16	3.140	650	653	656	rBV2	545	372	0.02%	0.002%
17	3.169	659	662	664	rBV2	436	306	0.01%	0.002%
18	3.217	675	677	679	rBV	382	187	0.01%	0.001%
19	3.272	691	694	697	rVB2	464	263	0.01%	0.001%
20	3.294	697	701	703	rBV	550	450	0.02%	0.003%
21	3.368	722	724	727	rVB2	382	209	0.01%	0.001%
22	3.388	729	730	732	rBV	433	168	0.01%	0.001%
23	3.436	743	745	747	rBV	332	174	0.01%	0.001%
24	3.613	796	800	802	rBV	533	471	0.02%	0.003%
25	3.664	812	816	817	rBV	348	296	0.01%	0.002%
26	3.735	835	838	840	rBV2	427	250	0.01%	0.001%
27	3.796	855	857	861	rBV	440	254	0.01%	0.001%
28	3.825	863	866	868	rBV4	1035	679	0.03%	0.004%
29	3.899	878	889	920	rBV	120613	407433	17.32%	2.293%
30	4.156	966	969	971	rBV2	875	574	0.02%	0.003%
31	4.275	1001	1006	1010	rBV2	1038	1033	0.04%	0.006%
32	4.352	1014	1030	1058	rVV2	405610	1007968	42.85%	5.674%
33	4.905	1200	1202	1206	rVB3	781	457	0.02%	0.003%
34	4.973	1221	1223	1225	rBV2	477	218	0.01%	0.001%
35	5.050	1229	1247	1278	rBV2	915269	2352489	100.00%	13.242%
36	5.346	1337	1339	1344	rVB4	785	521	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040221\
 Data File : VW020890.D
 Acq On : 02 Apr 2021 20:15
 Operator : SY/MD
 Sample : M1879-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.462	1373	1375	1378	rVB3	782	426	0.02%	0.002%
38	5.619	1410	1424	1456	rBV	710500	1420232	60.37%	7.994%
39	5.912	1504	1515	1533	rBV2	30827	67421	2.87%	0.380%
40	6.072	1552	1565	1591	rBV	511373	1035962	44.04%	5.831%
41	6.352	1649	1652	1653	rBV2	539	290	0.01%	0.002%
42	6.410	1668	1670	1674	rVB	704	436	0.02%	0.002%
43	6.436	1674	1678	1682	rVB2	764	596	0.03%	0.003%
44	6.465	1685	1687	1689	rBV	492	226	0.01%	0.001%
45	6.564	1715	1718	1719	rBV	507	267	0.01%	0.002%
46	6.600	1726	1729	1734	rVV3	533	466	0.02%	0.003%
47	6.622	1734	1736	1738	rVV	551	304	0.01%	0.002%
48	6.645	1741	1743	1746	rBV3	458	300	0.01%	0.002%
49	6.680	1752	1754	1757	rVB3	1048	468	0.02%	0.003%
50	6.696	1757	1759	1761	rVB	496	169	0.01%	0.001%
51	6.716	1761	1765	1770	rBV3	698	757	0.03%	0.004%
52	6.825	1797	1799	1802	rBV2	399	221	0.01%	0.001%
53	6.867	1808	1812	1813	rBV	892	579	0.02%	0.003%
54	6.918	1826	1828	1832	rVB2	428	295	0.01%	0.002%
55	6.989	1839	1850	1875	rBV	294081	535810	22.78%	3.016%
56	7.269	1935	1937	1940	rVB	872	360	0.02%	0.002%
57	7.320	1940	1953	1970	rBV	1112909	1932266	82.14%	10.876%
58	7.625	2038	2048	2069	rBV	207223	367196	15.61%	2.067%
59	7.879	2125	2127	2129	rBV	615	350	0.01%	0.002%
60	7.931	2140	2143	2144	rBV2	916	575	0.02%	0.003%
61	8.021	2168	2171	2173	rVB2	597	329	0.01%	0.002%
62	8.095	2183	2194	2225	rBV	495095	956117	40.64%	5.382%
63	8.404	2288	2290	2292	rBV2	636	289	0.01%	0.002%
64	8.632	2359	2361	2364	rVB2	565	262	0.01%	0.001%
65	8.767	2400	2403	2406	rBV3	830	525	0.02%	0.003%
66	8.857	2419	2431	2454	rBV	1057711	1714321	72.87%	9.650%
67	9.072	2494	2498	2501	rBV3	882	787	0.03%	0.004%
68	9.352	2582	2585	2587	rBV4	647	320	0.01%	0.002%
69	9.506	2632	2633	2636	rVB2	619	245	0.01%	0.001%
70	9.648	2674	2677	2679	rBV2	830	478	0.02%	0.003%
71	9.757	2708	2711	2712	rBV2	383	178	0.01%	0.001%
72	9.908	2754	2758	2760	rBV3	574	520	0.02%	0.003%
73	9.937	2764	2767	2770	rVB2	749	411	0.02%	0.002%
74	10.024	2784	2794	2805	rBV3	34489	57328	2.44%	0.323%
75	10.133	2821	2828	2838	rVB5	4151	6264	0.27%	0.035%
76	10.220	2844	2855	2875	rBV	712489	1140634	48.49%	6.420%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040221\
 Data File : VW020890.D
 Acq On : 02 Apr 2021 20:15
 Operator : SY/MD
 Sample : M1879-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.831	3042	3045	3046	rBV	470	287	0.01%	0.002%
78	10.857	3050	3053	3057	rVB5	1546	1181	0.05%	0.007%
79	10.921	3066	3073	3079	rBV5	5130	6524	0.28%	0.037%
80	11.005	3097	3099	3100	rBV2	538	239	0.01%	0.001%
81	11.030	3103	3107	3111	rBV4	983	892	0.04%	0.005%
82	11.146	3138	3143	3146	rBV6	2021	2199	0.09%	0.012%
83	11.256	3165	3177	3202	rBV	1064954	1634202	69.47%	9.199%
84	11.526	3258	3261	3263	rBV4	1136	600	0.03%	0.003%
85	11.632	3281	3294	3313	rBV	1175452	1860693	79.09%	10.474%
86	11.899	3373	3377	3379	rBV3	583	457	0.02%	0.003%
87	11.963	3395	3397	3398	rBV	598	266	0.01%	0.001%
88	12.098	3436	3439	3442	rBV	632	350	0.01%	0.002%
89	12.210	3471	3474	3479	rBV3	1154	978	0.04%	0.006%
90	12.423	3537	3540	3542	rBV2	970	548	0.02%	0.003%
91	12.545	3576	3578	3580	rBV2	604	270	0.01%	0.002%
92	12.600	3593	3595	3596	rBV	488	187	0.01%	0.001%
93	12.950	3702	3704	3705	rBV	595	188	0.01%	0.001%
94	13.194	3776	3780	3782	rBV2	524	340	0.01%	0.002%
95	13.239	3791	3794	3797	rBV3	588	442	0.02%	0.002%
96	13.265	3800	3802	3806	rBV3	733	435	0.02%	0.002%
97	13.419	3847	3850	3854	rBV2	1174	806	0.03%	0.005%
98	13.696	3933	3936	3938	rBV2	699	460	0.02%	0.003%
99	13.976	4021	4023	4026	rBV	790	473	0.02%	0.003%
100	14.088	4056	4058	4060	rBV2	769	418	0.02%	0.002%




Sum of corrected areas: 17765627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020890.D
Acq On : 02 Apr 2021 20:15
Operator : SY/MD
Sample : M1879-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

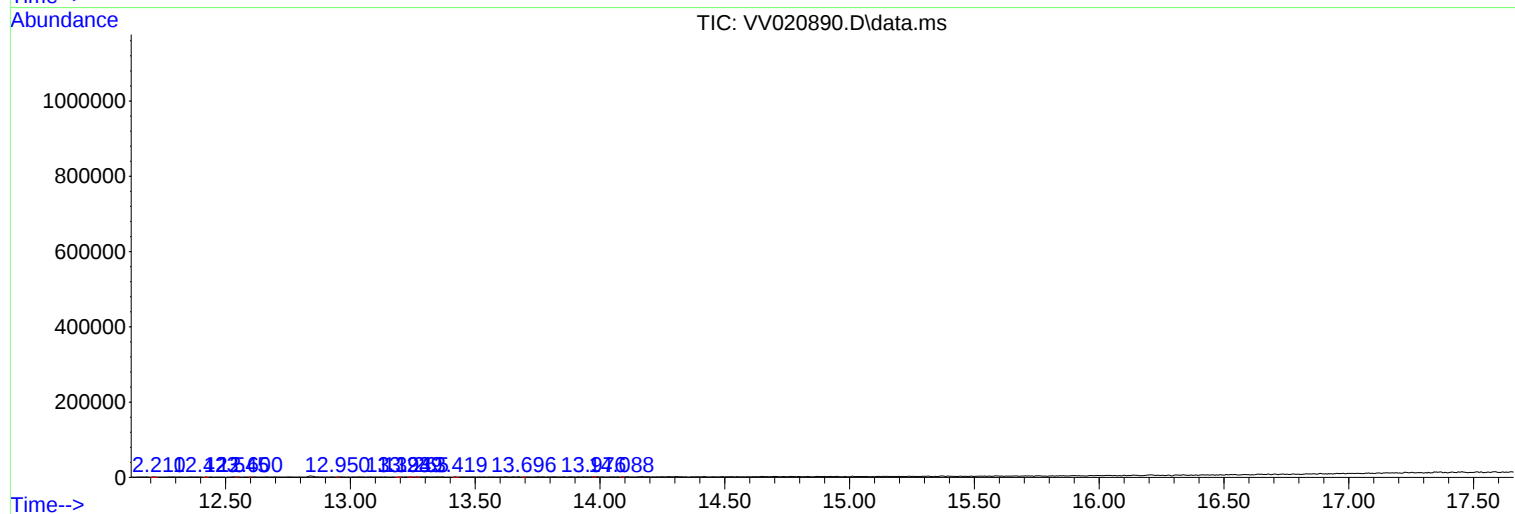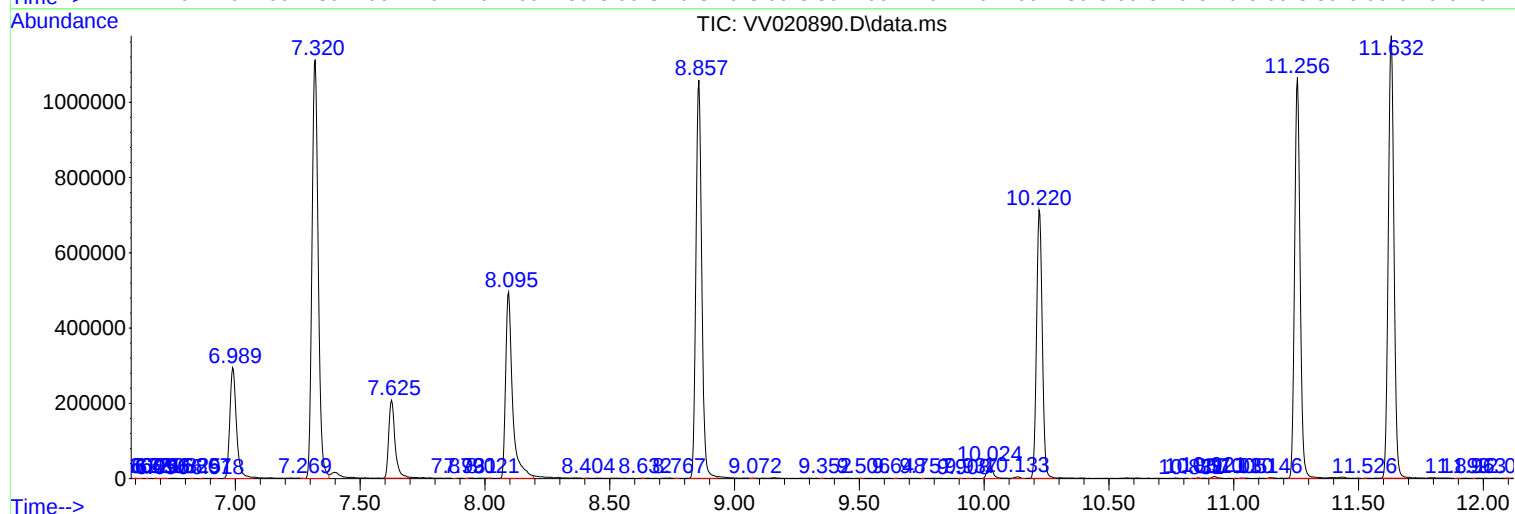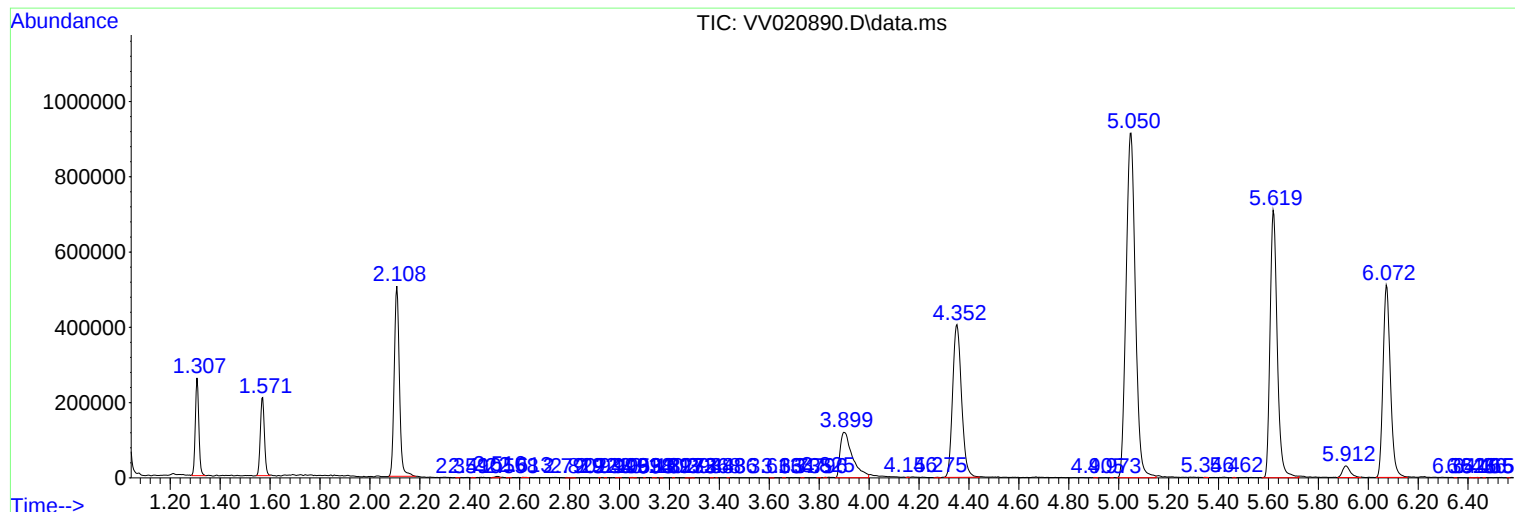

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020890.D
Acq On : 02 Apr 2021 20:15
Operator : SY/MD
Sample : M1879-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020890.D
Acq On : 02 Apr 2021 20:15
Operator : SY/MD
Sample : M1879-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
