

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020895.D
 Acq On : 02 Apr 2021 22:38
 Operator : SY/MD
 Sample : M1879-16DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rVB2	1142108	1171781	8.23%	3.543%
2	1.568	158	164	174	rVB	195801	220973	1.55%	0.668%
3	2.108	322	332	347	rBV2	484647	716959	5.03%	2.168%
4	2.256	376	378	380	rBV2	593	372	0.00%	0.001%
5	2.294	386	390	396	rVB4	845	785	0.01%	0.002%
6	2.359	408	410	413	rVB3	901	445	0.00%	0.001%
7	2.381	413	417	418	rBV2	718	491	0.00%	0.001%
8	2.426	429	431	435	rVB5	1129	656	0.00%	0.002%
9	2.471	443	445	448	rBV2	1345	538	0.00%	0.002%
10	2.603	482	486	487	rBV2	776	506	0.00%	0.002%
11	2.645	495	499	502	rBV3	525	329	0.00%	0.001%
12	2.728	523	525	527	rBV2	455	287	0.00%	0.001%
13	2.767	527	537	550	rVV3	18493	32185	0.23%	0.097%
14	2.844	559	561	564	rVB2	488	315	0.00%	0.001%
15	2.863	564	567	568	rBV2	406	270	0.00%	0.001%
16	2.889	573	575	579	rBV3	510	378	0.00%	0.001%
17	2.957	595	596	599	rBV3	565	277	0.00%	0.001%
18	3.275	693	695	697	rVB	570	283	0.00%	0.001%
19	3.336	710	714	716	rBV2	404	324	0.00%	0.001%
20	3.352	717	719	723	rVV	386	283	0.00%	0.001%
21	3.381	726	728	731	rBV2	415	279	0.00%	0.001%
22	3.445	742	748	752	rVB3	532	597	0.00%	0.002%
23	3.552	775	781	783	rBV3	805	725	0.01%	0.002%
24	3.571	786	787	790	rVV2	626	301	0.00%	0.001%
25	3.600	792	796	798	rBV3	459	272	0.00%	0.001%
26	3.613	798	800	804	rBV3	541	403	0.00%	0.001%
27	3.674	817	819	823	rVB2	501	295	0.00%	0.001%
28	3.712	828	831	832	rBV	373	213	0.00%	0.001%
29	3.841	865	871	874	rBV2	541	568	0.00%	0.002%
30	3.912	874	893	930	rBV	5891398	14241745	100.00%	43.056%
31	4.352	1017	1030	1054	rVB	388795	936675	6.58%	2.832%
32	4.809	1169	1172	1174	rVB3	1133	486	0.00%	0.001%
33	4.834	1174	1180	1183	rBV5	1072	999	0.01%	0.003%
34	4.941	1211	1213	1216	rBV3	739	372	0.00%	0.001%
35	4.982	1225	1226	1229	rBV	476	244	0.00%	0.001%
36	5.050	1229	1247	1279	rBV2	864554	2220814	15.59%	6.714%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020895.D
 Acq On : 02 Apr 2021 22:38
 Operator : SY/MD
 Sample : M1879-16DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 EW1C2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.381	1348	1350	1352	rBV	690	445	0.00%	0.001%
38	5.407	1355	1358	1363	rVB5	1216	1229	0.01%	0.004%
39	5.497	1380	1386	1387	rBV	882	782	0.01%	0.002%
40	5.622	1413	1425	1452	rBV	598512	1208553	8.49%	3.654%
41	5.918	1502	1517	1546	rBV2	999746	2006671	14.09%	6.067%
42	6.072	1553	1565	1591	rVB	472521	963182	6.76%	2.912%
43	6.336	1645	1647	1648	rBV	544	237	0.00%	0.001%
44	6.368	1655	1657	1659	rBV	534	206	0.00%	0.001%
45	6.381	1659	1661	1665	rBV2	438	271	0.00%	0.001%
46	6.487	1690	1694	1697	rBV2	561	385	0.00%	0.001%
47	6.593	1725	1727	1729	rBV2	570	279	0.00%	0.001%
48	6.632	1735	1739	1740	rBV	826	473	0.00%	0.001%
49	6.667	1747	1750	1751	rBV2	476	255	0.00%	0.001%
50	6.741	1771	1773	1780	rVB6	1150	900	0.01%	0.003%
51	6.805	1791	1793	1795	rBV2	918	438	0.00%	0.001%
52	6.854	1806	1808	1810	rBV	656	297	0.00%	0.001%
53	6.902	1822	1823	1826	rVV2	448	236	0.00%	0.001%
54	6.989	1837	1850	1871	rBV	285061	517376	3.63%	1.564%
55	7.320	1941	1953	1972	rBV	1057021	1822405	12.80%	5.510%
56	7.625	2037	2048	2064	rBV2	202504	341938	2.40%	1.034%
57	7.863	2120	2122	2123	rBV	657	317	0.00%	0.001%
58	7.892	2128	2131	2135	rVB3	846	602	0.00%	0.002%
59	7.911	2135	2137	2139	rBV	618	297	0.00%	0.001%
60	8.095	2183	2194	2228	rBV	477993	937875	6.59%	2.835%
61	8.564	2337	2340	2342	rVB2	1172	658	0.00%	0.002%
62	8.577	2342	2344	2346	rBV2	500	252	0.00%	0.001%
63	8.677	2373	2375	2378	rBV3	400	296	0.00%	0.001%
64	8.805	2410	2415	2416	rBV	641	549	0.00%	0.002%
65	8.857	2419	2431	2457	rVV	919759	1482550	10.41%	4.482%
66	9.127	2513	2515	2518	rBV4	638	382	0.00%	0.001%
67	9.230	2545	2547	2550	rBV2	690	402	0.00%	0.001%
68	9.429	2606	2609	2610	rBV2	431	218	0.00%	0.001%
69	9.474	2621	2623	2627	rVB	496	297	0.00%	0.001%
70	9.535	2640	2642	2645	rVB	749	359	0.00%	0.001%
71	9.590	2655	2659	2661	rBV2	1113	807	0.01%	0.002%
72	9.603	2661	2663	2665	rVV	578	294	0.00%	0.001%
73	9.821	2727	2731	2732	rBV2	342	240	0.00%	0.001%
74	9.911	2756	2759	2763	rVB4	743	483	0.00%	0.001%
75	9.937	2763	2767	2769	rBV2	677	552	0.00%	0.002%
76	9.979	2777	2780	2781	rBV	771	366	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020895.D
 Acq On : 02 Apr 2021 22:38
 Operator : SY/MD
 Sample : M1879-16DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1C2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.095	2814	2816	2820	rVB2	501	257	0.00%	0.001%
78	10.133	2820	2828	2833	rBV6	3954	5875	0.04%	0.018%
79	10.220	2843	2855	2878	rBV	690279	1078799	7.57%	3.261%
80	10.387	2903	2907	2909	rBV	615	456	0.00%	0.001%
81	10.458	2926	2929	2931	rBV3	908	494	0.00%	0.001%
82	10.786	3028	3031	3032	rBV2	1286	620	0.00%	0.002%
83	10.831	3043	3045	3047	rBV2	523	294	0.00%	0.001%
84	11.040	3108	3110	3114	rVB3	719	412	0.00%	0.001%
85	11.255	3165	3177	3197	rBV	893827	1380284	9.69%	4.173%
86	11.538	3264	3265	3267	rBV	404	211	0.00%	0.001%
87	11.632	3282	3294	3315	rBV	1125112	1755473	12.33%	5.307%
88	11.869	3366	3368	3373	rVB3	812	566	0.00%	0.002%
89	11.895	3374	3376	3378	rBV2	724	322	0.00%	0.001%
90	11.924	3383	3385	3386	rBV	683	265	0.00%	0.001%
91	12.062	3426	3428	3433	rBV2	681	356	0.00%	0.001%
92	12.574	3583	3587	3590	rBV2	701	545	0.00%	0.002%
93	12.644	3607	3609	3610	rBV2	540	252	0.00%	0.001%
94	12.818	3661	3663	3666	rVB2	854	320	0.00%	0.001%
95	12.869	3676	3679	3681	rBV2	793	541	0.00%	0.002%
96	12.940	3699	3701	3703	rBV2	573	270	0.00%	0.001%
97	13.175	3771	3774	3778	rBV4	685	495	0.00%	0.001%
98	13.358	3829	3831	3834	rBV	529	422	0.00%	0.001%
99	13.911	4000	4003	4008	rBV3	1396	1183	0.01%	0.004%
100	14.461	4172	4174	4175	rBV2	1111	487	0.00%	0.001%




Sum of corrected areas: 33076978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020895.D
Acq On : 02 Apr 2021 22:38
Operator : SY/MD
Sample : M1879-16DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

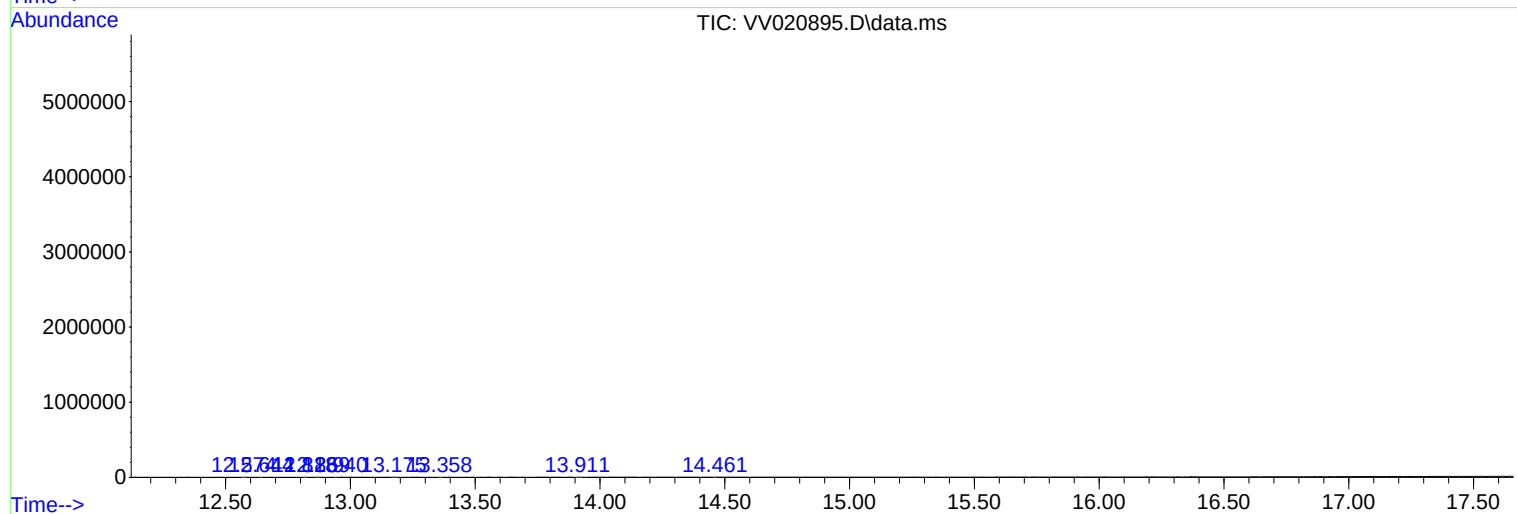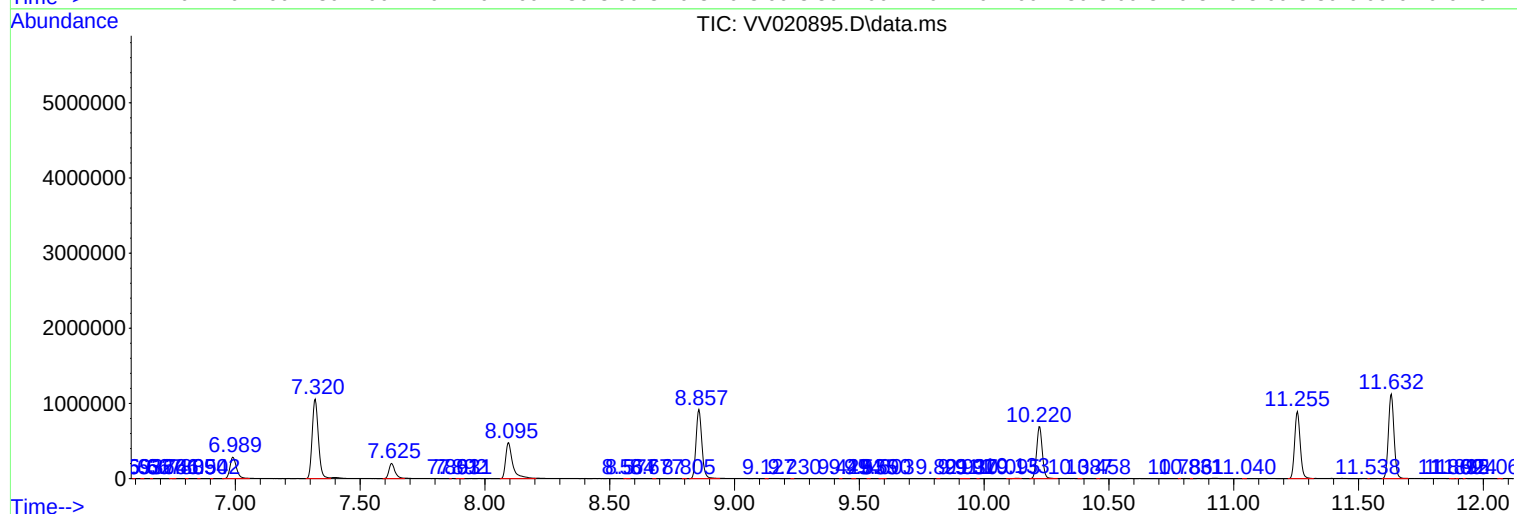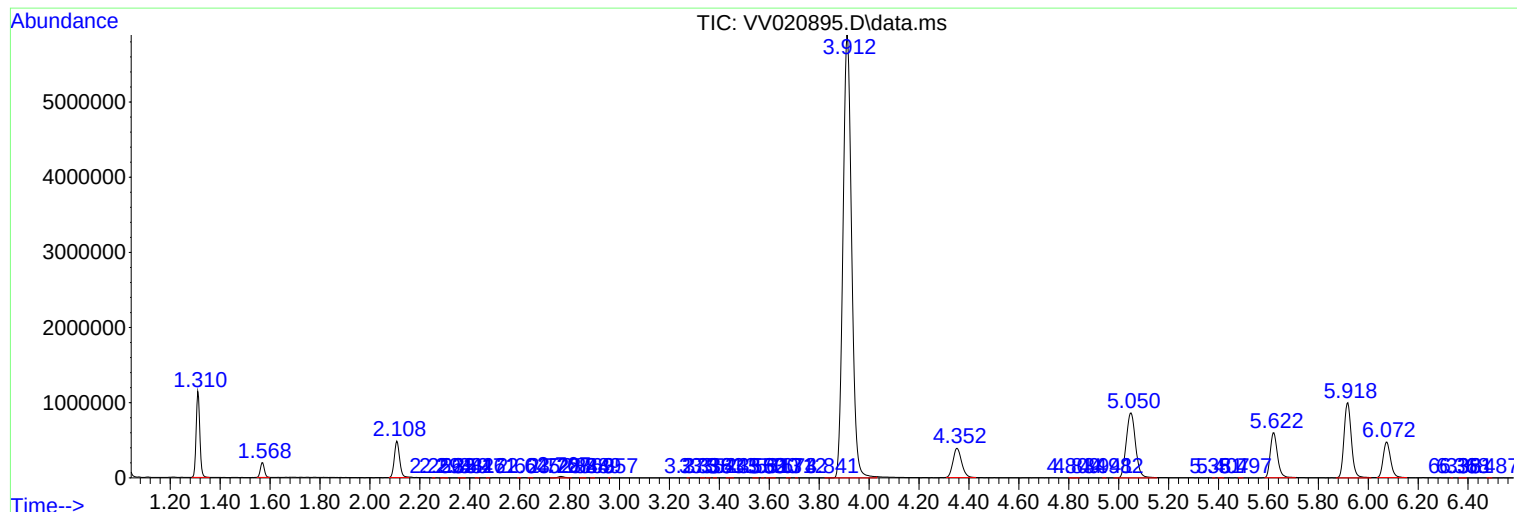

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020895.D
Acq On : 02 Apr 2021 22:38
Operator : SY/MD
Sample : M1879-16DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020895.D
Acq On : 02 Apr 2021 22:38
Operator : SY/MD
Sample : M1879-16DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1C2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
