

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020897.D
 Acq On : 02 Apr 2021 23:26
 Operator : SY/MD
 Sample : M1845-11DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB2	1080536	1142082	50.54%	6.104%
2	1.571	158	165	175	rBV	202455	224824	9.95%	1.202%
3	2.108	322	332	344	rBV	475822	688163	30.45%	3.678%
4	2.294	386	390	393	rBV3	1146	1100	0.05%	0.006%
5	2.426	428	431	432	rBV2	750	351	0.02%	0.002%
6	2.510	449	457	466	rBV6	2923	5145	0.23%	0.027%
7	2.703	515	517	519	rVB	680	284	0.01%	0.002%
8	2.799	544	547	548	rBV2	584	357	0.02%	0.002%
9	2.831	554	557	559	rBV2	705	373	0.02%	0.002%
10	2.851	559	563	567	rVV2	644	632	0.03%	0.003%
11	2.918	583	584	588	rBV2	498	243	0.01%	0.001%
12	2.960	592	597	603	rBV2	418	576	0.03%	0.003%
13	3.002	607	610	614	rBV2	453	469	0.02%	0.003%
14	3.146	651	655	657	rBV2	427	358	0.02%	0.002%
15	3.182	660	666	667	rBV3	501	347	0.02%	0.002%
16	3.230	679	681	684	rVB	530	256	0.01%	0.001%
17	3.333	710	713	714	rBV	477	290	0.01%	0.002%
18	3.407	732	736	739	rVB4	615	496	0.02%	0.003%
19	3.436	742	745	747	rBV	540	251	0.01%	0.001%
20	3.458	748	752	754	rBV3	412	335	0.01%	0.002%
21	3.539	774	777	781	rBV2	578	408	0.02%	0.002%
22	3.616	799	801	806	rVB2	444	285	0.01%	0.002%
23	3.645	807	810	813	rVB2	547	328	0.01%	0.002%
24	3.670	814	818	822	rVB3	331	307	0.01%	0.002%
25	3.760	843	846	848	rBV2	760	486	0.02%	0.003%
26	3.850	871	874	878	rBV4	695	648	0.03%	0.003%
27	3.912	878	893	930	rBV2	578891	1575884	69.73%	8.423%
28	4.352	1015	1030	1058	rBV	396219	962321	42.58%	5.143%
29	4.902	1198	1201	1202	rBV	493	244	0.01%	0.001%
30	5.050	1230	1247	1274	rBV2	879412	2259936	100.00%	12.079%
31	5.619	1411	1424	1452	rBV	611722	1233492	54.58%	6.593%
32	5.912	1507	1515	1539	rVB3	32329	66958	2.96%	0.358%
33	6.072	1552	1565	1591	rBV	493005	998487	44.18%	5.337%
34	6.358	1651	1654	1657	rVB3	717	391	0.02%	0.002%
35	6.535	1707	1709	1714	rBV	693	462	0.02%	0.002%
36	6.609	1728	1732	1736	rBV3	507	354	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020897.D
 Acq On : 02 Apr 2021 23:26
 Operator : SY/MD
 Sample : M1845-11DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

37	6.629	1736	1738	1740	rVV	762	313	0.01%	0.002%
38	6.641	1740	1742	1744	rVB	621	242	0.01%	0.001%
39	6.747	1771	1775	1777	rBV	749	450	0.02%	0.002%
40	6.854	1805	1808	1812	rBV3	611	501	0.02%	0.003%
41	6.905	1823	1824	1831	rVB3	692	608	0.03%	0.003%
42	6.937	1831	1834	1835	rBV	384	237	0.01%	0.001%
43	6.989	1839	1850	1876	rBV	283473	521334	23.07%	2.786%
44	7.320	1941	1953	1972	rBV	1083616	1870780	82.78%	9.999%
45	7.625	2038	2048	2066	rBV	200677	353954	15.66%	1.892%
46	7.825	2106	2110	2112	rBV2	1291	794	0.04%	0.004%
47	7.854	2117	2119	2120	rBV2	590	270	0.01%	0.001%
48	8.095	2183	2194	2223	rBV	469455	936706	41.45%	5.006%
49	8.336	2266	2269	2272	rBV3	1092	659	0.03%	0.004%
50	8.445	2301	2303	2305	rBV3	829	485	0.02%	0.003%
51	8.481	2311	2314	2315	rBV2	610	327	0.01%	0.002%
52	8.529	2327	2329	2333	rBV5	739	427	0.02%	0.002%
53	8.603	2350	2352	2353	rBV	587	301	0.01%	0.002%
54	8.638	2361	2363	2366	rBV2	619	313	0.01%	0.002%
55	8.693	2378	2380	2383	rVB3	573	367	0.02%	0.002%
56	8.712	2383	2386	2387	rBV2	889	603	0.03%	0.003%
57	8.857	2419	2431	2458	rBV	921828	1490296	65.94%	7.965%
58	9.053	2490	2492	2498	rVB3	1091	595	0.03%	0.003%
59	9.146	2518	2521	2524	rVB4	1323	773	0.03%	0.004%
60	9.278	2559	2562	2563	rBV2	459	229	0.01%	0.001%
61	9.390	2594	2597	2598	rBV	394	215	0.01%	0.001%
62	9.452	2613	2616	2618	rBV2	492	330	0.01%	0.002%
63	9.490	2625	2628	2631	rVB3	766	464	0.02%	0.002%
64	9.516	2633	2636	2638	rBV2	589	401	0.02%	0.002%
65	9.667	2681	2683	2685	rBV	367	213	0.01%	0.001%
66	9.744	2702	2707	2710	rBV	592	416	0.02%	0.002%
67	9.760	2710	2712	2715	rBV2	340	221	0.01%	0.001%
68	9.879	2747	2749	2755	rVB3	897	747	0.03%	0.004%
69	9.911	2755	2759	2760	rBV	311	220	0.01%	0.001%
70	9.927	2761	2764	2770	rVV3	672	661	0.03%	0.004%
71	10.017	2790	2792	2794	rBV	888	553	0.02%	0.003%
72	10.133	2820	2828	2836	rBV4	2783	4727	0.21%	0.025%
73	10.223	2842	2856	2872	rBV	715030	1118620	49.50%	5.979%
74	10.368	2897	2901	2902	rBV3	939	595	0.03%	0.003%
75	10.480	2932	2936	2940	rVB2	900	690	0.03%	0.004%
76	10.509	2940	2945	2948	rBV3	644	559	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020897.D
 Acq On : 02 Apr 2021 23:26
 Operator : SY/MD
 Sample : M1845-11DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1B7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	10.554	2957	2959	2961	rBV2	545	293	0.01%	0.002%
78	10.603	2972	2974	2977	rBV	838	545	0.02%	0.003%
79	10.670	2993	2995	3000	rVB3	941	663	0.03%	0.004%
80	10.731	3010	3014	3019	rVB3	668	613	0.03%	0.003%
81	10.773	3025	3027	3029	rBV	607	302	0.01%	0.002%
82	10.889	3061	3063	3065	rBV	447	211	0.01%	0.001%
83	10.927	3067	3075	3081	rVV8	3820	5084	0.22%	0.027%
84	10.992	3093	3095	3097	rVB2	634	211	0.01%	0.001%
85	11.085	3122	3124	3125	rBV	569	219	0.01%	0.001%
86	11.117	3132	3134	3139	rVB2	497	370	0.02%	0.002%
87	11.146	3139	3143	3144	rBV2	1513	1090	0.05%	0.006%
88	11.255	3162	3177	3203	rBV	931444	1421356	62.89%	7.597%
89	11.490	3248	3250	3254	rVB3	672	352	0.02%	0.002%
90	11.632	3281	3294	3314	rBV	1137793	1793108	79.34%	9.584%
91	11.921	3379	3384	3388	rBV5	840	875	0.04%	0.005%
92	12.014	3411	3413	3416	rBV2	907	492	0.02%	0.003%
93	12.101	3438	3440	3446	rBV3	649	387	0.02%	0.002%
94	12.278	3492	3495	3497	rBV3	940	498	0.02%	0.003%
95	12.802	3651	3658	3664	rBV4	859	1379	0.06%	0.007%
96	13.332	3818	3823	3824	rBV2	563	486	0.02%	0.003%
97	13.374	3833	3836	3840	rBV4	735	732	0.03%	0.004%
98	13.551	3889	3891	3893	rBV2	835	369	0.02%	0.002%
99	13.947	4011	4014	4017	rBV3	1110	670	0.03%	0.004%
100	14.631	4224	4227	4228	rBV	1169	577	0.03%	0.003%




Sum of corrected areas: 18710001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020897.D
Acq On : 02 Apr 2021 23:26
Operator : SY/MD
Sample : M1845-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

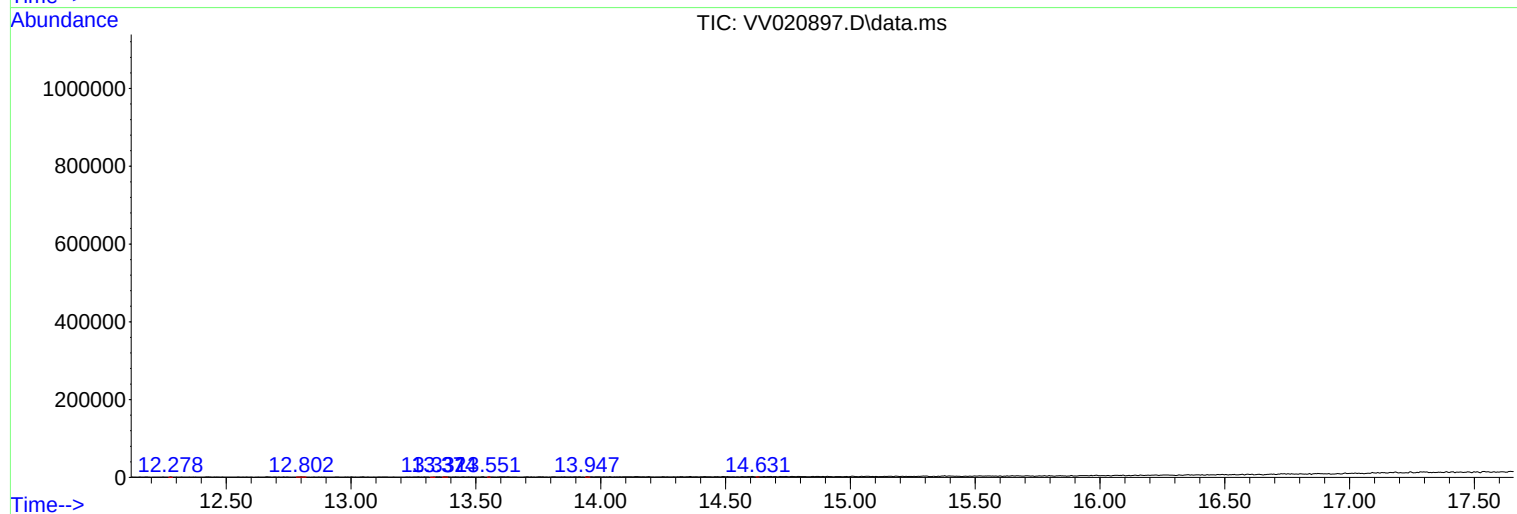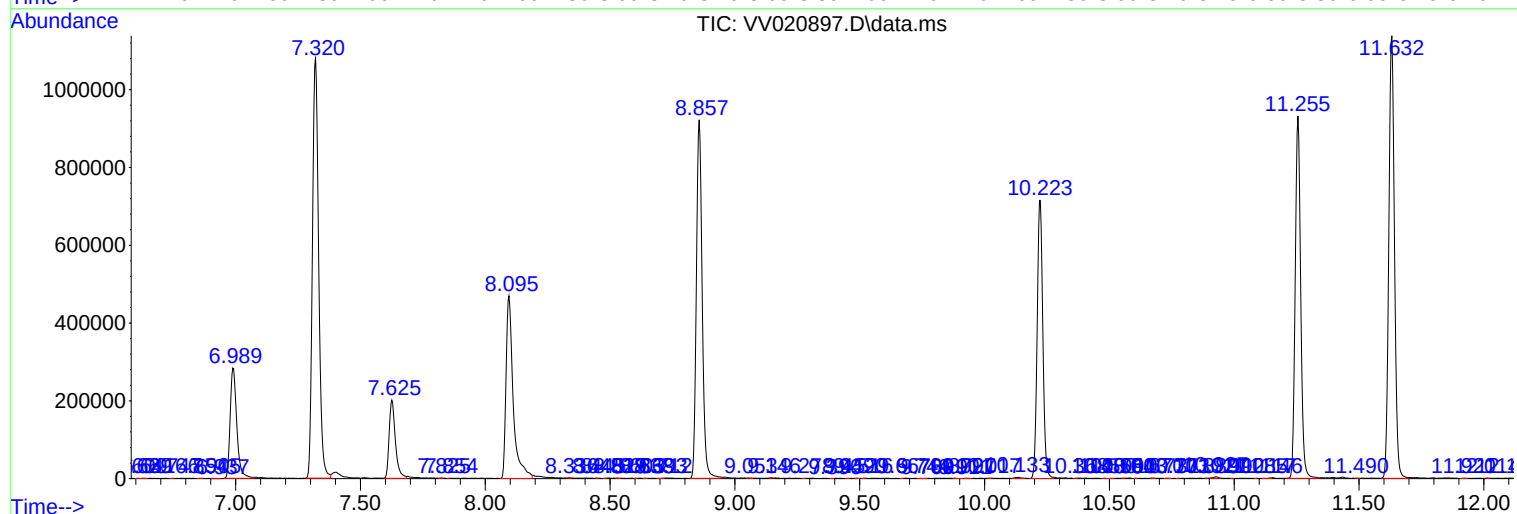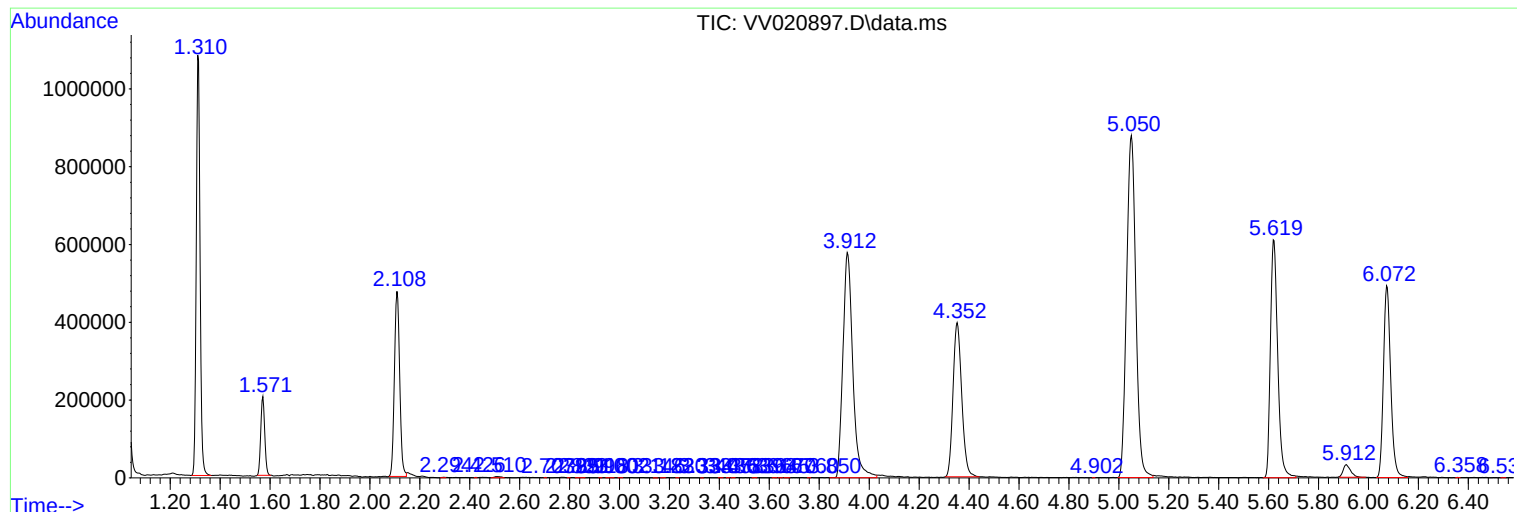

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020897.D
Acq On : 02 Apr 2021 23:26
Operator : SY/MD
Sample : M1845-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B7DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.912	2.71 ug/L	66958	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Clorethate	322	C5H4Cl6O3	005634-37-7	28
2			Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	27
3			Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	23
4			5-Aminoindazole	133	C7H7N3	019335-11-6	9
5			Benzene, fluoro-	96	C6H5F	000462-06-6	9

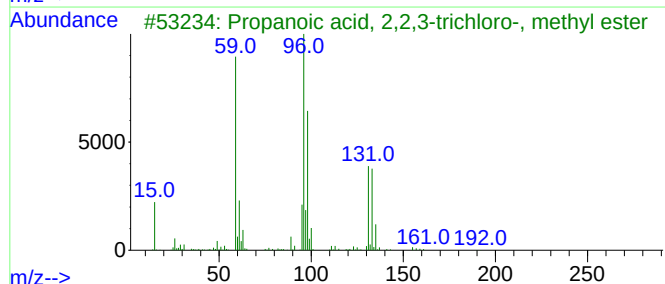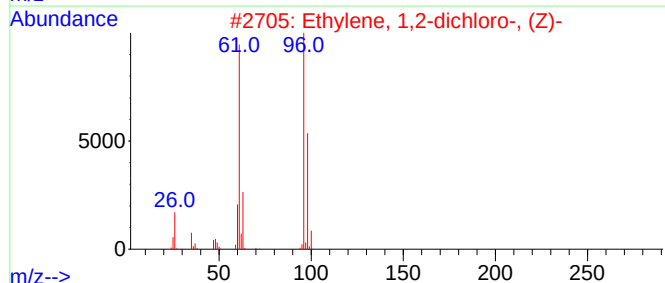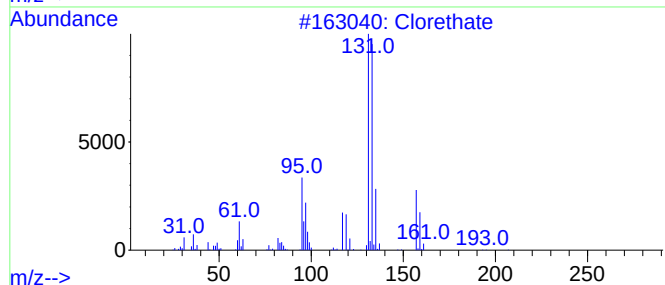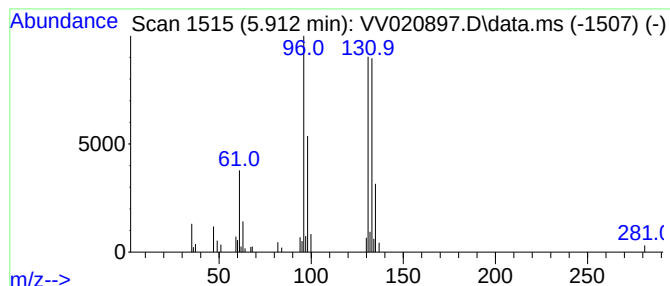

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
Data File : VV020897.D
Acq On : 02 Apr 2021 23:26
Operator : SY/MD
Sample : M1845-11DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1B7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	5.912	2.7	ug/L	66958	1	5.622	1233490	50.0