
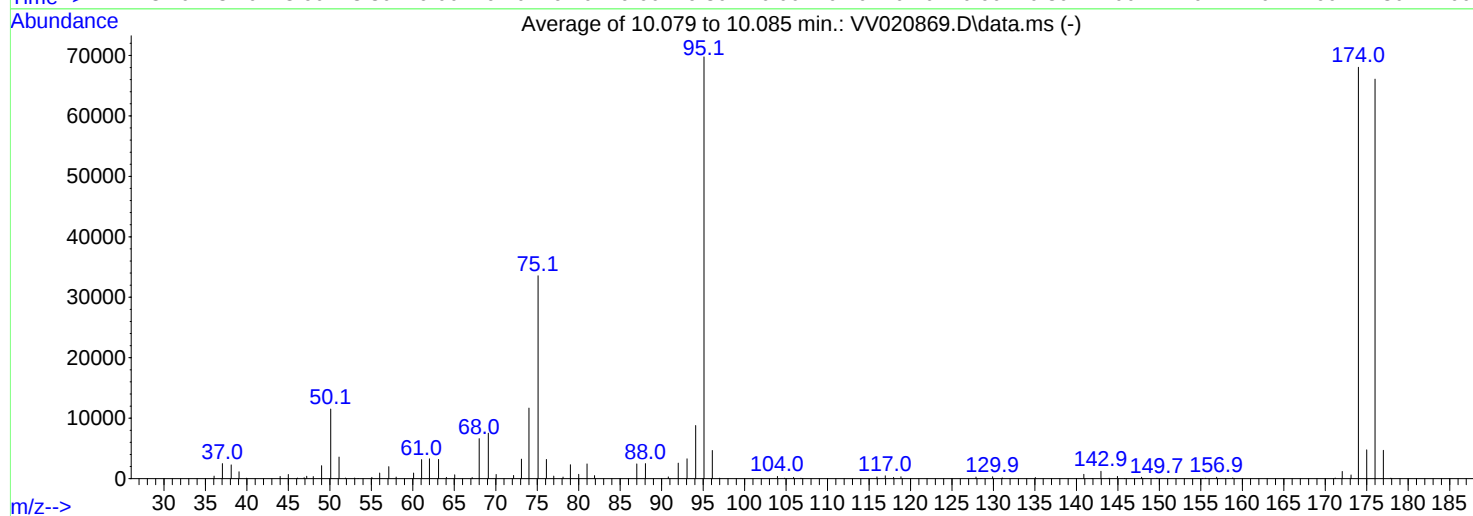


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040221\
 Data File : VV020869.D
 Acq On : 02 Apr 2021 09:01
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis
 Last Update : Wed Apr 07 02:10:23 2021

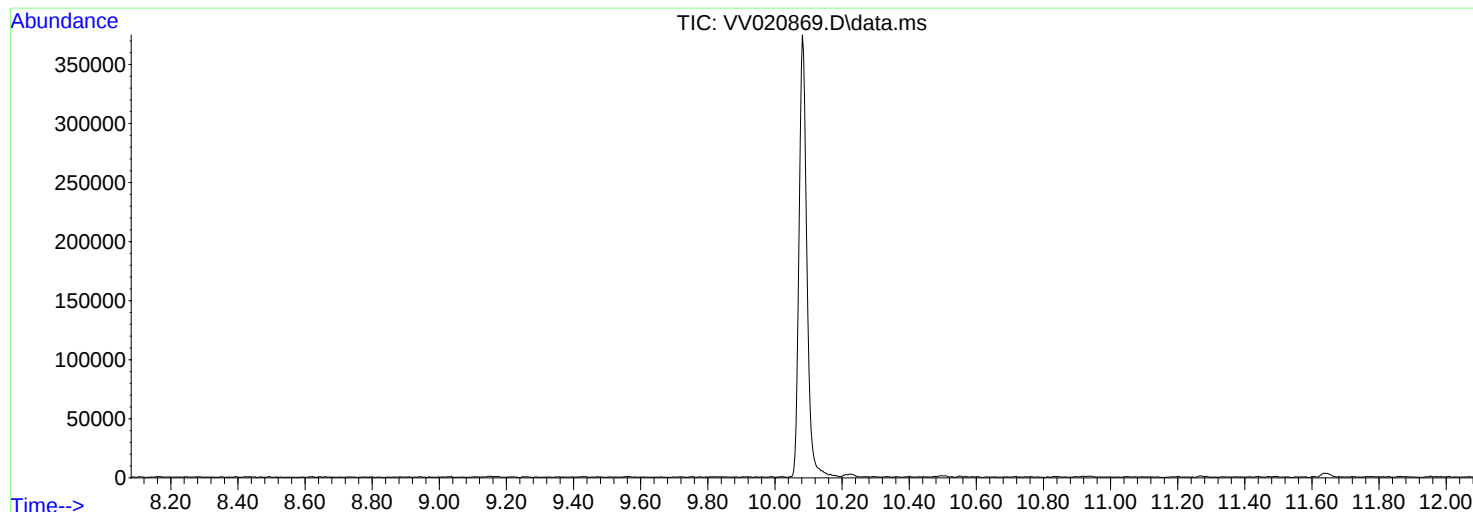

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	11515	PASS
75	95	30	80	48.1	33555	PASS
95	95	100	100	100.0	69768	PASS
96	95	5	9	6.7	4670	PASS
173	174	0.00	2	0.9	605	PASS
174	95	50	120	97.5	68048	PASS
175	174	5	9	7.0	4758	PASS
176	174	95	101	97.1	66093	PASS
177	176	5	9	7.1	4676	PASS

m/z	Abundance
36.10	441.0
37.00	2550.0
38.10	2479.0
39.00	1260.0
40.10	265.0
44.00	732.0
45.00	680.0
46.90	474.0
48.00	365.0
49.00	2160.0
50.10	10875.0
51.10	3490.0
53.00	158.0
55.00	145.0
56.00	926.0
57.10	1914.0
58.00	310.0
60.10	930.0
61.00	3419.0
62.00	3175.0
63.10	3048.0
64.10	242.0
65.10	710.0
67.10	212.0
68.00	6582.0
69.10	7300.0
70.10	726.0
72.20	444.0
73.10	2981.0
74.00	11520.0
75.10	32936.0
76.20	3414.0
77.00	393.0
78.10	298.0
79.00	2471.0
80.00	721.0
81.00	2468.0
81.90	433.0
87.00	2234.0
88.10	2583.0
90.80	249.0
92.00	2534.0
93.10	3281.0
94.10	8187.0
95.10	67456.0
96.10	4627.0
97.00	119.0
104.00	452.0
105.90	234.0
106.80	122.0
115.90	272.0
116.90	451.0
118.10	193.0
118.90	353.0
127.90	166.0
129.90	260.0
131.10	117.0
135.00	144.0
140.90	758.0
142.90	1190.0
144.00	107.0
145.00	322.0
147.80	211.0
155.60	128.0
156.90	196.0
158.90	117.0
171.20	167.0
172.00	1132.0
173.10	913.0
174.00	63576.0
175.00	5017.0
176.00	62712.0
177.00	4376.0
177.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.10	435.0
37.00	2642.0
38.10	2255.0
39.00	1144.0
40.10	245.0
44.10	773.0
45.00	738.0
46.10	155.0
47.20	561.0
48.00	368.0
49.00	2026.0
50.10	11979.0
51.10	3743.0
51.90	165.0
53.00	151.0
55.00	231.0
56.00	958.0
57.10	2129.0
58.00	249.0
60.10	925.0
61.00	3258.0
62.00	3282.0
63.10	3289.0
64.10	224.0
65.00	660.0
67.10	187.0
68.00	6909.0
69.10	7921.0
70.10	680.0
72.10	564.0
73.10	3425.0
74.00	11967.0
75.10	34976.0
76.10	3208.0
77.00	459.0
78.10	265.0
79.00	2428.0
80.00	746.0
81.00	2518.0
81.90	492.0
87.00	2559.0
88.00	2557.0
90.80	332.0
92.00	2721.0
93.10	3405.0
94.10	9130.0
95.10	71864.0
96.10	4808.0
104.00	377.0
104.80	113.0
105.90	215.0
106.80	124.0
115.90	297.0
117.00	488.0
117.90	213.0
118.80	320.0
127.90	266.0
129.90	347.0
131.10	157.0
135.00	211.0
140.90	736.0
143.00	1229.0
143.90	109.0
144.90	407.0
147.90	264.0
149.70	122.0
155.60	118.0
156.90	259.0
158.80	145.0
171.20	164.0
172.00	1260.0
173.10	902.0
174.00	70640.0
175.00	4867.0
176.00	68776.0
177.00	4989.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	404.0
37.10	2266.0
38.10	2132.0
39.10	1002.0
40.00	283.0
44.10	689.0
45.00	621.0
46.10	165.0
47.20	607.0
48.00	329.0
49.00	2253.0
50.10	11690.0
51.10	3516.0
51.90	160.0
53.40	111.0
55.10	259.0
56.00	938.0
57.10	1910.0
58.00	211.0
60.10	908.0
61.10	2805.0
62.00	3402.0
63.10	3237.0
63.90	196.0
65.00	566.0
67.20	149.0
68.00	6336.0
69.10	7336.0
70.00	636.0
72.10	566.0
73.10	3324.0
74.00	11540.0
75.10	32752.0
76.00	2930.0
77.00	429.0
78.10	220.0
79.00	2003.0
80.00	705.0
81.00	2306.0
81.90	588.0
87.00	2506.0
88.00	2289.0
90.80	295.0
92.00	2442.0
93.00	3138.0
94.10	9075.0
95.10	69984.0
96.10	4576.0
97.00	106.0
103.90	331.0
104.80	133.0
105.90	203.0
107.00	109.0
116.00	294.0
117.00	482.0
117.90	275.0
118.80	281.0
127.90	351.0
128.50	113.0
129.90	364.0
131.00	137.0
135.10	178.0
140.90	680.0
141.90	105.0
143.00	1244.0
144.90	420.0
145.80	128.0
147.90	278.0
149.70	105.0
155.20	104.0
156.90	234.0
158.80	133.0
172.10	1217.0
174.00	69928.0
175.00	4389.0
176.00	66792.0
177.00	4662.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Scan 2799 (10.040 min): VV020869.D\data.ms
BFB71

m/z	Abundance
39.90	181.0
44.00	362.0
89.50	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71