

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
 Data File : VV034927.D
 Acq On : 02 Apr 2024 12:46
 Operator : SY/MD
 Sample : P1925-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 FB(20240326)

Quant Time: Apr 03 05:19:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 03 05:08:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	175094	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	171960	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	75541	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	73097	5.066	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.400%	
7) Chloroethane-d5	1.532	69	58812	4.943	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.800%	
11) 1,1-Dichloroethene-d2	2.056	65	32337	4.934	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.600%	
20) 2-Butanone-d5	3.834	46	92412	40.930	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	81.860%	
24) Chloroform-d	4.249	84	111995	4.797	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
26) 1,2-Dichloroethane-d4	4.944	65	54561	5.174	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.400%	
32) Benzene-d6	4.960	84	228288	5.075	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
36) 1,2-Dichloropropane-d6	5.989	67	70074	5.308	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.200%	
41) Toluene-d8	7.243	98	193500	4.736	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.800%	
43) trans-1,3-Dichloroprop...	7.561	79	21420	4.567	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.400%	
46) 2-Hexanone-d5	8.030	63	75467	46.884	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.760%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	46772	5.077	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152	63806	5.362	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.200%	
Target Compounds						
16) Methylene chloride	2.445	84	6538	0.448	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
Data File : VV034927.D
Acq On : 02 Apr 2024 12:46
Operator : SY/MD
Sample : P1925-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
FB(20240326)

Quant Time: Apr 03 05:19:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 03 05:08:19 2024
Response via : Initial Calibration

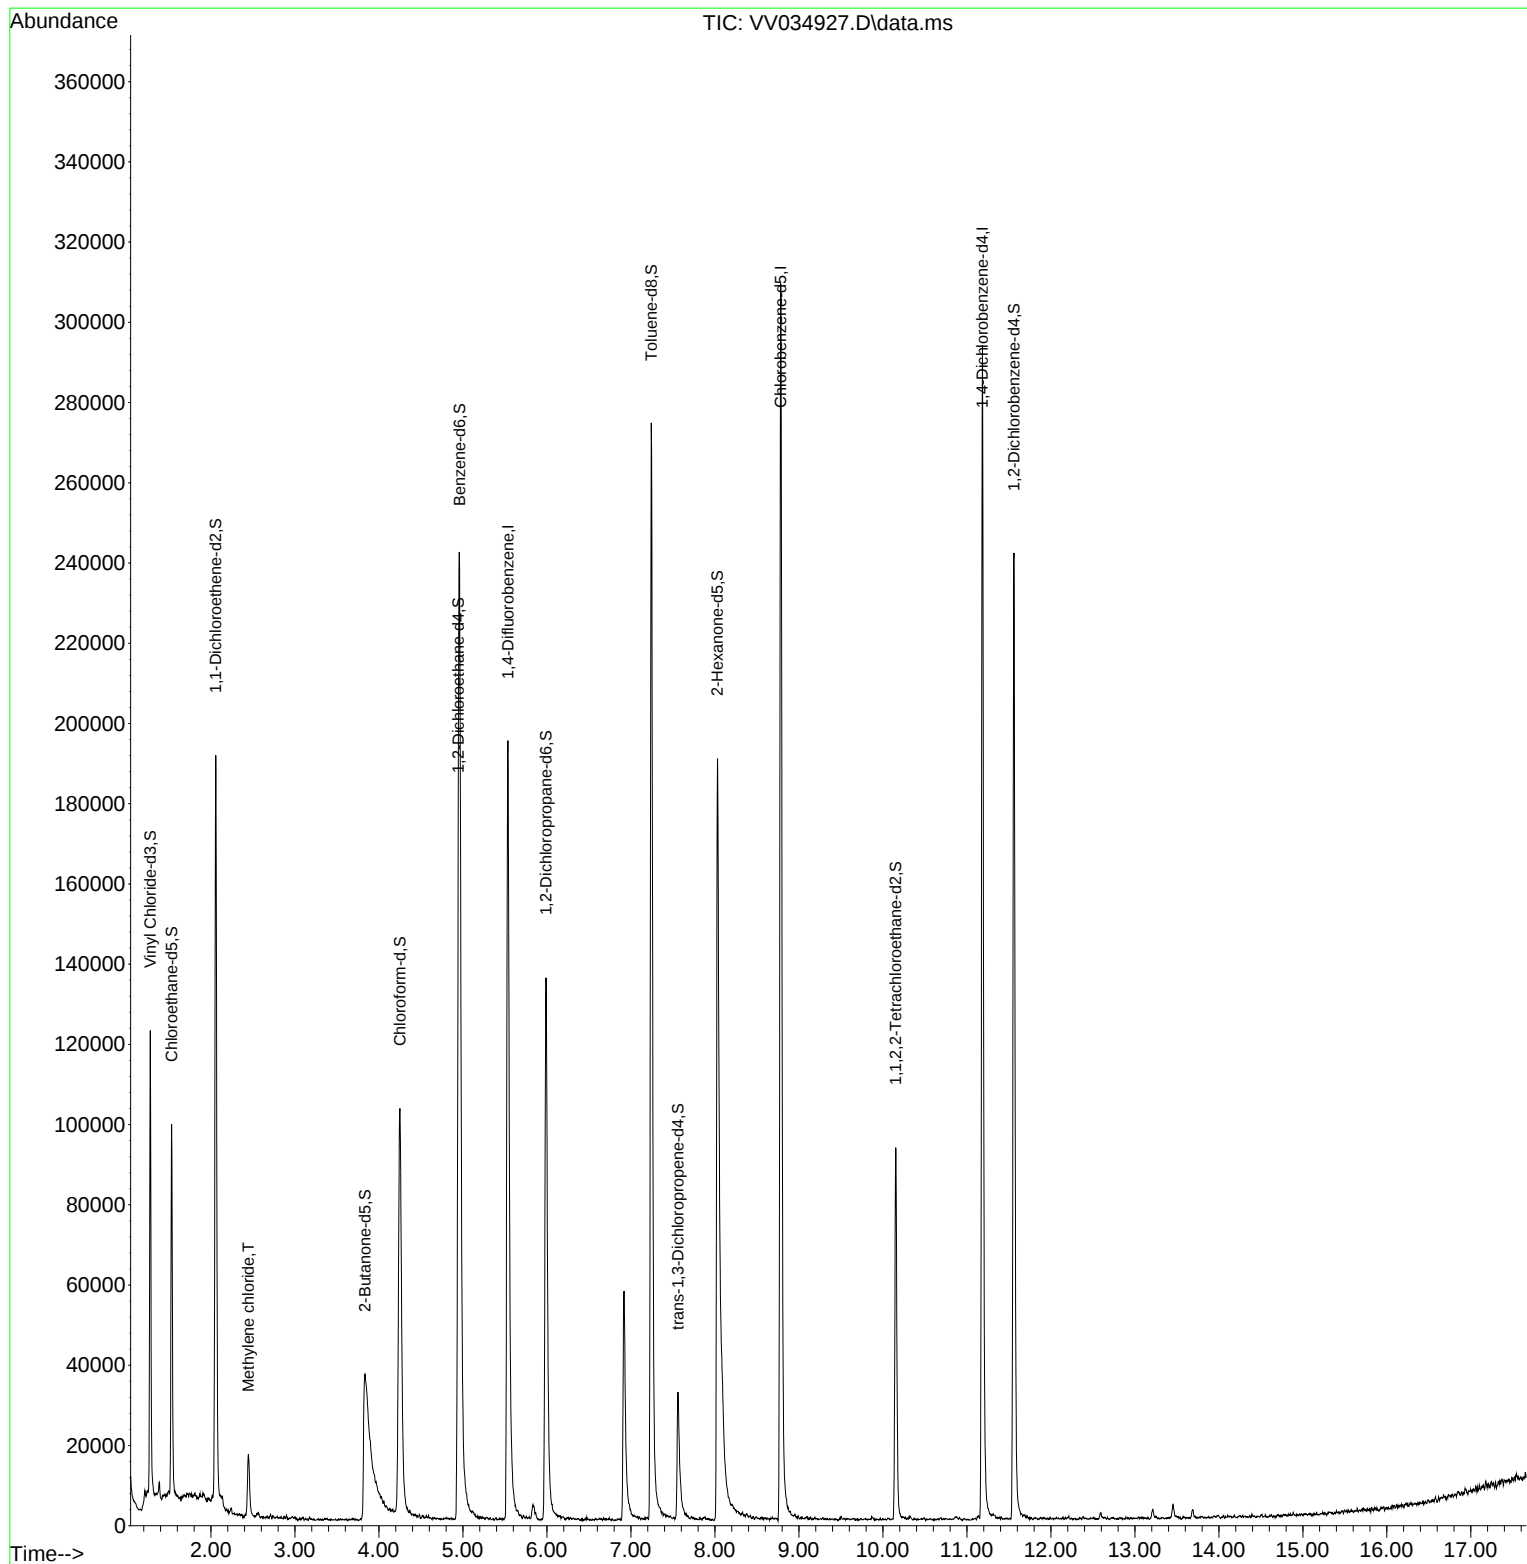

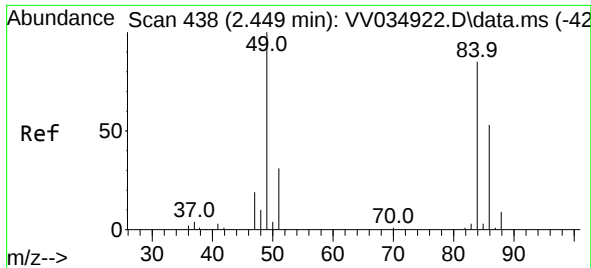

#16
Methylene chloride
Concen: 0.448 ug/L
RT: 2.445 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV034927.D
Acq: 02 Apr 2024 12:46

Instrument :
MSVOA_V
ClientSampleId :
FB(20240326)

Tgt Ion:	84	Resp:	6538
Ion	Ratio	Lower	Upper
84	100		
86	62.8	43.5	80.9
49	131.0	82.5	153.3

