

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
 Data File : VV034929.D
 Acq On : 02 Apr 2024 13:34
 Operator : SY/MD
 Sample : P1925-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 FB(20240327)

Quant Time: Apr 03 05:19:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 03 05:08:19 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	169577	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	170777	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	73453	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	74321	5.318	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 106.400%		
7) Chloroethane-d5	1.532	69	62070	5.387	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 107.800%		
11) 1,1-Dichloroethene-d2	2.060	65	33112	5.217	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 104.400%		
20) 2-Butanone-d5	3.815	46	76112	34.807	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 69.620%		
24) Chloroform-d	4.249	84	120345	5.322	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 106.400%		
26) 1,2-Dichloroethane-d4	4.947	65	58045	5.684	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 113.600%		
32) Benzene-d6	4.960	84	248558	5.564	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 111.200%		
36) 1,2-Dichloropropane-d6	5.989	67	74520	5.684	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 113.600%		
41) Toluene-d8	7.243	98	207479	5.113	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 102.200%		
43) trans-1,3-Dichloroprop...	7.561	79	24138	5.182	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 103.600%		
46) 2-Hexanone-d5	8.030	63	84692	52.980	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 105.960%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	50870	5.561	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 111.200%		
66) 1,2-Dichlorobenzene-d4	11.561	152	69857	6.038	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 120.800%#		
Target Compounds						
16) Methylene chloride	2.449	84	9021	0.639	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
Data File : VV034929.D
Acq On : 02 Apr 2024 13:34
Operator : SY/MD
Sample : P1925-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
FB(20240327)

Quant Time: Apr 03 05:19:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 03 05:08:19 2024
Response via : Initial Calibration

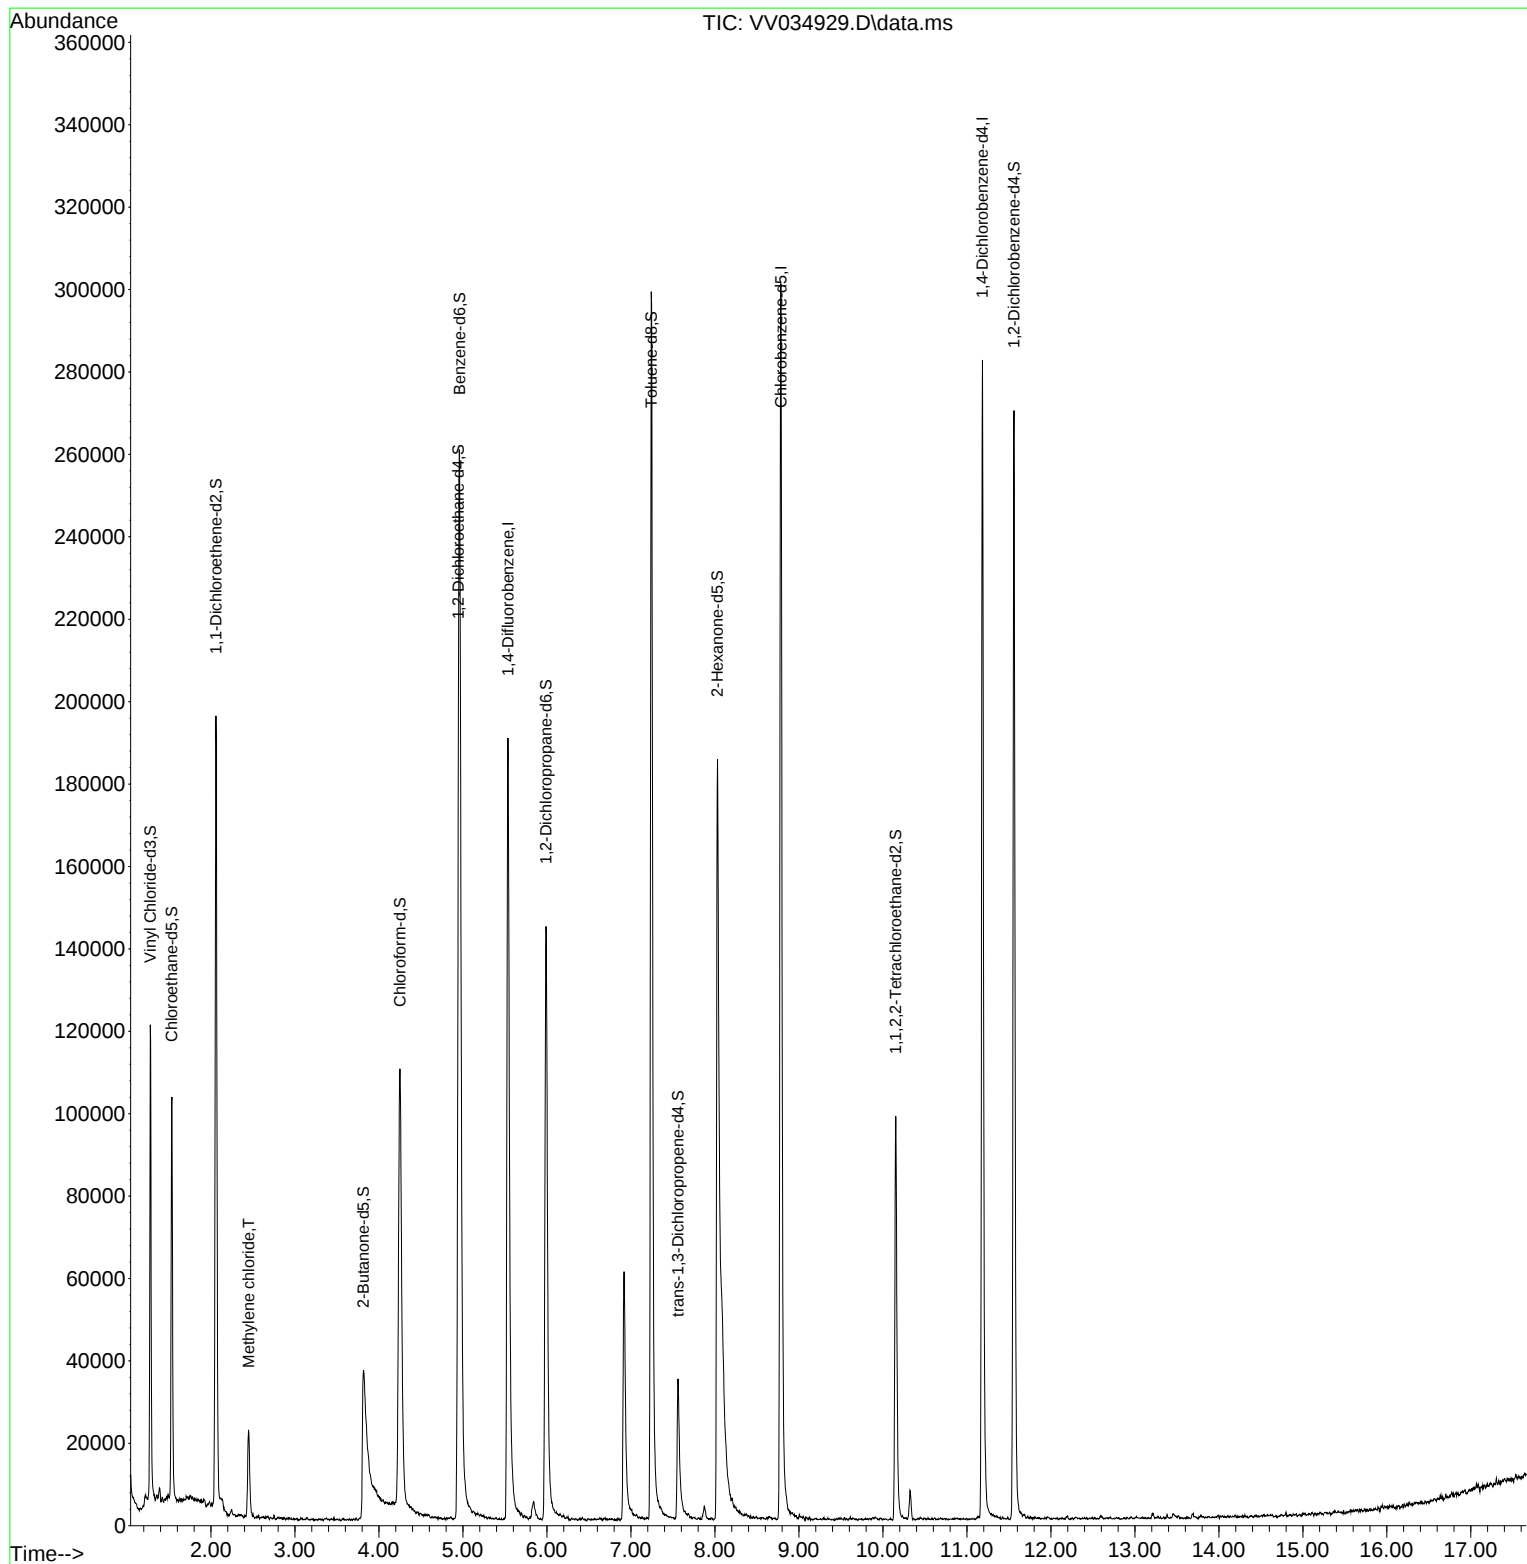

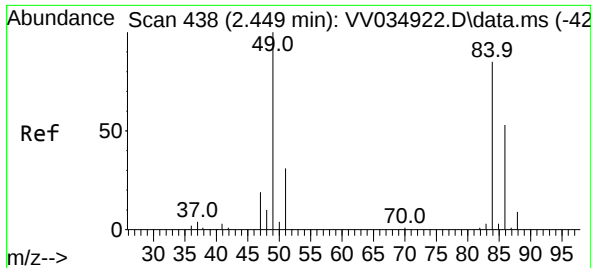

#16
Methylene chloride
Concen: 0.639 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV034929.D
Acq: 02 Apr 2024 13:34

Instrument :
MSVOA_V
ClientSampleId :
FB(20240327)

Tgt Ion: 84 Resp: 9021

Ion	Ratio	Lower	Upper
84	100		
86	61.7	43.5	80.9
49	124.3	82.5	153.3

