

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
 Data File : VV034931.D
 Acq On : 02 Apr 2024 15:12
 Operator : SY/MD
 Sample : P1925-25
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 FB(20240328)

Quant Time: Apr 03 05:20:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 03 05:08:19 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	167663	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	166758	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	71675	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	69464	5.027	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.600%	
7) Chloroethane-d5		1.532	69	60397	5.302	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.000%	
11) 1,1-Dichloroethene-d2		2.060	65	32303	5.147	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.000%	
20) 2-Butanone-d5		3.841	46	104161	48.179	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.360%	
24) Chloroform-d		4.249	84	114059	5.101	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%	
26) 1,2-Dichloroethane-d4		4.947	65	57304	5.675	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.600%	
32) Benzene-d6		4.960	84	232148	5.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.400%	
36) 1,2-Dichloropropane-d6		5.989	67	73202	5.718	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.400%	
41) Toluene-d8		7.243	98	196019	4.947	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%	
43) trans-1,3-Dichloroprop...		7.561	79	22722	4.996	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.000%	
46) 2-Hexanone-d5		8.030	63	81864	52.445	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.880%	
56) 1,1,2,2-Tetrachloroeth...		10.152	84	48216	5.397	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.000%	
66) 1,2-Dichlorobenzene-d4		11.561	152	64174	5.684	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.600%	
Target Compounds							
16) Methylene chloride		2.449	84	6482	0.464	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
Data File : VV034931.D
Acq On : 02 Apr 2024 15:12
Operator : SY/MD
Sample : P1925-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
FB(20240328)


Quant Time: Apr 03 05:20:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 03 05:08:19 2024
Response via : Initial Calibration

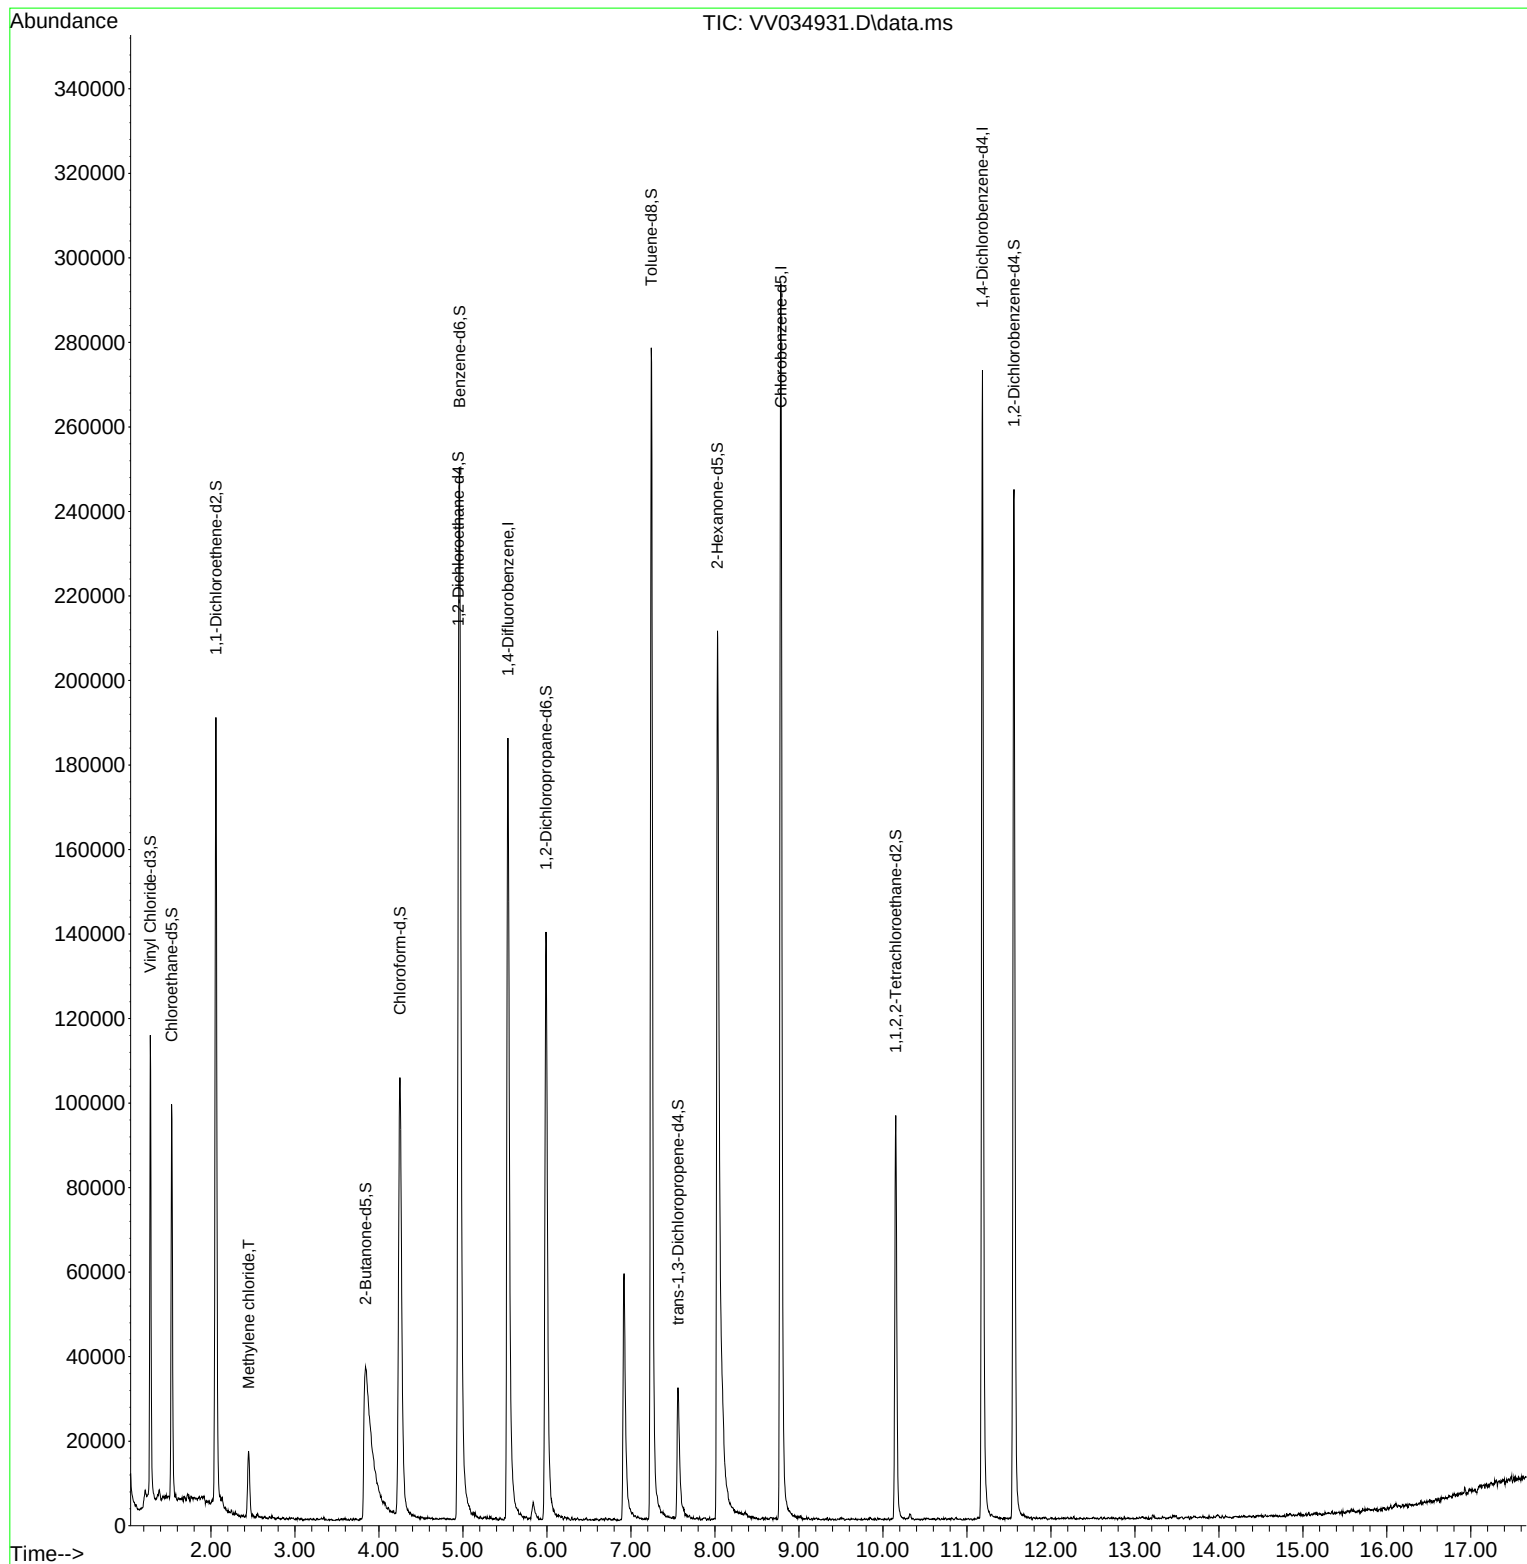

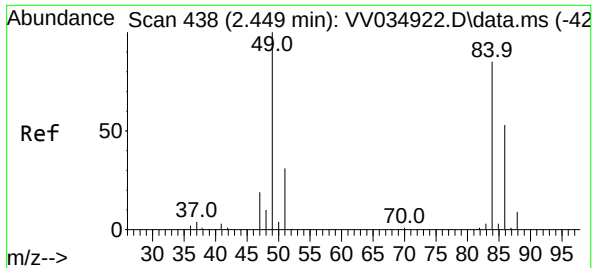

#16
Methylene chloride
Concen: 0.464 ug/L
RT: 2.449 min Scan# 41
Delta R.T. -0.000 min
Lab File: VV034931.D
Acq: 02 Apr 2024 15:12

Instrument :
MSVOA_V
ClientSampleId :
FB(20240328)

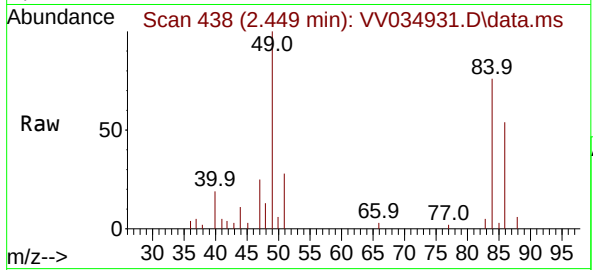

Tgt Ion:	84	Resp:	6482
Ion	Ratio	Lower	Upper
84	100		
86	71.7	43.5	80.9
49	132.3	82.5	153.3

