
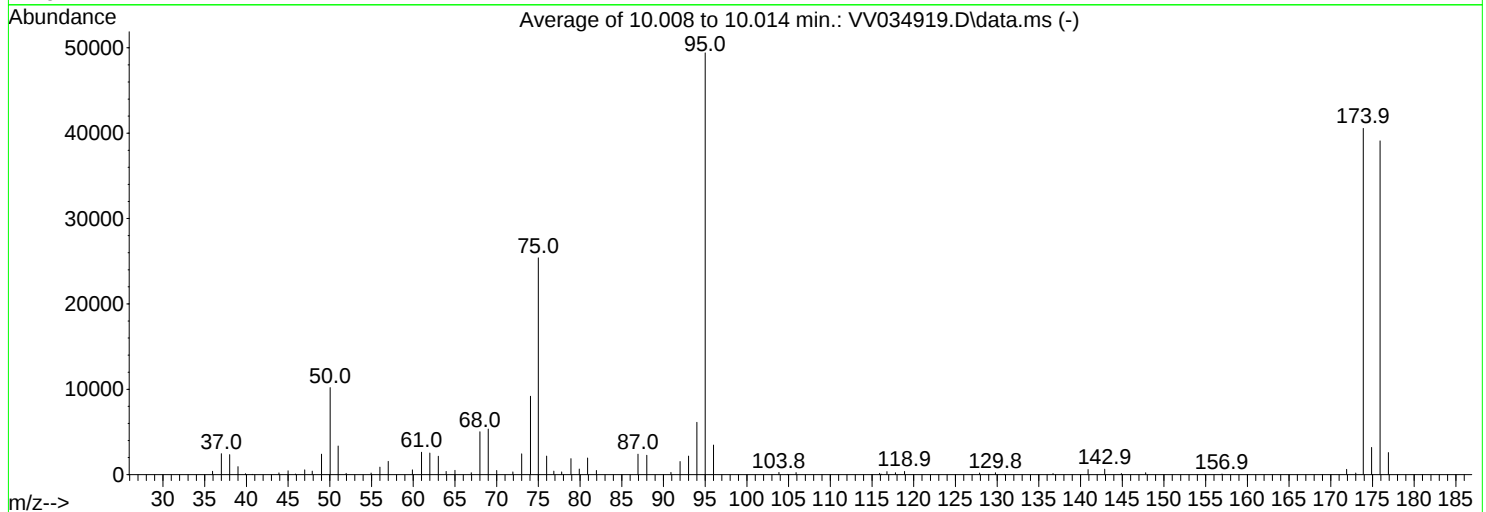


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040224\
Data File : VV034919.D
Acq On : 02 Apr 2024 08:21
Operator : SY/MD
Sample : BFB264
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB264

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 04 02:49:59 2024

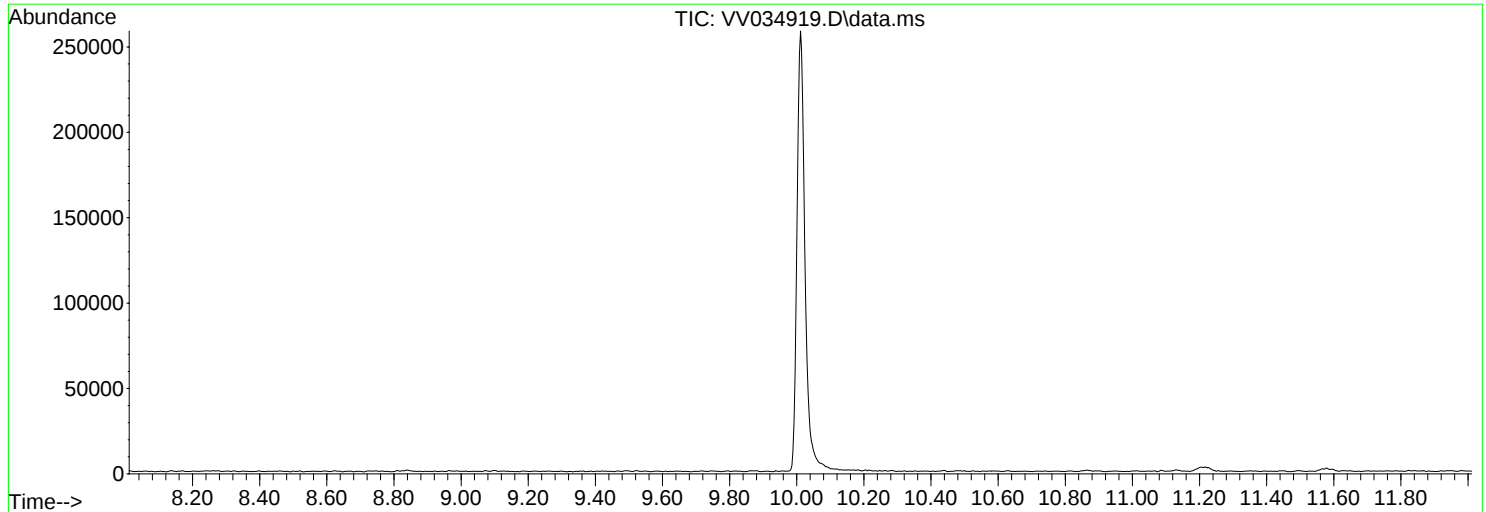

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	10190	PASS
75	95	30	80	51.4	25392	PASS
95	95	100	100	100.0	49411	PASS
96	95	5	9	7.0	3462	PASS
173	174	0.00	2	0.5	193	PASS
174	95	50	120	82.1	40571	PASS
175	174	5	9	7.8	3178	PASS
176	174	95	105	96.4	39099	PASS
177	176	5	10	6.6	2591	PASS

m/z	Abundance
40.00	1086.0
44.00	526.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	408.0
37.00	2461.0
38.00	2376.0
39.00	980.0
39.90	1197.0
43.90	802.0
45.00	451.0
47.10	557.0
47.90	371.0
49.00	2381.0
50.00	10204.0
51.00	3480.0
52.00	150.0
55.00	166.0
56.00	872.0
57.00	1487.0
59.90	486.0
61.00	2704.0
62.00	2584.0
63.00	2113.0
64.00	370.0
65.00	464.0
67.00	215.0
68.00	5099.0
69.00	5421.0
70.00	483.0
72.00	368.0
73.00	2343.0
74.00	9337.0
75.00	25616.0
76.00	2169.0
76.90	392.0
77.80	284.0
78.90	1825.0
79.90	611.0
80.90	1879.0
81.90	498.0
86.90	2392.0
88.00	2134.0
90.90	233.0
92.00	1510.0
93.00	2078.0
94.00	6032.0
95.00	48560.0
96.00	3331.0
103.80	229.0
104.90	102.0
105.90	200.0
115.90	249.0
116.80	317.0
117.80	248.0
118.90	340.0
127.90	174.0
129.80	242.0
136.70	128.0
140.90	550.0
142.90	669.0
144.90	122.0
147.80	212.0
171.90	598.0
173.00	578.0
173.90	38712.0
174.90	2967.0
175.90	36648.0
176.90	2524.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	392.0
37.00	2559.0
38.00	2425.0
39.00	946.0
39.90	1224.0
40.70	102.0
43.90	745.0
45.00	463.0
45.90	123.0
47.00	543.0
47.90	431.0
49.00	2514.0
50.00	10535.0
51.00	3448.0
51.90	152.0
54.90	186.0
56.00	936.0
57.00	1604.0
59.90	580.0
61.00	2679.0
62.00	2604.0
63.00	2213.0
64.00	385.0
65.00	516.0
66.90	233.0
68.00	5144.0
69.00	5491.0
70.00	520.0
71.90	326.0
73.00	2522.0
74.00	9407.0
75.00	26160.0
76.00	2267.0
76.90	438.0
77.80	332.0
78.90	1927.0
79.90	647.0
80.90	1986.0
81.90	485.0
87.00	2460.0
88.00	2390.0
90.90	276.0
92.00	1603.0
93.00	2197.0
94.00	6335.0
95.00	51120.0
96.00	3600.0
103.80	283.0
105.90	236.0
115.90	189.0
116.80	369.0
117.80	218.0
118.90	399.0
127.90	201.0
129.80	222.0
130.90	101.0
136.70	145.0
140.90	631.0
142.90	672.0
144.90	120.0
147.80	244.0
157.00	114.0
171.90	628.0
173.90	41840.0
174.90	3360.0
175.90	40520.0
176.90	2658.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
36.00	377.0
37.00	2345.0
38.00	2224.0
39.00	914.0
39.90	1178.0
43.90	670.0
45.00	447.0
45.90	131.0
46.90	581.0
47.90	428.0
49.00	2316.0
50.10	9831.0
51.00	3126.0
51.90	140.0
54.90	197.0
56.00	829.0
57.00	1558.0
59.90	602.0
61.00	2497.0
62.00	2397.0
63.00	2127.0
63.90	373.0
65.00	513.0
67.00	217.0
68.00	4828.0
69.00	5109.0
70.00	459.0
71.90	284.0
73.00	2436.0
74.10	8791.0
75.00	24400.0
76.00	2072.0
76.80	401.0
77.80	331.0
78.90	1894.0
79.90	686.0
80.90	1981.0
82.00	474.0
87.00	2346.0
88.00	2268.0
90.90	253.0
92.00	1508.0
93.00	2233.0
94.00	6019.0
95.00	48552.0
96.00	3456.0
103.90	274.0
105.90	295.0
116.10	166.0
116.80	363.0
117.80	197.0
118.90	399.0
127.90	185.0
129.00	106.0
129.80	193.0
136.70	127.0
140.90	621.0
142.90	591.0
144.90	132.0
147.80	203.0
154.90	111.0
156.90	100.0
171.90	637.0
173.90	41160.0
174.90	3208.0
175.90	40128.0
176.90	2591.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264