


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040419\
 Data File : VV010106.D
 Acq On : 04 Apr 2019 10:54
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.00G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Title : VOC Analysis
 Last Update : Thu Apr 04 06:01:11 2019

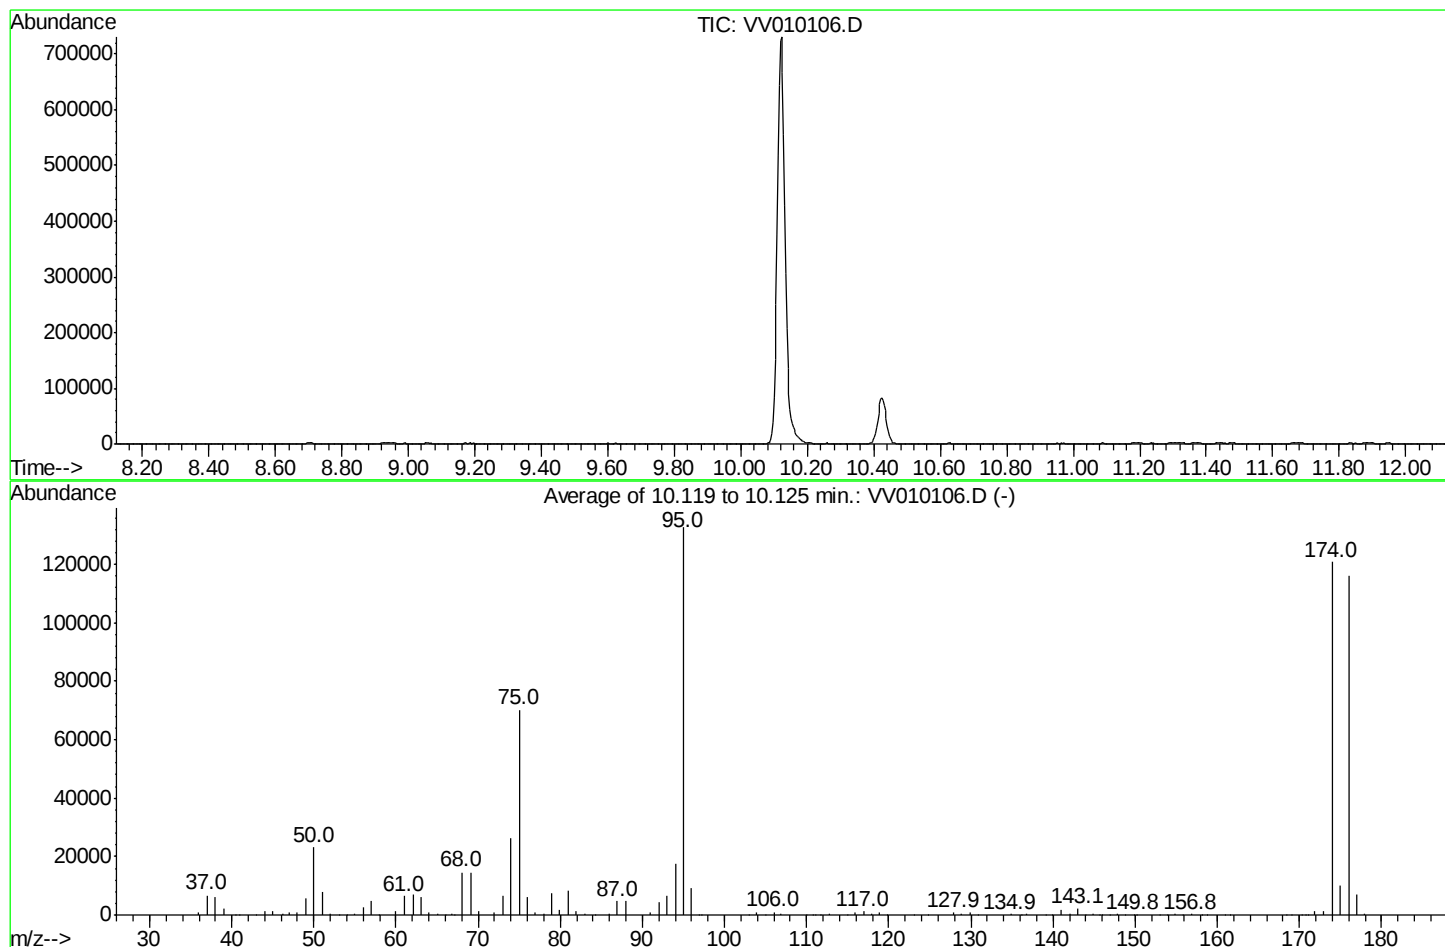

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23162	PASS
75	95	30	80	52.8	70093	PASS
95	95	100	100	100.0	132653	PASS
96	95	5	9	7.1	9372	PASS
173	174	0.00	2	1.1	1376	PASS
174	95	50	120	91.1	120856	PASS
175	174	5	9	8.2	9882	PASS
176	174	95	101	95.9	115914	PASS
177	176	5	9	6.0	7005	PASS