


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040419\
Data File : VV010117.D
Acq On : 04 Apr 2019 18:43
Operator : SY/MD
Sample : K2215-19
Misc : 5.41G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF2P9

Manual Integrations
APPROVED

MMDadoda
4/5/2019 3:25:36 PM

Quant Time: Apr 05 02:25:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 01:26:41 2019
Response via : Initial Calibration

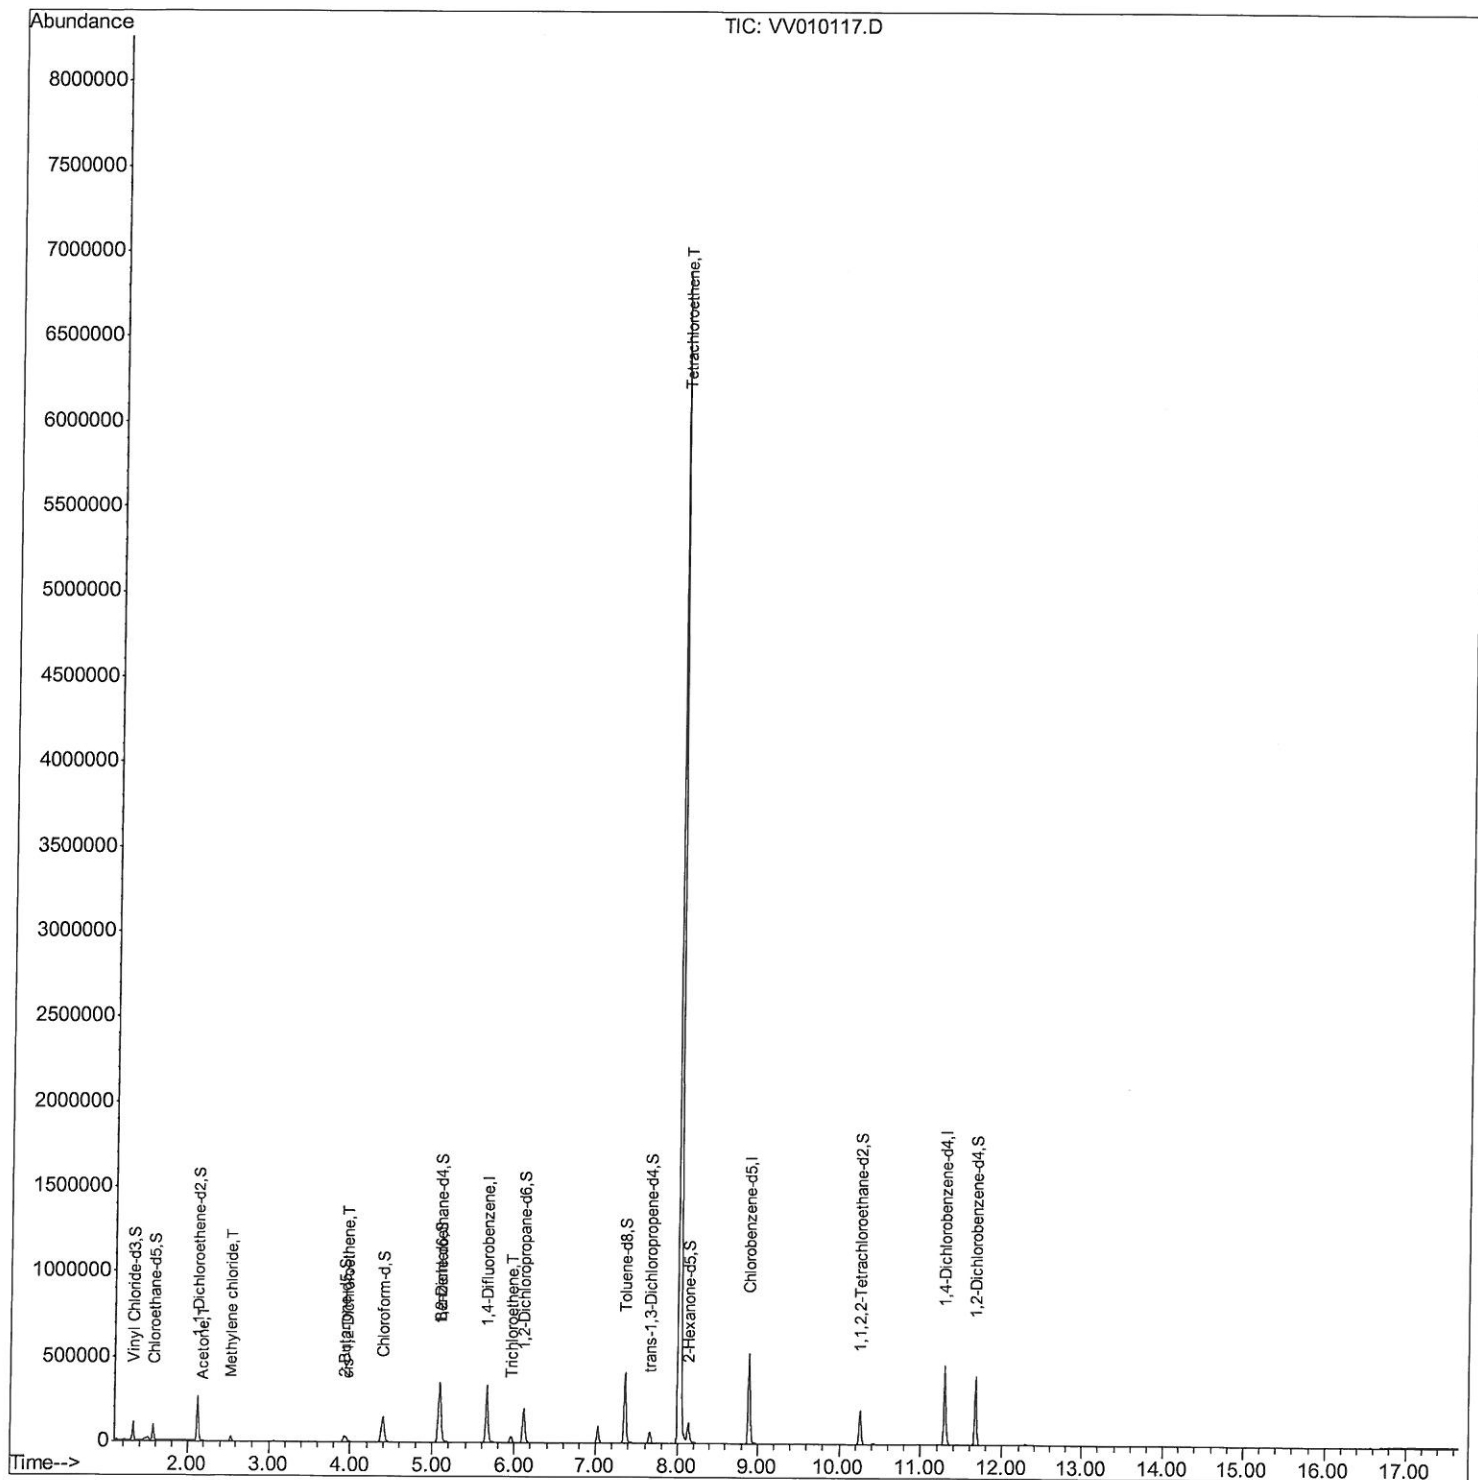


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040419\
Data File : VV010117.D
Acq On : 04 Apr 2019 18:43
Operator : SY/MD
Sample : K2215-19
Misc : 5.41G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF2P9

Manual Integrations
APPROVED

MMDadoda
4/5/2019 3:25:36 PM

Quant Time: Apr 05 01:31:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 01:26:41 2019
Response via : Initial Calibration

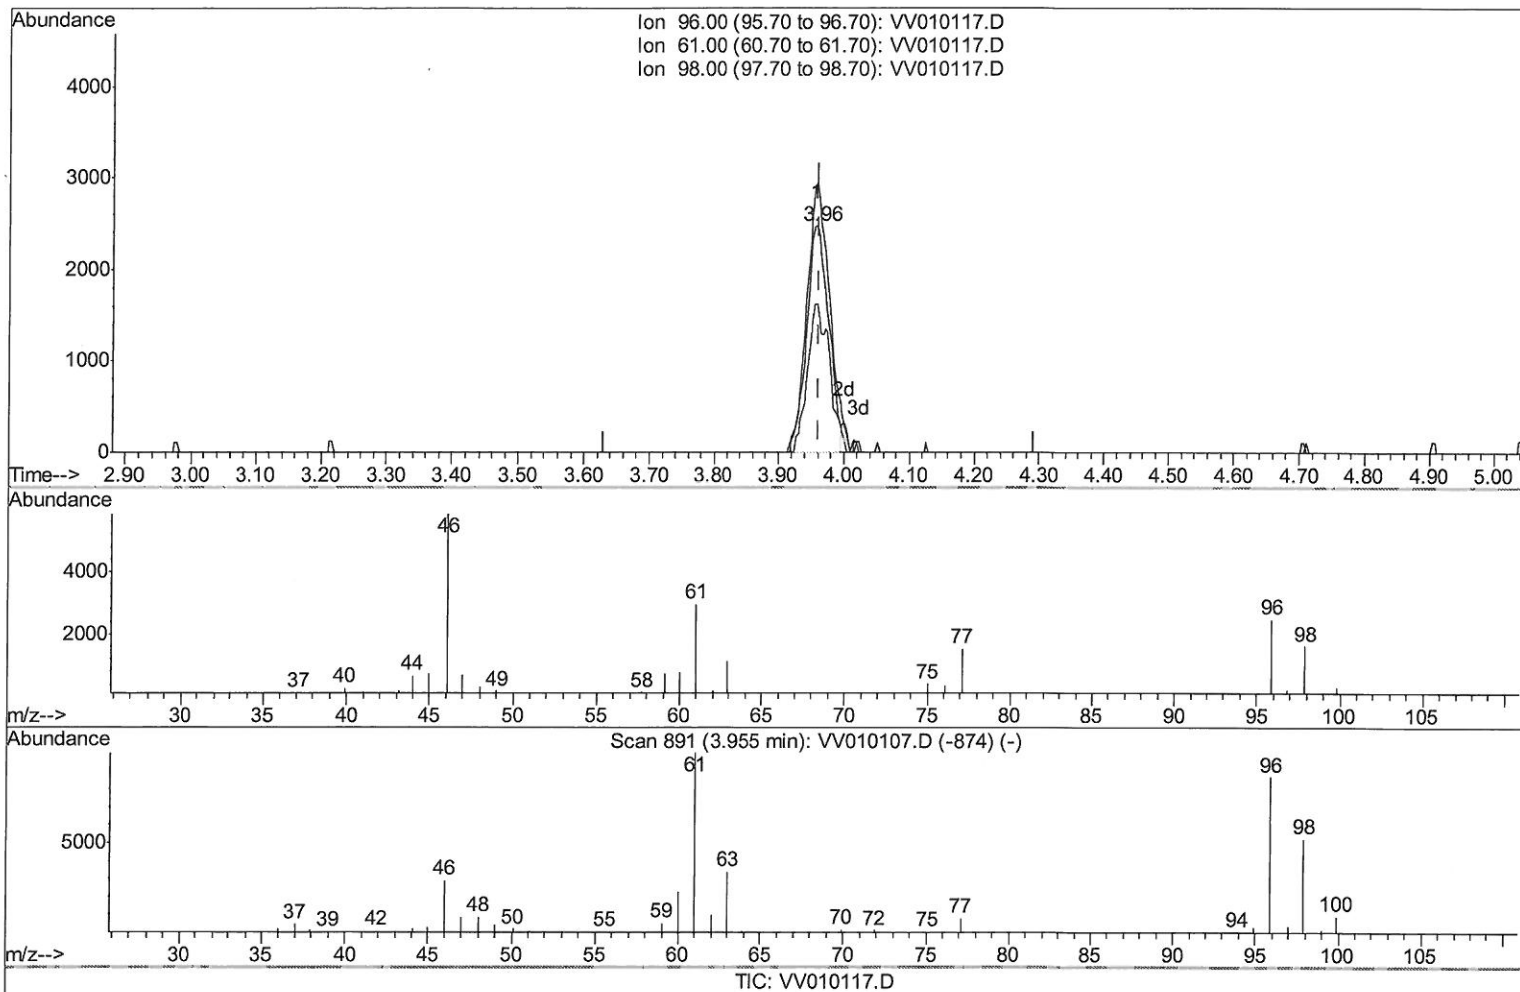

(22) cis-1,2-Dichloroethene (T)

3.958min (-0.003) 1.48ug/L

response 5832

Ion	Exp%	Act%
96.00	100	100
61.00	118.10	119.14
98.00	62.70	65.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040419\
Data File : VV010117.D
Acq On : 04 Apr 2019 18:43
Operator : SY/MD
Sample : K2215-19
Misc : 5.41G/10mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BF2P9

Manual Integrations
APPROVED

MMDadoda
4/5/2019 3:25:36 PM

Quant Time: Apr 05 01:31:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 05 01:26:41 2019
Response via : Initial Calibration

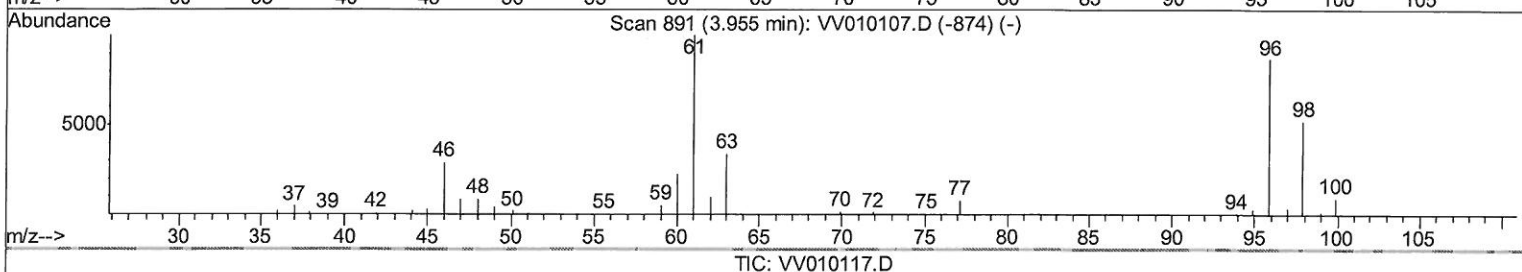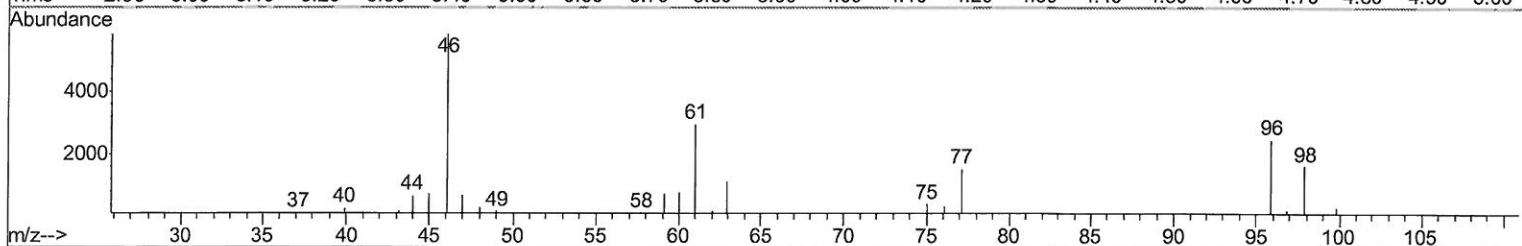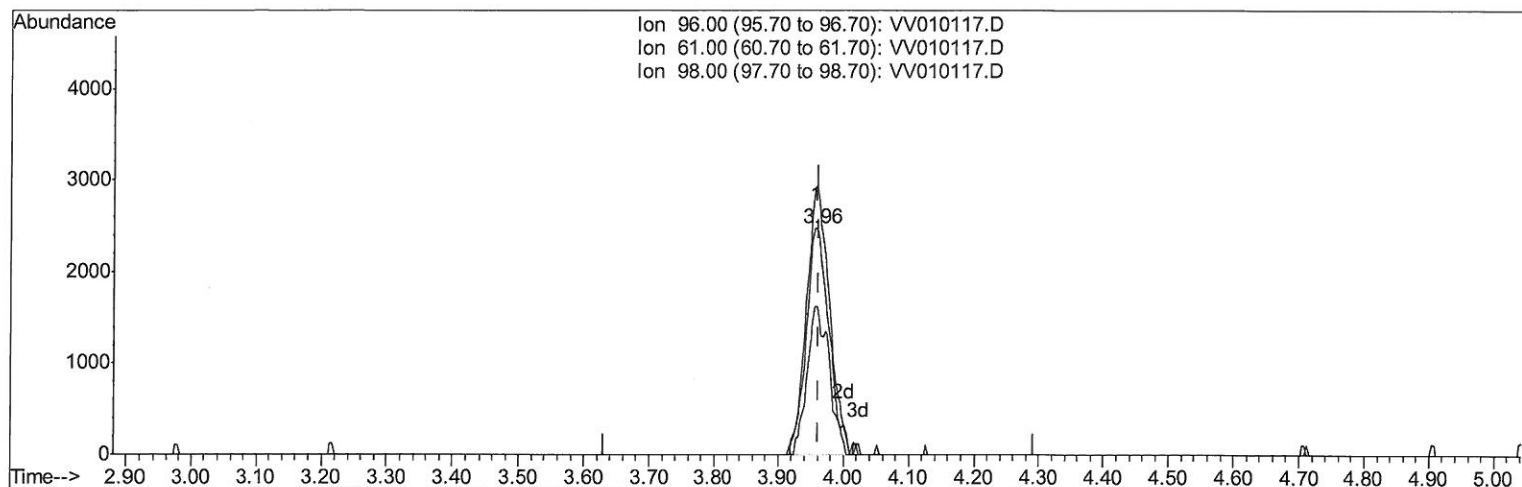

TIC: VV010117.D

(22) cis-1,2-Dichloroethene (T)

3.958min (-0.003) 1.53ug/L m

response 6023

Ion	Exp%	Act%
96.00	100	100
61.00	118.10	119.14
98.00	62.70	65.67
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV040419\
 Data File : VV010117.D
 Acq On : 04 Apr 2019 18:43
 Operator : SY/MD
 Sample : K2215-19
 Misc : 5.41G/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BF2P9

Manual Integrations
 APPROVED

MMDadoda
 4/5/2019 3:25:36 PM

Quant Time: Apr 05 02:25:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 05 01:26:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	296339	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	302069	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	128052	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	61846	15.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.36%
7) Chloroethane-d5	1.57	69	64383	13.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.28%
10) 1,1-Dichloroethene-d2	2.12	63	131997	13.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.76%
20) 2-Butanone-d5	3.93	46	48444	42.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.82%
24) Chloroform-d	4.40	84	144965	19.42	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.68%
26) 1,2-Dichloroethane-d4	5.08	65	91337	21.87	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.48%
29) Benzene-d6	5.10	84	310490	19.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.28%
33) 1,2-Dichloropropane-d6	6.12	67	94606	20.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.84%
37) Toluene-d8	7.36	98	286434	18.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.92%
38) trans-1,3-Dichloropropene-	7.66	79	34103	17.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.04%
39) 2-Hexanone-d5	8.13	63	37848	40.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.64%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	91364	20.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.16%
61) 1,2-Dichlorobenzene-d4	11.67	152	107864	21.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.48%

Target Compounds

					Qvalue
13) Acetone	2.19	43	4329	3.879	ug/L 86
16) Methylene chloride	2.53	84	11340	2.178	ug/L 94
22) cis-1,2-Dichloroethene	3.96	96	6023m	1.533	ug/L
35) Trichloroethene	5.96	95	10134	2.383	ug/L 95
47) Tetrachloroethene	8.02	164	1452235	408.055	ug/L 96

7 MLO
 4/7/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed