


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040419\
 Data File : VV010106.D
 Acq On : 04 Apr 2019 10:54
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.00G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
 Title : VOC Analysis
 Last Update : Fri Apr 05 01:26:41 2019

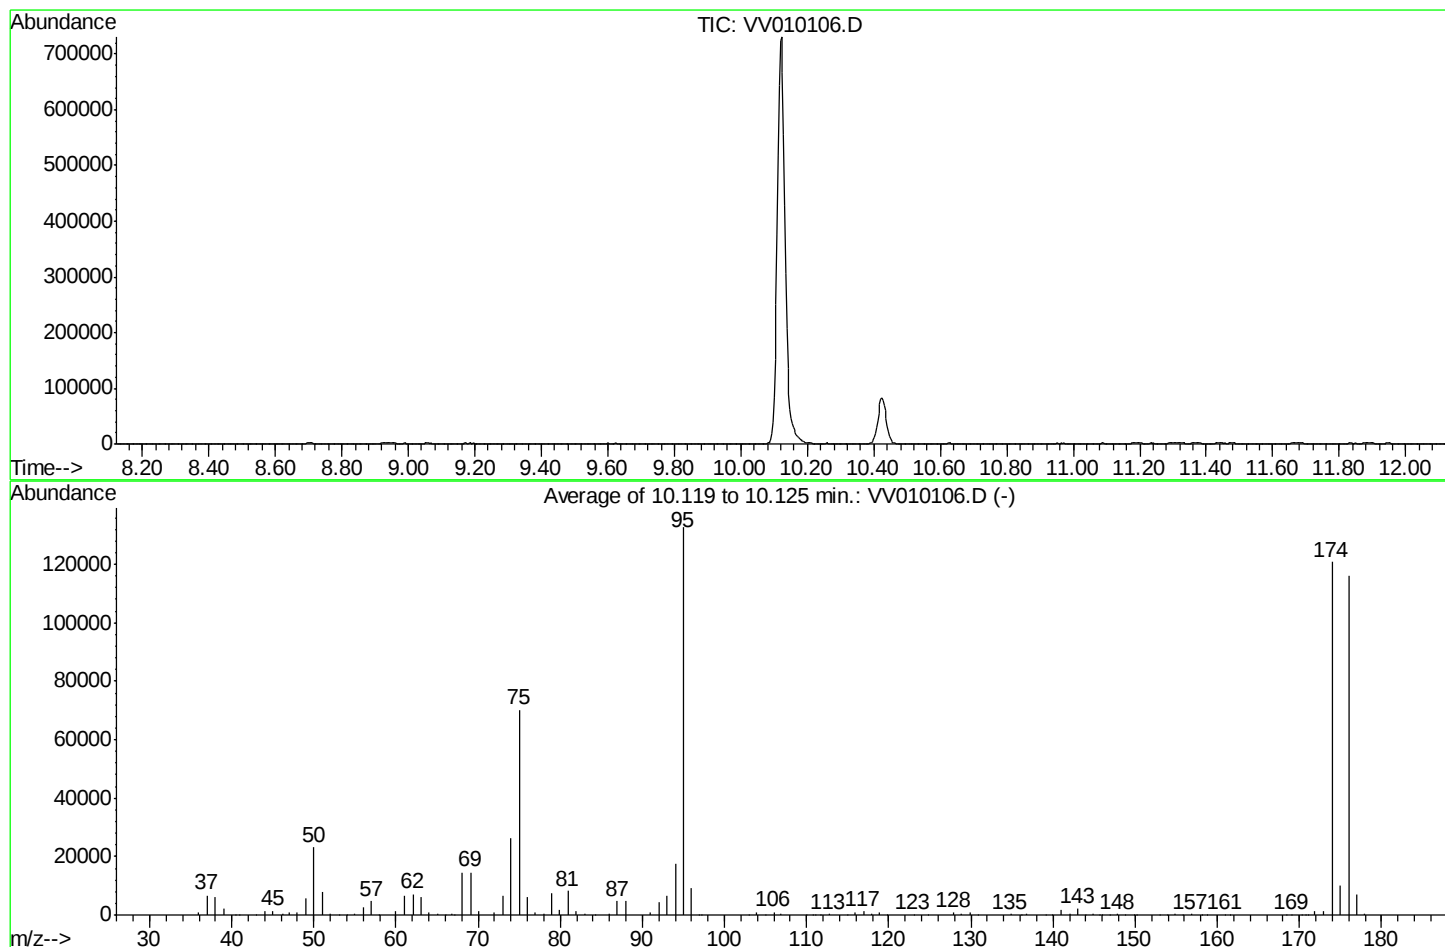

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	23162	PASS
75	95	30	80	52.8	70093	PASS
95	95	100	100	100.0	132653	PASS
96	95	5	9	7.1	9372	PASS
173	174	0.00	2	1.1	1376	PASS
174	95	50	120	91.1	120856	PASS
175	174	5	9	8.2	9882	PASS
176	174	95	101	95.9	115914	PASS
177	176	5	9	6.0	7005	PASS

Scan 2795 (10.077 min): VV010106.D
BFB84

m/z	Abundance
36.00	105.0
38.70	101.0
40.00	201.0
41.20	108.0
44.00	313.0
169.20	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1114.0
37.00	6909.0
38.00	6305.0
39.00	2677.0
40.00	192.0
40.50	108.0
40.90	101.0
43.00	159.0
44.00	1450.0
45.00	1295.0
46.20	282.0
47.00	1104.0
47.90	817.0
49.00	5978.0
50.00	24032.0
51.00	8323.0
52.00	412.0
54.00	138.0
54.90	513.0
56.00	3135.0
57.00	4791.0
57.90	209.0
60.00	1445.0
61.00	6539.0
62.00	7462.0
63.00	6362.0
63.90	714.0
65.00	585.0
66.80	296.0
67.10	287.0
68.00	15224.0
69.00	14992.0
70.10	1361.0
72.00	978.0
73.00	6816.0
74.00	27288.0
75.00	72512.0
76.00	6168.0
76.90	711.0
78.00	474.0
79.00	7826.0
79.90	2056.0
80.90	8253.0
81.90	1578.0
82.90	229.0
84.20	123.0
85.90	316.0
87.00	4992.0
88.00	4880.0
91.00	996.0
92.00	4605.0
93.00	6641.0
94.00	18408.0
95.00	137408.0
96.00	9196.0
96.90	265.0
103.90	1013.0
105.00	224.0
106.00	963.0
106.80	260.0
110.00	255.0
110.70	131.0
111.10	191.0
112.80	304.0
115.00	106.0
115.80	834.0
116.90	1293.0
117.80	580.0
118.90	1015.0
119.80	129.0
123.00	122.0
124.80	115.0
127.90	757.0
128.90	366.0
130.00	723.0
130.80	282.0
134.90	338.0
136.80	332.0
139.10	116.0
139.90	139.0
140.90	1906.0
142.00	385.0
143.10	1923.0
144.00	150.0
144.90	405.0
145.70	268.0
146.00	264.0
146.90	145.0
147.90	337.0
148.80	125.0
150.10	103.0
153.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

154.00	176.0
154.90	336.0
156.80	374.0
158.80	211.0
160.90	209.0
161.50	124.0
169.10	200.0
170.30	204.0
171.00	330.0
171.80	1303.0
173.00	2055.0
174.00	119496.0
175.00	10641.0
176.00	117016.0
177.00	7162.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	1138.0
37.00	6816.0
38.00	6446.0
39.10	2407.0
40.00	191.0
40.50	143.0
40.90	133.0
42.90	137.0
44.00	1495.0
45.00	1444.0
46.20	391.0
47.00	1110.0
47.90	829.0
49.00	5856.0
50.00	23720.0
51.00	8064.0
51.90	353.0
53.10	123.0
55.00	433.0
56.00	2917.0
57.00	4784.0
58.00	255.0
60.00	1565.0
61.00	6468.0
62.10	7275.0
63.00	6251.0
63.90	740.0
65.00	513.0
66.90	331.0
68.00	14977.0
69.00	15034.0
70.10	1342.0
72.00	990.0
73.00	7059.0
74.00	27360.0
75.00	72216.0
76.00	6332.0
76.90	826.0
78.00	459.0
78.90	7604.0
79.90	2076.0
80.90	8407.0
81.90	1531.0
83.00	276.0
84.20	160.0
85.90	277.0
87.00	4780.0
87.90	4713.0
91.00	971.0
92.00	4644.0
93.00	6713.0
94.00	18088.0
95.00	137472.0
96.00	9781.0
96.90	238.0
102.90	101.0
103.90	934.0
106.00	976.0
106.80	271.0
110.00	238.0
111.10	234.0
111.70	119.0
112.80	307.0
115.90	740.0
116.90	1197.0
117.80	656.0
118.90	992.0
127.90	802.0
128.80	352.0
129.90	747.0
130.80	213.0
134.90	429.0
136.10	135.0
136.80	342.0
139.90	228.0
141.00	1799.0
142.00	402.0
143.00	2108.0
144.00	168.0
144.80	361.0
145.60	208.0
146.00	207.0
146.90	185.0
147.90	324.0
153.90	157.0
154.80	353.0
156.80	395.0
158.10	132.0
158.80	245.0
161.00	168.0
168.40	101.0
169.10	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

171.00	313.0
171.90	1406.0
173.00	2073.0
174.00	125480.0
175.00	10156.0
176.00	119800.0
177.00	7172.0
177.90	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	1012.0
37.00	6275.0
38.00	6097.0
39.10	2093.0
39.90	196.0
40.50	164.0
40.90	132.0
42.90	123.0
44.00	1503.0
45.00	1362.0
46.10	403.0
47.00	1049.0
47.90	705.0
49.00	5305.0
50.00	21736.0
51.00	6952.0
52.00	238.0
53.10	143.0
55.00	497.0
56.00	2427.0
57.00	4292.0
58.00	252.0
60.00	1498.0
61.00	6229.0
62.10	6550.0
63.00	5417.0
63.90	699.0
64.90	340.0
66.00	121.0
66.90	343.0
68.00	13421.0
69.10	13659.0
70.00	1242.0
72.00	876.0
73.00	6470.0
74.00	24264.0
75.00	65552.0
76.10	6024.0
76.90	897.0
78.00	438.0
78.90	6872.0
79.90	1843.0
80.90	7701.0
81.90	1407.0
82.90	278.0
84.20	103.0
85.90	209.0
86.90	4452.0
87.90	4358.0
91.00	812.0
92.00	4225.0
93.00	5978.0
94.00	16274.0
95.00	123080.0
96.00	9139.0
96.90	163.0
97.20	130.0
104.00	839.0
104.80	170.0
106.00	862.0
106.90	201.0
110.00	186.0
111.00	206.0
111.70	124.0
112.70	231.0
115.90	661.0
117.00	1132.0
117.90	642.0
118.80	953.0
127.90	714.0
128.70	280.0
129.80	792.0
130.90	157.0
134.90	446.0
136.10	117.0
136.80	407.0
139.90	278.0
141.00	1661.0
142.00	304.0
143.00	2066.0
144.00	150.0
144.70	263.0
145.50	153.0
146.00	130.0
146.90	197.0
147.90	300.0
149.80	121.0
153.80	171.0
154.80	323.0
155.80	128.0
156.80	348.0
158.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

158.80	221.0
161.00	157.0
168.30	143.0
169.10	203.0
170.10	103.0
170.70	248.0
171.90	1285.0
174.00	117592.0
175.00	8850.0
176.00	110928.0
177.00	6683.0
177.90	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84