




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:21:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 05 01:21:20 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/05/2022
Supervised By :Mahesh Dadoda 04/05/2022

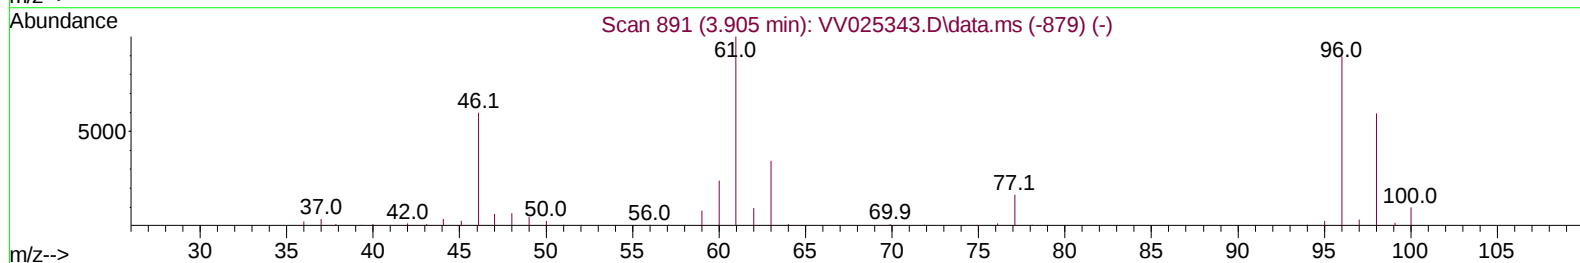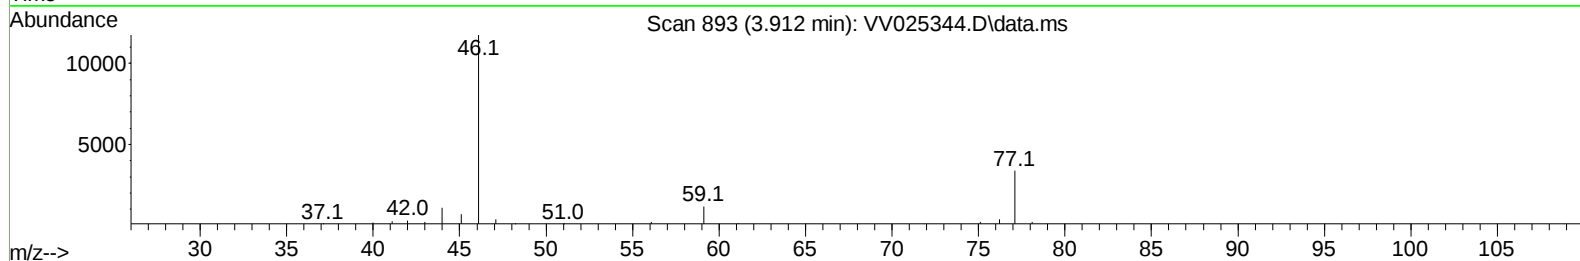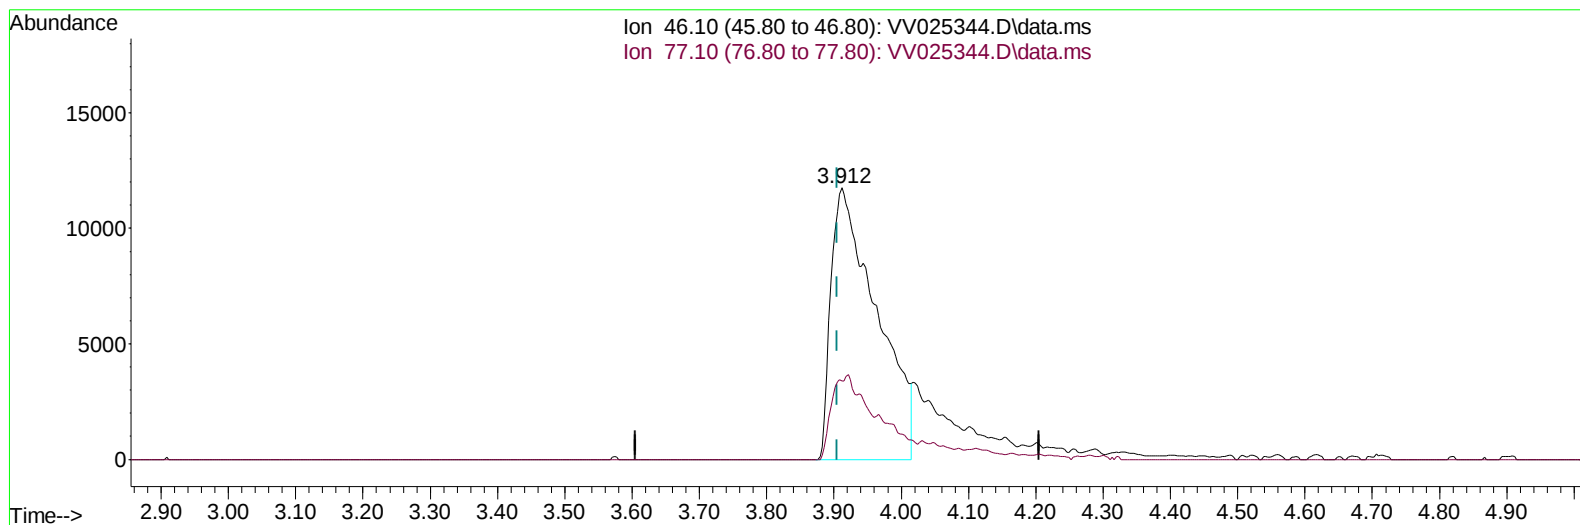

TIC: VV025344.D\data.ms

(20) 2-Butanone-d5 (S)

3.912min (+ 0.006) 34.72 ug/L

response 55201

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	22.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:21:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 05 01:21:20 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/05/2022
Supervised By :Mahesh Dadoda 04/05/2022

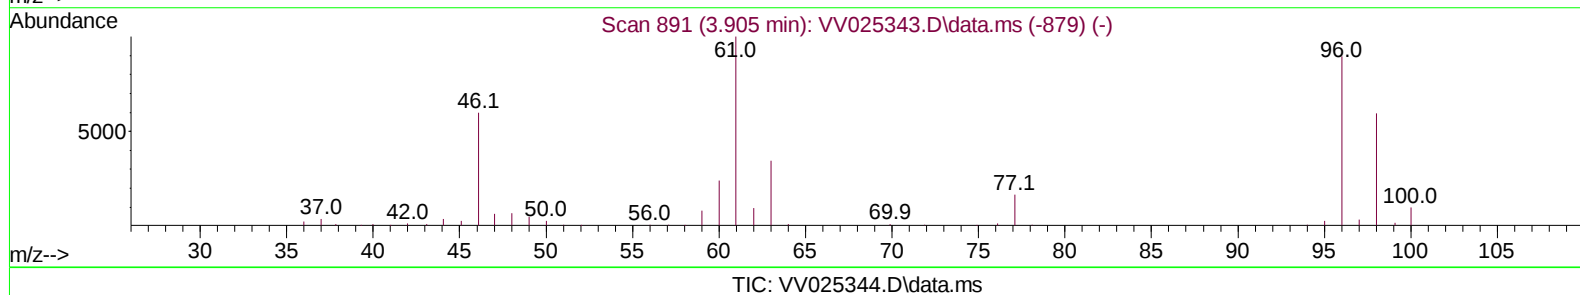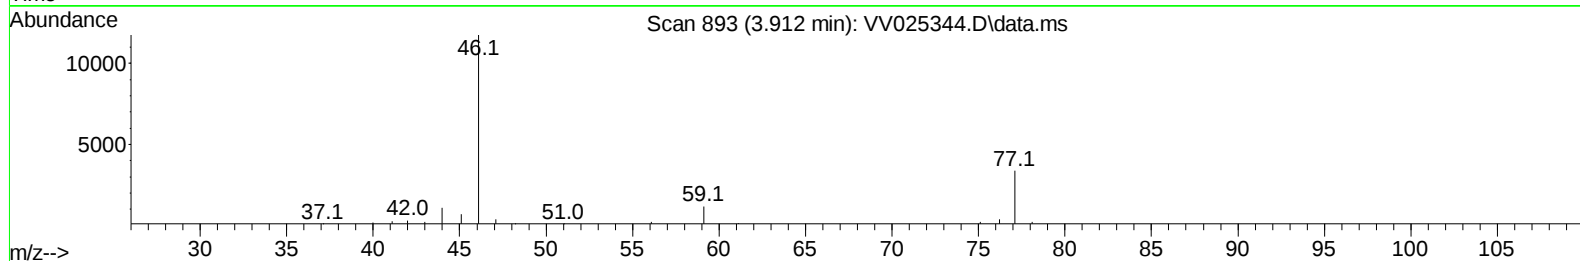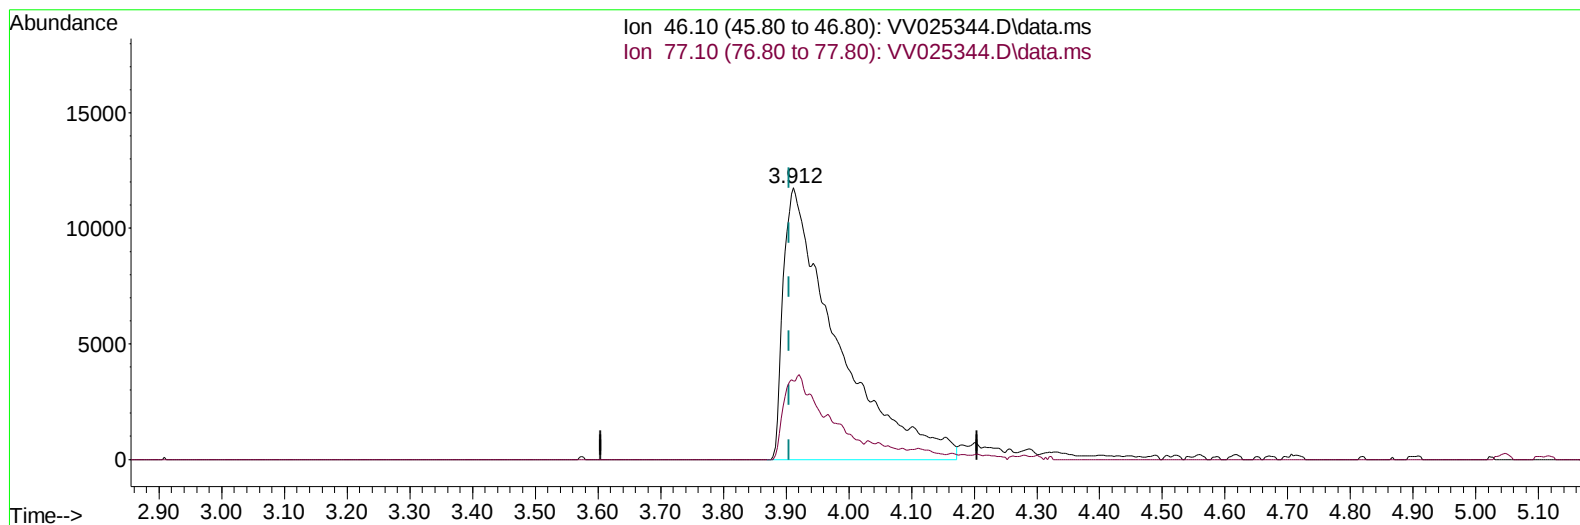

(20) 2-Butanone-d5 (S)

3.912min (+ 0.006) 43.95 ug/L m

response 69878

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.90	17.46
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
 Data File : VV025344.D
 Acq On : 04 Apr 2022 11:54
 Operator : SY/MD
 Sample : VV0404WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK333

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 04/05/2022
 Supervised By : Mahesh Dadoda 04/05/2022

Quant Time: Apr 05 01:21:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 05 01:21:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	170879	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	159147	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	66256	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	63592	3.984	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	79.600%		
7) Chloroethane-d5	1.568	69	56729	4.235	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	84.600%		
11) 1,1-Dichloroethene-d2	2.105	63	111094	3.213	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.200%		
20) 2-Butanone-d5	3.912	46	69878m	43.950	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	87.900%		
24) Chloroform-d	4.342	84	87715	4.211	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.200%		
26) 1,2-Dichloroethane-d4	5.027	65	38827	4.217	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	84.400%		
32) Benzene-d6	5.043	84	166759	4.142	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	82.800%		
36) 1,2-Dichloropropane-d6	6.066	67	49387	4.377	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	87.600%		
41) Toluene-d8	7.313	98	140550	3.806	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	76.200%		
43) trans-1,3-Dichloroprop...	7.622	79	14671	3.986	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	79.800%		
46) 2-Hexanone-d5	8.088	63	52526	39.509	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	79.020%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32446	4.312	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	86.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	46132	4.335	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	86.800%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:21:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 05 01:21:20 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/05/2022
Supervised By :Mahesh Dadoda 04/05/2022

