

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
 Data File : VV025344.D
 Acq On : 04 Apr 2022 11:54
 Operator : SY/MD
 Sample : VV0404WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK333

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rVB	100732	108051	23.23%	2.740%
2	1.568	156	164	176	rVB	92748	103123	22.17%	2.615%
3	2.105	320	331	353	rVB	215285	321411	69.09%	8.151%
4	2.506	447	456	466	rVB3	5565	9457	2.03%	0.240%
5	3.912	881	893	908	rBV2	20457	71065	15.28%	1.802%
6	4.342	1011	1027	1050	rBV	81291	206193	44.32%	5.229%
7	5.043	1228	1245	1280	rBV2	176199	447582	96.21%	11.351%
8	5.612	1409	1422	1450	rBV	189035	386368	83.05%	9.799%
9	5.908	1505	1514	1525	rBV7	2982	6257	1.35%	0.159%
10	6.066	1550	1563	1587	rBV2	99055	206856	44.47%	5.246%
11	6.985	1834	1849	1870	rBV2	41673	83625	17.98%	2.121%
12	7.313	1939	1951	1969	rBV	203325	362570	77.94%	9.195%
13	7.622	2038	2047	2068	rBV	24159	44925	9.66%	1.139%
14	8.088	2182	2192	2223	rBV	135582	302068	64.93%	7.661%
15	8.850	2417	2429	2455	rBV	281814	465196	100.00%	11.798%
16	10.214	2843	2853	2867	rBV	68203	109603	23.56%	2.780%
17	11.246	3164	3174	3196	rBV	259346	400523	86.10%	10.158%
18	11.622	3278	3291	3309	rBV	185088	296673	63.77%	7.524%
19	12.246	3476	3485	3496	rVB2	3335	5922	1.27%	0.150%
20	14.040	4032	4043	4051	rBV2	3256	5648	1.21%	0.143%




Sum of corrected areas: 3943116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

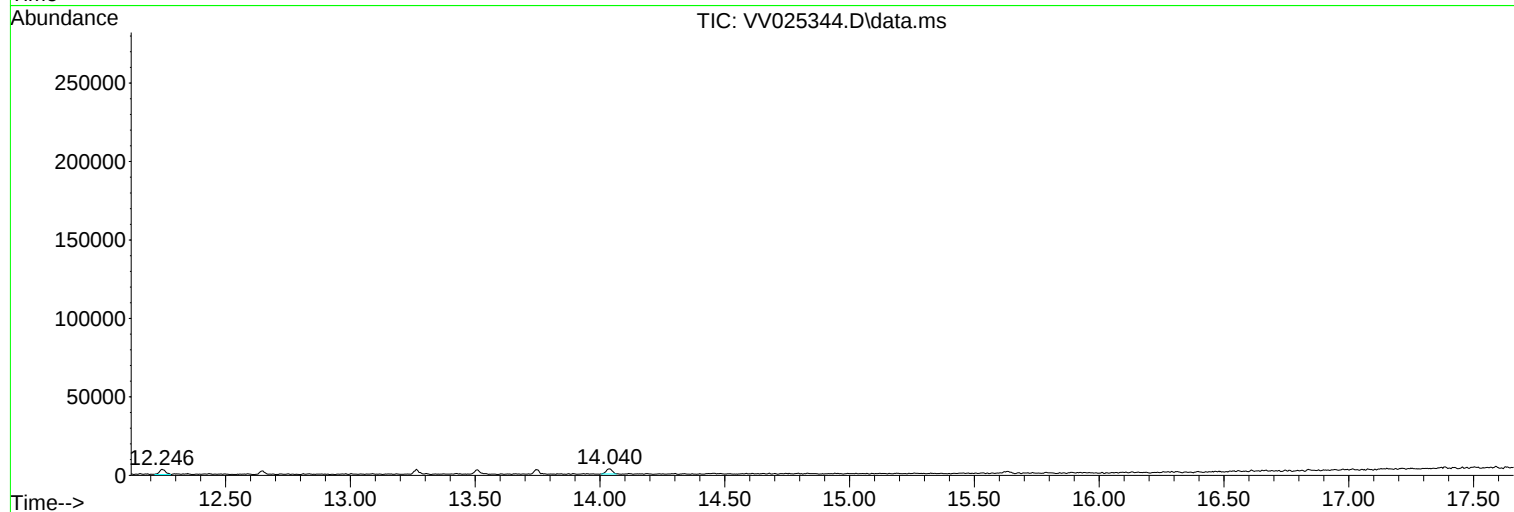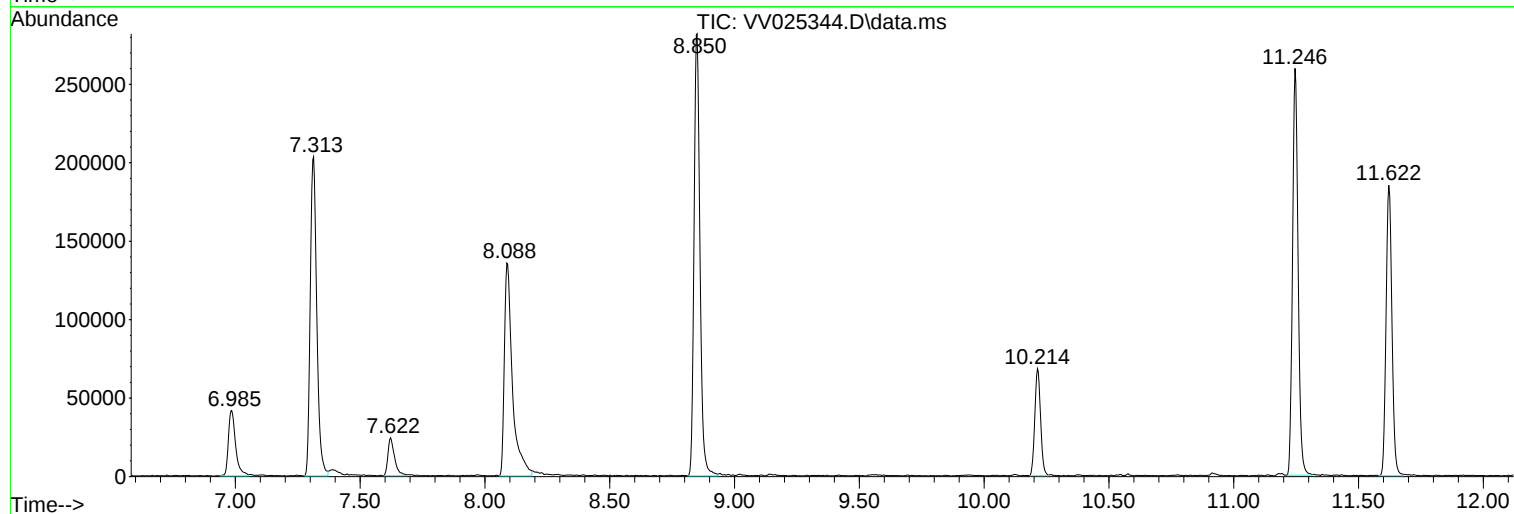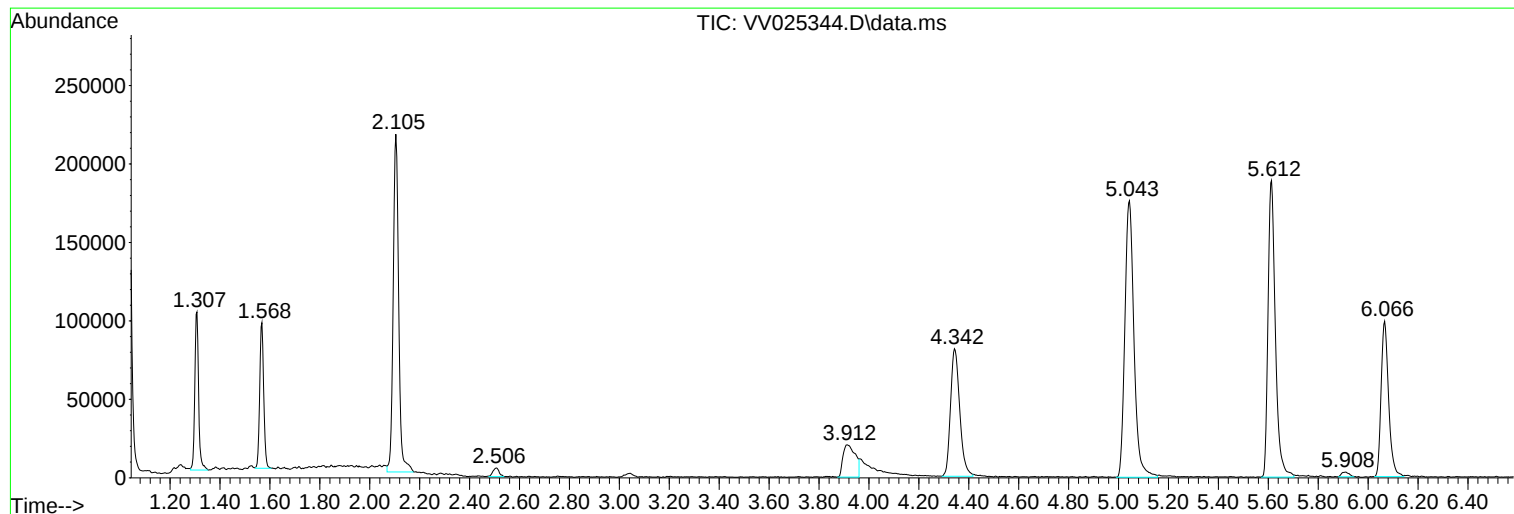

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025344.D
Acq On : 04 Apr 2022 11:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
