

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
 Data File : VV025345.D
 Acq On : 04 Apr 2022 12:26
 Operator : SY/MD
 Sample : N2165-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rVB	91924	93587	23.54%	2.789%
2	1.568	155	164	175	rBV	82088	93861	23.61%	2.797%
3	2.105	321	331	354	rVB	169024	257165	64.70%	7.664%
4	2.506	447	456	467	rBV3	5843	9744	2.45%	0.290%
5	3.912	882	893	894	rBV	16901	22102	5.56%	0.659%
6	4.346	1012	1028	1053	rBV3	72188	187563	47.19%	5.590%
7	5.043	1228	1245	1279	rBV4	158482	397502	100.00%	11.846%
8	5.612	1405	1422	1444	rBV	146678	301077	75.74%	8.972%
9	5.911	1505	1515	1527	rVB5	3321	6907	1.74%	0.206%
10	6.066	1550	1563	1584	rBV2	87850	189212	47.60%	5.639%
11	6.985	1839	1849	1863	rBV2	39495	71770	18.06%	2.139%
12	7.313	1939	1951	1973	rBV	182428	323536	81.39%	9.642%
13	7.622	2037	2047	2063	rBV3	20548	38992	9.81%	1.162%
14	8.088	2181	2192	2229	rBV2	118083	273879	68.90%	8.162%
15	8.850	2418	2429	2452	rBV	228804	376988	94.84%	11.235%
16	10.214	2841	2853	2873	rVB	61523	99680	25.08%	2.971%
17	11.246	3161	3174	3197	rBV	211965	329268	82.83%	9.812%
18	11.622	3280	3291	3311	rBV	172603	274383	69.03%	8.177%
19	12.246	3476	3485	3496	rVB2	2535	4172	1.05%	0.124%
20	14.040	4030	4043	4052	rBV2	2442	4235	1.07%	0.126%




Sum of corrected areas: 3355623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025345.D
Acq On : 04 Apr 2022 12:26
Operator : SY/MD
Sample : N2165-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

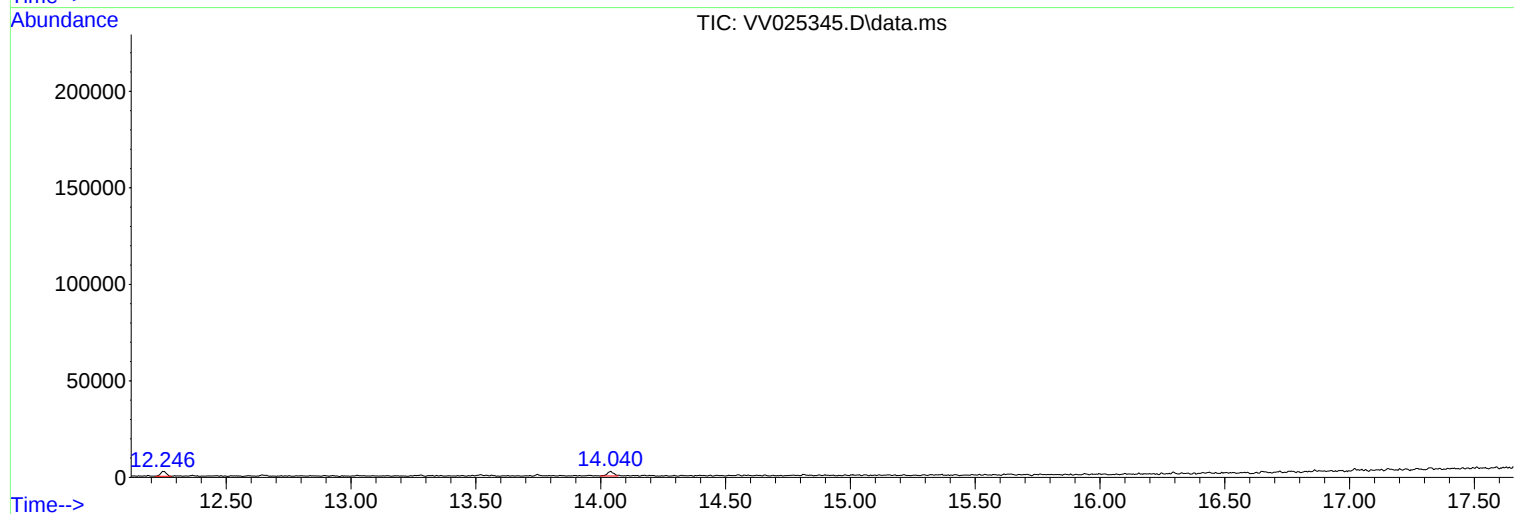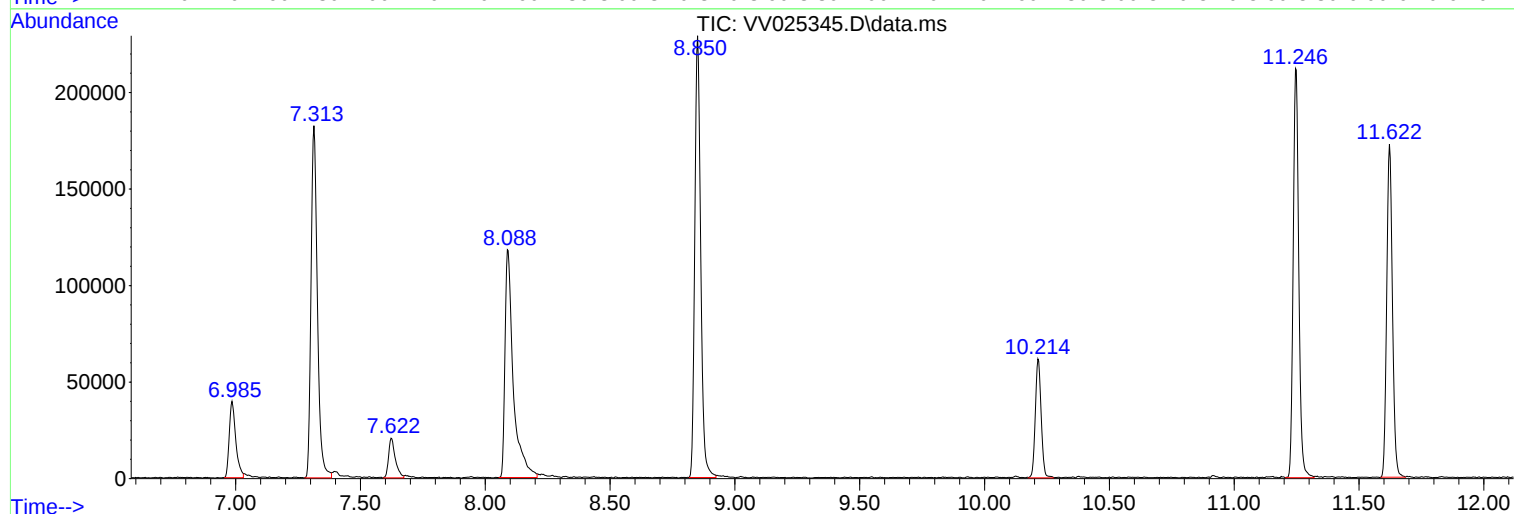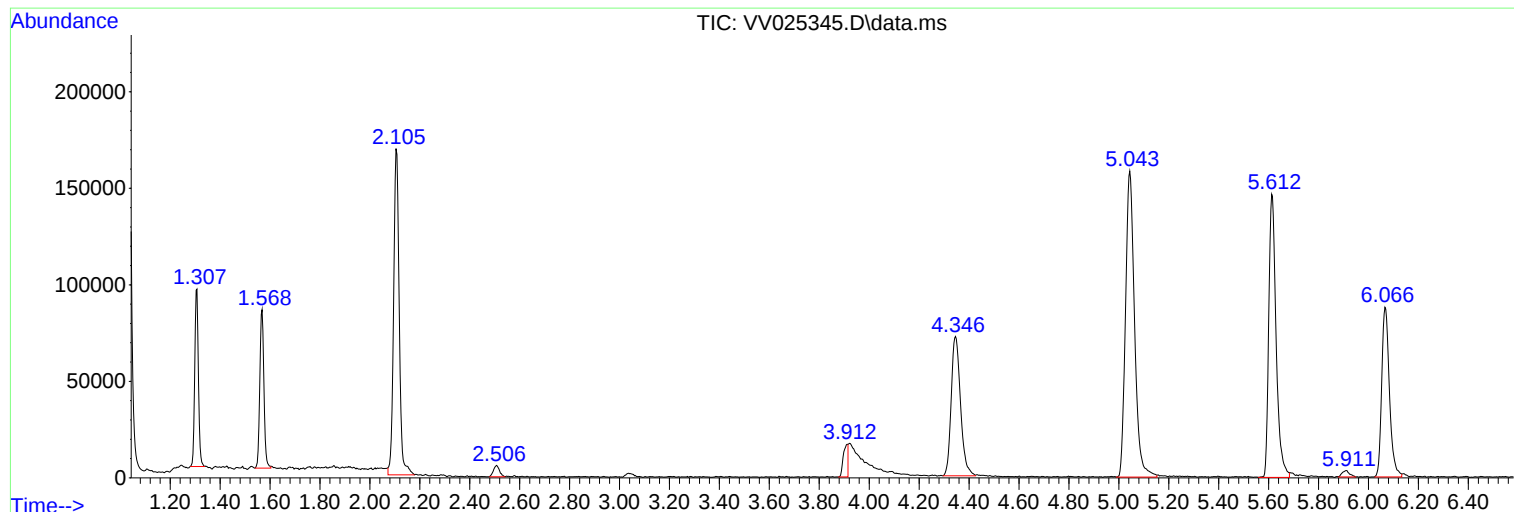

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025345.D
Acq On : 04 Apr 2022 12:26
Operator : SY/MD
Sample : N2165-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Methane, oxybis[chloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.985	1.19 ug/L	71770	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	53
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	47
3			Thiophosgene	114	CCl2S	000463-71-8	36
4			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	33
5			.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	28

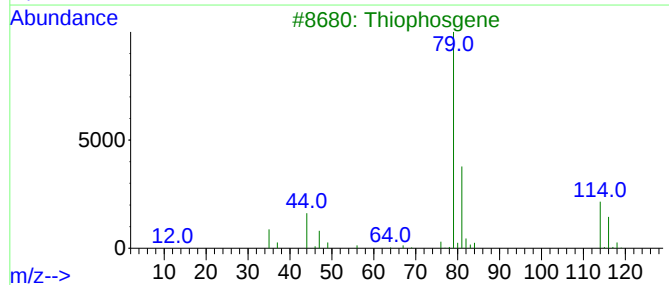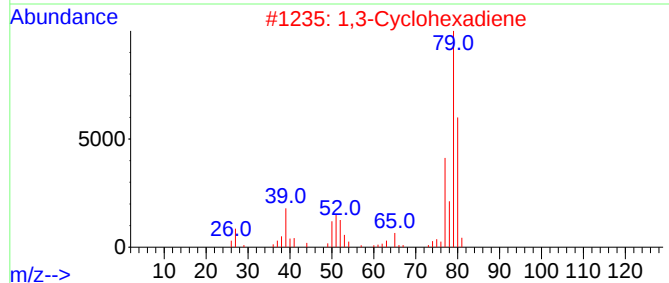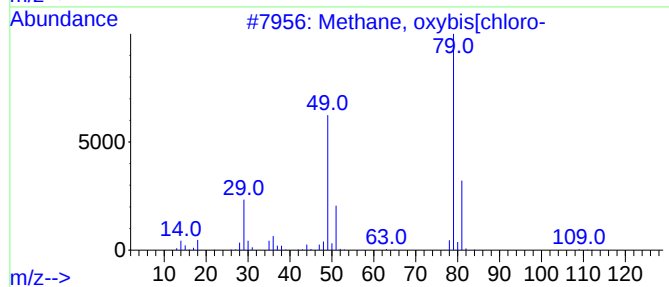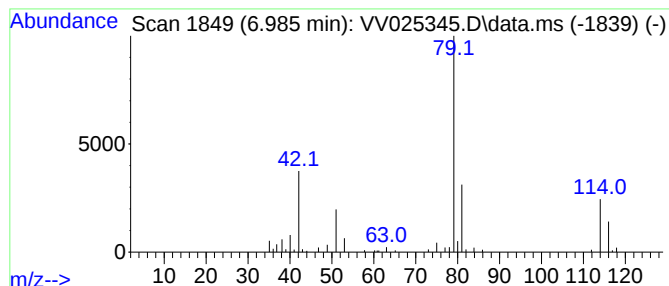

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025345.D
Acq On : 04 Apr 2022 12:26
Operator : SY/MD
Sample : N2165-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methane, oxybis...	6.985	1.2	ug/L	71770	1	5.616	301077	5.0