


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040422\
Data File : VV025342.D
Acq On : 04 Apr 2022 09:38
Operator : SY/MD
Sample : BFB294
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB294

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 05 01:21:20 2022

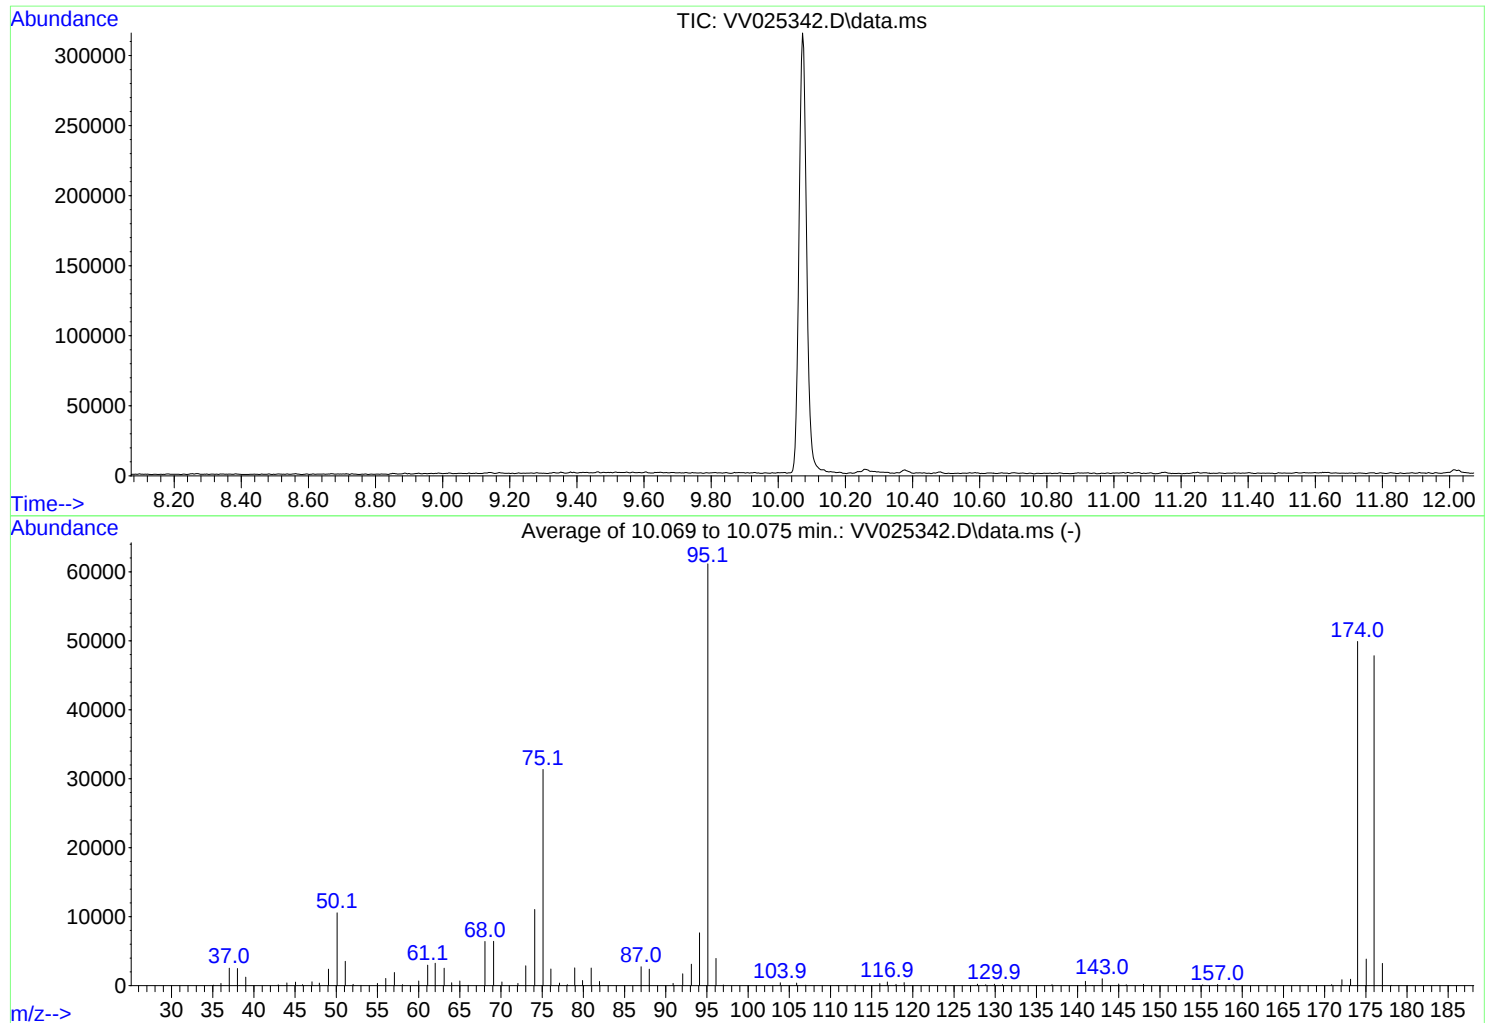

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10563	PASS
75	95	30	80	51.3	31349	PASS
95	95	100	100	100.0	61152	PASS
96	95	5	9	6.5	3953	PASS
173	174	0.00	2	1.9	936	PASS
174	95	50	120	81.6	49901	PASS
175	174	5	9	7.7	3842	PASS
176	174	95	105	95.9	47840	PASS
177	176	5	10	6.7	3223	PASS

Scan 2796 (10.030 min): VV025342.D\data.ms
BFB294

m/z	Abundance
36.10	692.0
38.00	281.0
40.00	686.0
44.00	476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
36.00	988.0
37.00	2494.0
38.00	2573.0
39.00	1278.0
40.00	587.0
43.00	120.0
44.00	804.0
45.10	555.0
45.90	121.0
47.10	544.0
47.90	383.0
49.10	2418.0
50.10	10141.0
51.10	3442.0
52.00	162.0
55.00	295.0
56.00	1120.0
57.10	1989.0
58.10	122.0
60.00	701.0
61.10	3023.0
62.00	3274.0
63.10	2566.0
64.00	439.0
65.00	596.0
66.00	117.0
68.00	6354.0
69.10	6377.0
70.10	561.0
72.10	322.0
73.00	2583.0
74.10	10809.0
75.10	31384.0
76.00	2355.0
77.10	370.0
78.00	222.0
79.00	2670.0
79.90	739.0
80.90	2613.0
81.90	535.0
87.00	2699.0
88.00	2392.0
90.90	349.0
92.10	1673.0
93.10	3132.0
94.10	7805.0
95.10	60552.0
96.10	3960.0
103.90	457.0
105.90	431.0
113.00	101.0
116.00	325.0
116.90	512.0
117.90	181.0
118.90	433.0
127.90	194.0
128.90	137.0
129.90	237.0
130.90	149.0
136.90	120.0
141.00	721.0
143.00	1017.0
145.00	231.0
145.90	156.0
148.00	179.0
154.80	164.0
157.00	166.0
158.90	135.0
170.70	147.0
172.10	895.0
173.10	877.0
174.00	50416.0
175.10	3746.0
176.00	48568.0
177.00	3344.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
36.00	1020.0
37.00	2628.0
38.10	2864.0
39.00	1285.0
40.00	630.0
42.90	123.0
44.00	865.0
45.10	531.0
45.90	145.0
47.00	577.0
47.90	402.0
49.00	2482.0
50.10	10938.0
51.10	3681.0
52.00	203.0
55.00	327.0
56.00	1091.0
57.00	1950.0
58.00	153.0
60.00	707.0
61.10	3081.0
62.00	3351.0
63.10	2571.0
64.00	429.0
65.00	711.0
68.00	6600.0
69.10	6674.0
70.10	575.0
72.10	322.0
73.00	2925.0
74.10	11485.0
75.10	32456.0
76.00	2488.0
77.10	376.0
78.10	217.0
78.90	2684.0
79.90	758.0
80.90	2593.0
82.00	628.0
87.00	2869.0
88.00	2397.0
90.90	319.0
92.00	1729.0
93.10	3210.0
94.10	7870.0
95.10	63296.0
96.10	4029.0
97.00	120.0
103.90	444.0
105.90	389.0
107.00	106.0
113.00	109.0
115.90	313.0
116.90	556.0
118.00	208.0
118.90	462.0
127.90	209.0
128.90	141.0
129.90	217.0
130.90	155.0
136.90	141.0
141.00	635.0
143.00	1043.0
145.00	230.0
145.90	142.0
148.00	191.0
155.20	168.0
157.00	176.0
158.90	136.0
170.80	142.0
172.10	889.0
173.10	984.0
174.00	51640.0
175.00	3927.0
176.00	49496.0
177.00	3370.0
178.10	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
35.10	206.0
36.00	1047.0
37.00	2486.0
38.10	2860.0
39.00	1122.0
40.00	635.0
42.90	124.0
44.00	915.0
45.00	467.0
45.90	151.0
47.00	552.0
48.00	361.0
49.00	2274.0
50.10	10609.0
51.10	3457.0
52.10	209.0
53.00	123.0
55.00	332.0
56.00	960.0
57.00	1747.0
58.00	140.0
60.00	646.0
61.10	2809.0
62.00	3128.0
63.10	2443.0
64.00	379.0
65.00	711.0
68.10	6280.0
69.10	6215.0
70.10	497.0
72.00	343.0
73.00	3096.0
74.10	10865.0
75.10	30208.0
76.10	2421.0
77.10	383.0
78.90	2396.0
79.90	707.0
81.00	2438.0
82.00	663.0
87.00	2678.0
88.00	2376.0
90.90	276.0
92.00	1719.0
93.10	3020.0
94.10	7290.0
95.10	59608.0
96.10	3870.0
97.00	154.0
103.90	340.0
105.90	330.0
107.00	117.0
110.80	101.0
116.10	252.0
116.90	517.0
118.00	201.0
119.00	416.0
127.80	231.0
128.80	113.0
129.90	210.0
130.90	142.0
136.90	132.0
140.90	506.0
141.80	102.0
143.00	960.0
145.00	231.0
145.90	133.0
148.00	176.0
155.20	188.0
157.00	168.0
158.90	111.0
171.00	137.0
172.10	766.0
173.20	947.0
174.00	47648.0
175.00	3853.0
176.00	45456.0
177.00	2956.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294