

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034970.D
 Acq On : 04 Apr 2024 11:59
 Operator : SY/MD
 Sample : P1893-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 04 21:35:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 04 21:33:57 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	407649	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	399927	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	172275	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	152655	38.776	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	77.560%	
7) Chloroethane-d5	1.532	69	159427	46.624	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	93.240%	
11) 1,1-Dichloroethene-d2	2.056	65	71260	41.292	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.580%	
21) 2-Butanone-d5	3.796	46	198480	85.006	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.010%	
24) Chloroform-d	4.246	84	291757	44.078	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.160%	
26) 1,2-Dichloroethane-d4	4.937	65	189225	45.027	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.060%	
32) Benzene-d6	4.957	84	586993	43.696	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.400%	
36) 1,2-Dichloropropane-d6	5.985	67	192706	45.174	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	90.340%	
41) Toluene-d8	7.239	98	508561	42.036	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	84.080%	
43) trans-1,3-Dichloroprop...	7.551	79	81074	39.094	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.180%	
47) 2-Hexanone-d5	8.027	63	120234	74.547	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	74.550%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	250277	42.604	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	85.200%	
66) 1,2-Dichlorobenzene-d4	11.558	152	185022	47.835	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.660%	
Target Compounds						
39) cis-1,3-Dichloropropene	6.908	75	4906	0.864	ug/L	Qvalue # 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034970.D
Acq On : 04 Apr 2024 11:59
Operator : SY/MD
Sample : P1893-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 04 21:35:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 21:33:57 2024
Response via : Initial Calibration

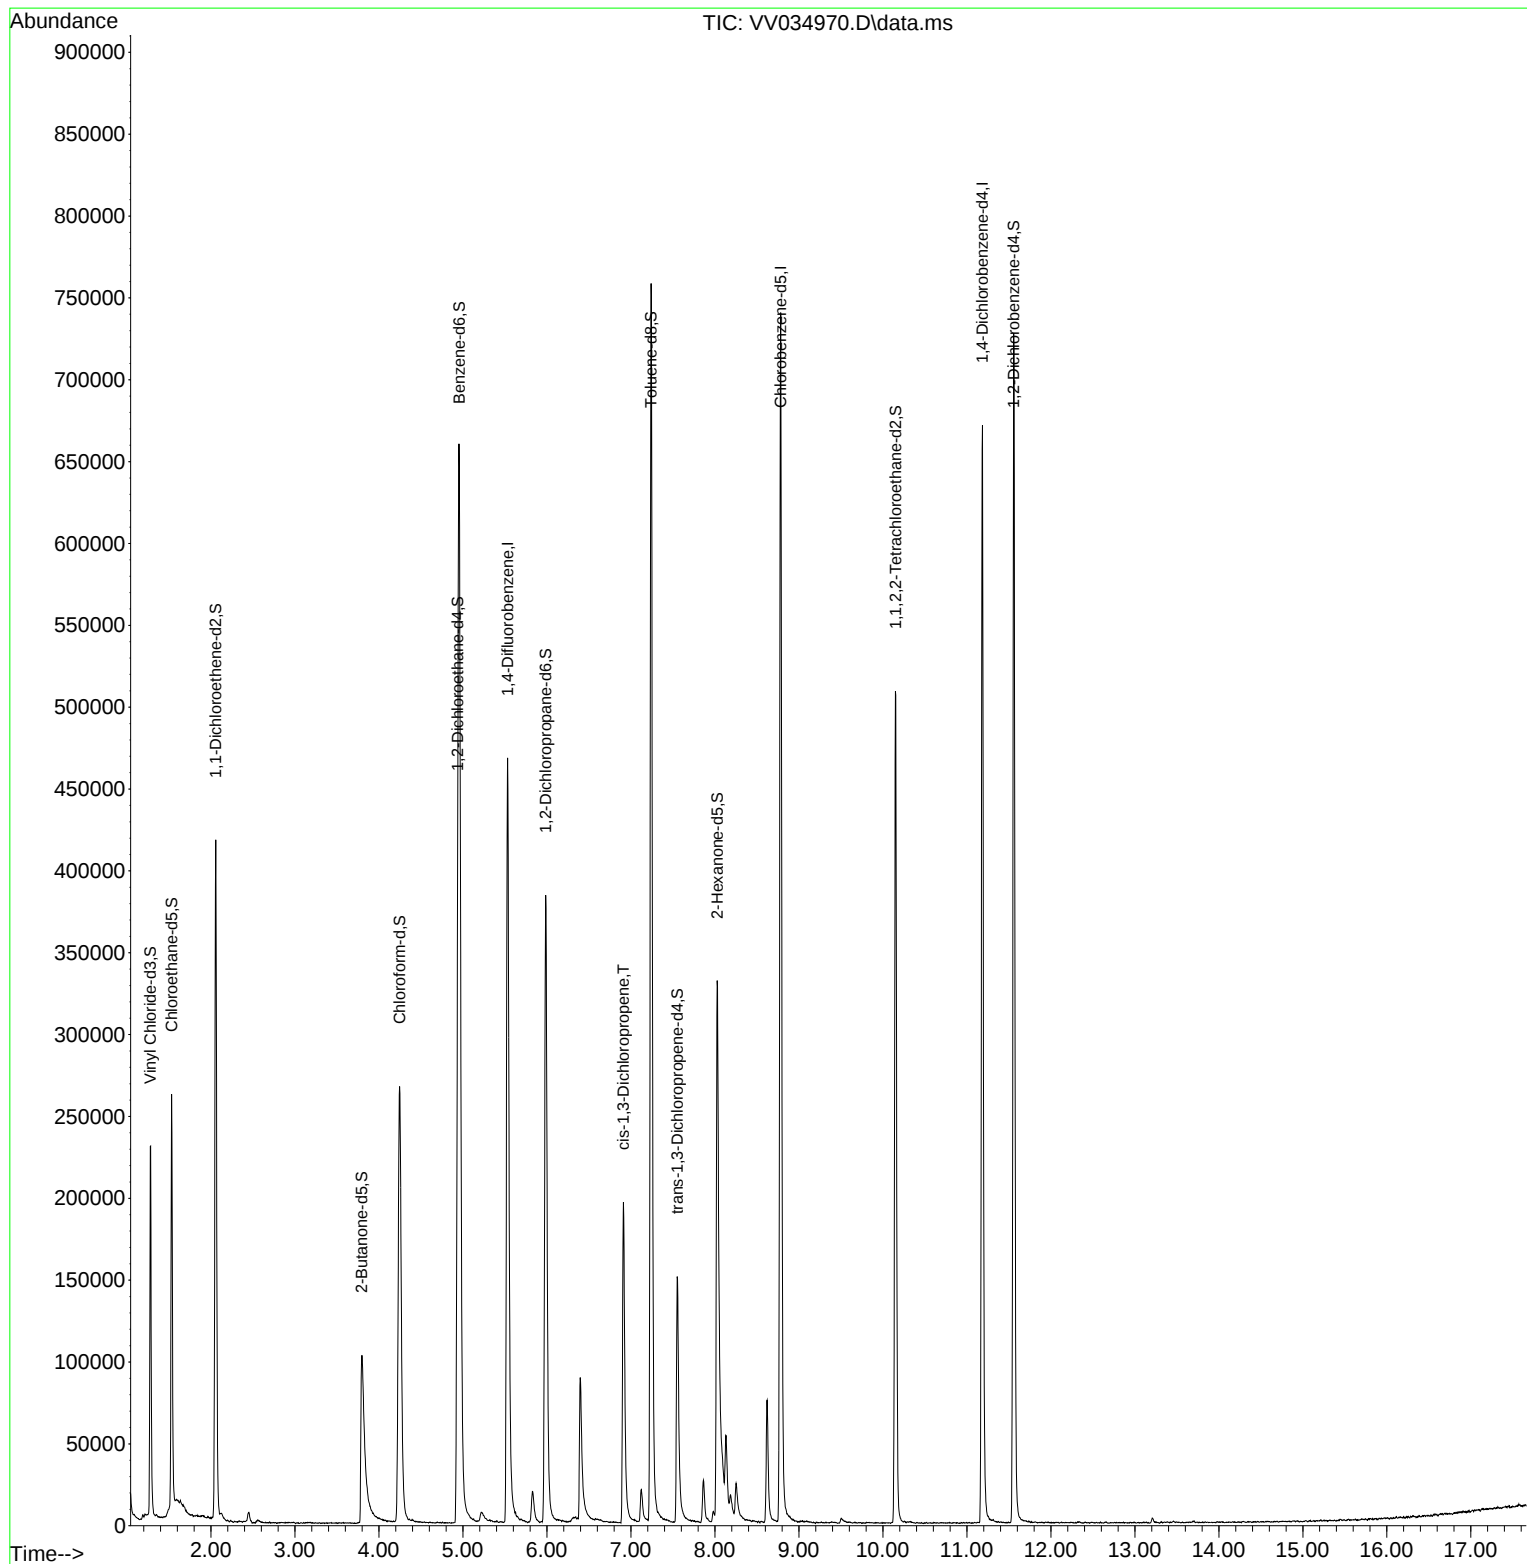

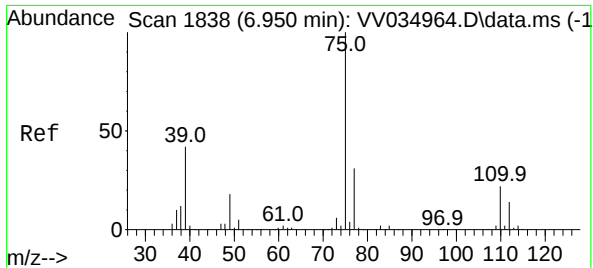

#39
 cis-1,3-Dichloropropene
 Concen: 0.864 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV034970.D
 Acq: 04 Apr 2024 11:59

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4906
 Ion Ratio Lower Upper
 75 100
 77 51.8 21.9 40.7#

