

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034965.D
 Acq On : 04 Apr 2024 09:54
 Operator : SY/MD
 Sample : VV0404WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	235275	256015	15.38%	2.087%
2	1.532	146	153	165	rBV	221763	258754	15.55%	2.109%
3	2.060	307	317	337	rBV	413975	606590	36.44%	4.945%
4	2.446	430	437	448	rVB5	2566	4535	0.27%	0.037%
5	2.761	531	535	538	rBV3	599	518	0.03%	0.004%
6	2.876	570	571	574	rBV	394	271	0.02%	0.002%
7	2.937	587	590	594	rBV2	400	224	0.01%	0.002%
8	2.957	594	596	599	rVB2	495	258	0.02%	0.002%
9	2.973	599	601	602	rBV	224	105	0.01%	0.001%
10	2.995	607	608	611	rBV2	303	129	0.01%	0.001%
11	3.011	611	613	614	rBV2	246	80	0.00%	0.001%
12	3.066	626	630	633	rBV2	317	274	0.02%	0.002%
13	3.101	639	641	642	rVB2	198	58	0.00%	0.000%
14	3.118	644	646	650	rVV2	370	266	0.02%	0.002%
15	3.140	650	653	655	rVB3	422	214	0.01%	0.002%
16	3.179	664	665	668	rBV2	306	177	0.01%	0.001%
17	3.310	704	706	707	rBV2	267	121	0.01%	0.001%
18	3.352	717	719	722	rBV	230	125	0.01%	0.001%
19	3.372	722	725	728	rBV2	459	285	0.02%	0.002%
20	3.417	737	739	741	rBV	406	218	0.01%	0.002%
21	3.452	748	750	751	rBV	230	112	0.01%	0.001%
22	3.516	769	770	771	rBV	138	36	0.00%	0.000%
23	3.526	771	773	776	rVB	280	116	0.01%	0.001%
24	3.616	799	801	803	rBV	213	94	0.01%	0.001%
25	3.632	805	806	809	rBV2	221	121	0.01%	0.001%
26	3.651	809	812	817	rVV	360	290	0.02%	0.002%
27	3.677	817	820	823	rBV2	358	283	0.02%	0.002%
28	3.757	837	845	846	rBV2	363	299	0.02%	0.002%
29	3.796	849	857	892	rBV	99140	318472	19.13%	2.596%
30	4.246	982	997	1030	rBV	257004	665767	40.00%	5.427%
31	4.642	1118	1120	1125	rVB3	749	493	0.03%	0.004%
32	4.664	1125	1127	1130	rBV	504	358	0.02%	0.003%
33	4.822	1172	1176	1177	rBV	374	232	0.01%	0.002%
34	4.953	1200	1217	1261	rBV2	623102	1664459	100.00%	13.569%
35	5.442	1367	1369	1370	rBV	404	146	0.01%	0.001%
36	5.532	1386	1397	1433	rBV	469826	981776	58.98%	8.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034965.D
 Acq On : 04 Apr 2024 09:54
 Operator : SY/MD
 Sample : VV0404WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.828	1479	1489	1505	rBV3	21584	48662	2.92%	0.397%
38	5.986	1526	1538	1565	rBV	361720	755408	45.38%	6.158%
39	6.359	1651	1654	1658	rBV3	444	426	0.03%	0.003%
40	6.465	1682	1687	1690	rBV3	553	422	0.03%	0.003%
41	6.503	1694	1699	1700	rBV	628	411	0.02%	0.003%
42	6.548	1710	1713	1715	rVB3	458	281	0.02%	0.002%
43	6.580	1721	1723	1724	rBV	499	285	0.02%	0.002%
44	6.674	1749	1752	1754	rBV2	477	280	0.02%	0.002%
45	6.728	1767	1769	1771	rBV3	551	309	0.02%	0.003%
46	6.799	1789	1791	1793	rVB	499	241	0.01%	0.002%
47	6.815	1793	1796	1799	rBV3	415	308	0.02%	0.003%
48	6.860	1804	1810	1814	rBV3	379	357	0.02%	0.003%
49	6.912	1815	1826	1862	rBV	177397	347695	20.89%	2.834%
50	7.240	1917	1928	1958	rBV	702673	1263481	75.91%	10.300%
51	7.551	2016	2025	2047	rBV	119695	222857	13.39%	1.817%
52	7.921	2138	2140	2142	rBV	485	164	0.01%	0.001%
53	8.027	2164	2173	2213	rBV3	296402	709283	42.61%	5.782%
54	8.548	2333	2335	2339	rBV3	404	267	0.02%	0.002%
55	8.690	2375	2379	2383	rBV5	712	630	0.04%	0.005%
56	8.738	2389	2394	2397	rBV5	528	456	0.03%	0.004%
57	8.783	2397	2408	2441	rBV	737603	1219827	73.29%	9.944%
58	9.140	2517	2519	2520	rBV2	652	264	0.02%	0.002%
59	9.317	2569	2574	2577	rBV3	699	578	0.03%	0.005%
60	9.333	2577	2579	2583	rVB2	435	255	0.02%	0.002%
61	9.368	2587	2590	2591	rBV	501	219	0.01%	0.002%
62	9.542	2642	2644	2646	rVB2	545	192	0.01%	0.002%
63	9.690	2686	2690	2692	rBV3	467	416	0.02%	0.003%
64	9.735	2700	2704	2709	rBV4	529	476	0.03%	0.004%
65	9.760	2709	2712	2715	rVB	290	151	0.01%	0.001%
66	9.773	2715	2716	2717	rBV	244	91	0.01%	0.001%
67	9.873	2742	2747	2749	rBV2	949	800	0.05%	0.007%
68	10.037	2796	2798	2801	rBV	363	232	0.01%	0.002%
69	10.149	2816	2833	2853	rBV	469862	749115	45.01%	6.107%
70	10.455	2926	2928	2931	rBV	354	149	0.01%	0.001%
71	10.481	2934	2936	2939	rBV3	560	390	0.02%	0.003%
72	10.715	3005	3009	3012	rBV2	648	554	0.03%	0.005%
73	10.780	3027	3029	3033	rBV	383	230	0.01%	0.002%
74	10.895	3062	3065	3068	rBV	520	317	0.02%	0.003%
75	10.915	3068	3071	3074	rVB2	664	434	0.03%	0.004%
76	10.953	3081	3083	3091	rVB3	599	677	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034965.D
 Acq On : 04 Apr 2024 09:54
 Operator : SY/MD
 Sample : VV0404WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.127	3129	3137	3143	rBV5	2168	2826	0.17%	0.023%
78	11.185	3143	3155	3185	rVV	655810	1047908	62.96%	8.543%
79	11.558	3259	3271	3304	rBV	681666	1076083	64.65%	8.772%
80	12.018	3412	3414	3415	rBV	418	140	0.01%	0.001%
81	12.101	3433	3440	3442	rBV3	551	624	0.04%	0.005%
82	12.458	3548	3551	3554	rBV	525	431	0.03%	0.004%
83	12.924	3693	3696	3699	rBV2	353	258	0.02%	0.002%
84	13.001	3717	3720	3723	rBV3	604	472	0.03%	0.004%
85	13.159	3763	3769	3775	rBV3	630	804	0.05%	0.007%
86	13.207	3775	3784	3798	rVV4	8156	12854	0.77%	0.105%
87	13.445	3850	3858	3873	rBV2	14290	24804	1.49%	0.202%
88	13.686	3925	3933	3943	rVB5	5013	8470	0.51%	0.069%
89	14.728	4253	4257	4263	rBV4	940	1075	0.06%	0.009%




Sum of corrected areas: 12266610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034965.D
Acq On : 04 Apr 2024 09:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

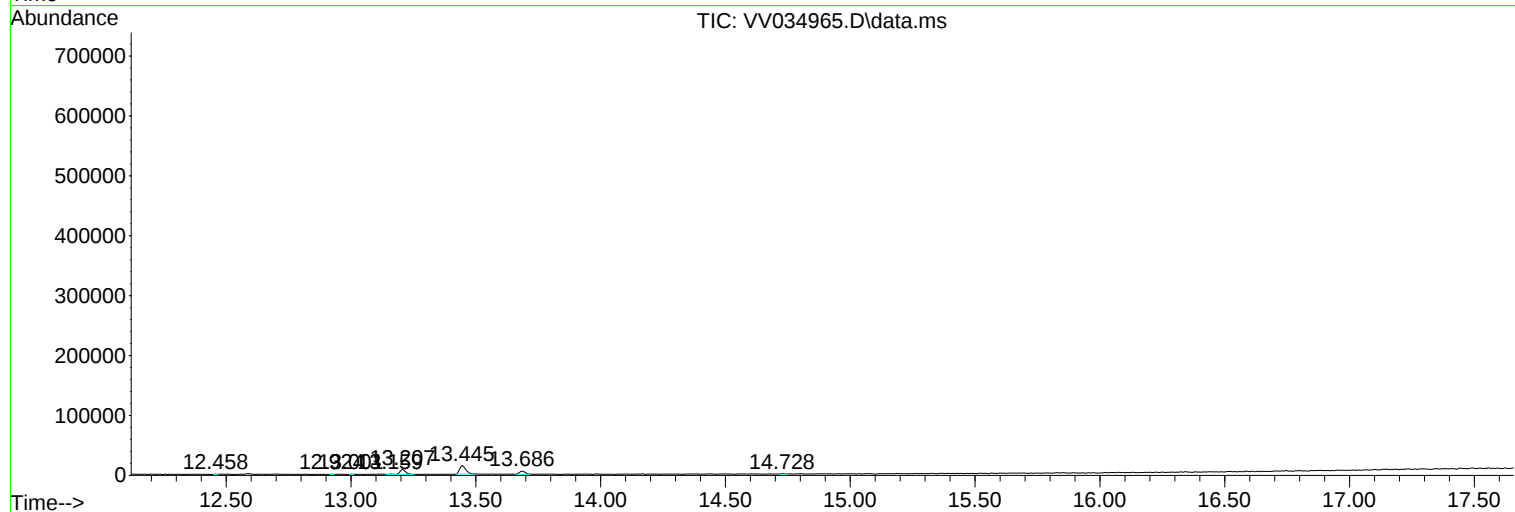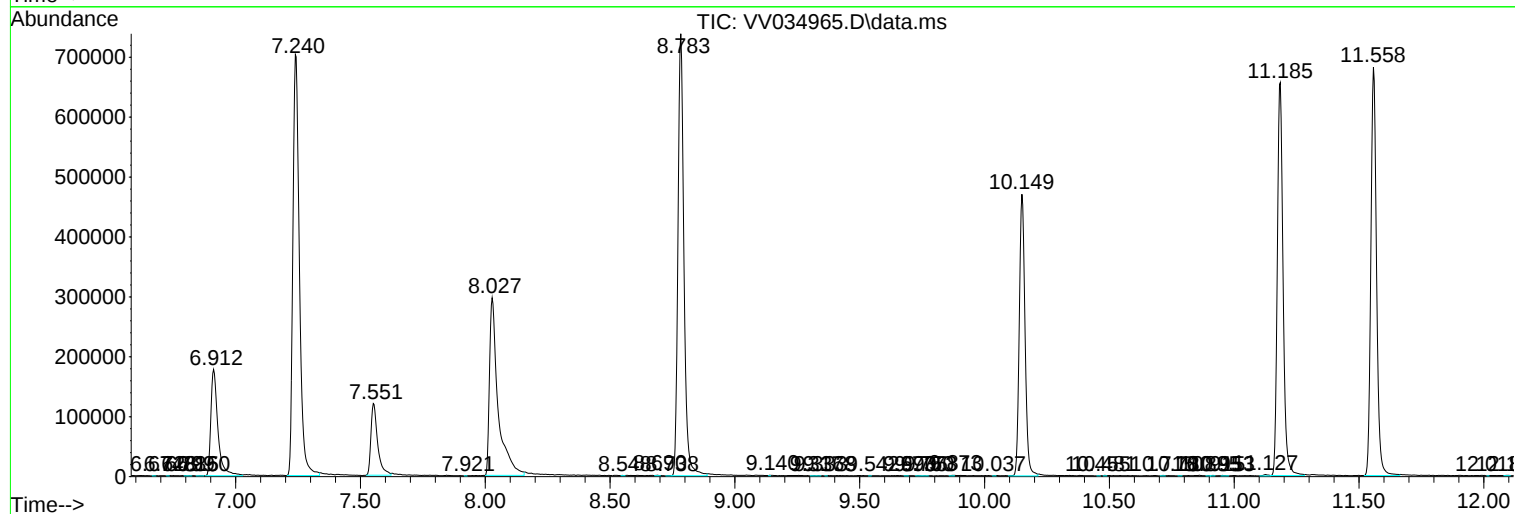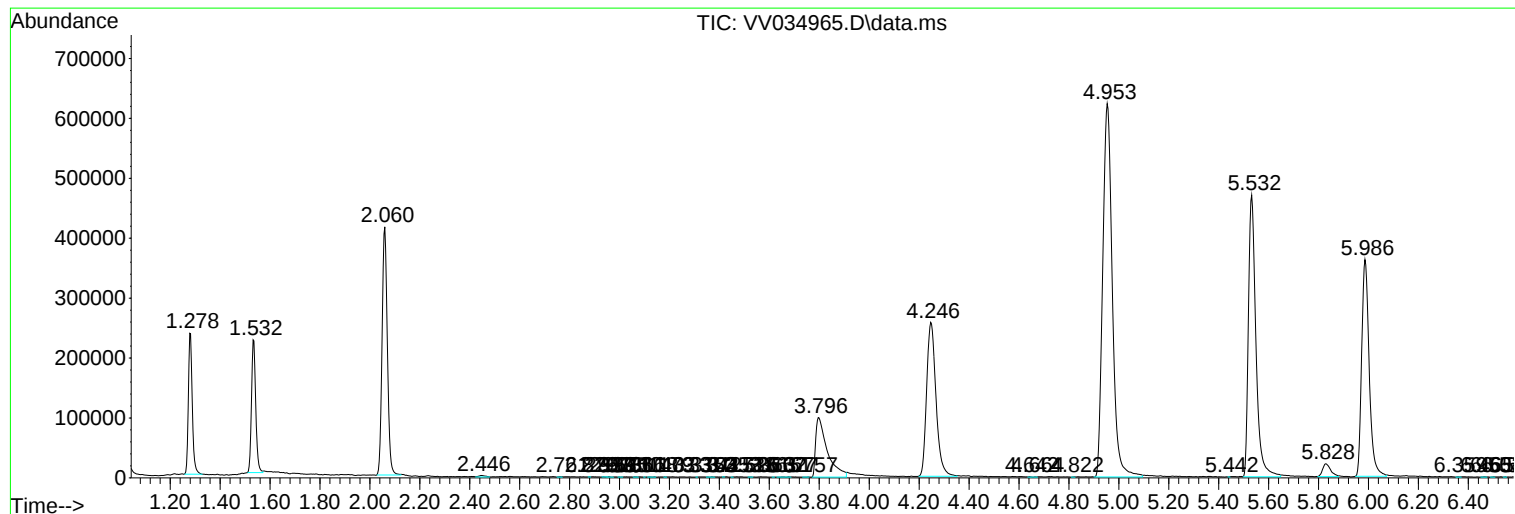

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034965.D
Acq On : 04 Apr 2024 09:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034965.D
Acq On : 04 Apr 2024 09:54
Operator : SY/MD
Sample : VV0404WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
