

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034971.D
 Acq On : 04 Apr 2024 12:22
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	42	47	52	rBV	19588	17812	1.07%	0.144%
2	1.278	68	74	91	rVB	225345	246430	14.80%	1.990%
3	1.532	146	153	166	rBV	226173	259398	15.58%	2.095%
4	2.060	307	317	331	rBV	403807	582953	35.01%	4.708%
5	2.230	368	370	373	rBV2	960	675	0.04%	0.005%
6	2.818	550	553	556	rBV2	593	403	0.02%	0.003%
7	3.143	651	654	655	rBV	298	164	0.01%	0.001%
8	3.201	669	672	673	rBV	399	216	0.01%	0.002%
9	3.233	678	682	684	rBV2	492	430	0.03%	0.003%
10	3.265	690	692	695	rBV3	339	174	0.01%	0.001%
11	3.285	695	698	699	rBV3	288	153	0.01%	0.001%
12	3.359	718	721	726	rBV3	413	304	0.02%	0.002%
13	3.468	752	755	756	rBV	243	123	0.01%	0.001%
14	3.516	768	770	775	rVB	604	338	0.02%	0.003%
15	3.593	787	794	795	rBV3	820	829	0.05%	0.007%
16	3.661	809	815	817	rBV2	441	414	0.02%	0.003%
17	3.706	826	829	830	rBV	376	217	0.01%	0.002%
18	3.732	834	837	839	rVV2	487	273	0.02%	0.002%
19	3.744	839	841	843	rVB2	218	99	0.01%	0.001%
20	3.796	848	857	900	rBV	107211	357330	21.46%	2.886%
21	4.249	983	998	1031	rBV	268262	741385	44.53%	5.987%
22	4.580	1099	1101	1106	rBV3	634	443	0.03%	0.004%
23	4.789	1164	1166	1169	rVB	442	204	0.01%	0.002%
24	4.867	1188	1190	1192	rBV2	390	220	0.01%	0.002%
25	4.953	1202	1217	1259	rBV2	624555	1664871	100.00%	13.446%
26	5.397	1352	1355	1360	rBV3	874	519	0.03%	0.004%
27	5.433	1364	1366	1369	rBV2	458	279	0.02%	0.002%
28	5.532	1382	1397	1429	rBV	464537	970037	58.26%	7.834%
29	5.828	1481	1489	1509	rVB3	22618	49692	2.98%	0.401%
30	5.986	1525	1538	1580	rBV	366205	766120	46.02%	6.187%
31	6.326	1642	1644	1648	rVB3	599	306	0.02%	0.002%
32	6.365	1655	1656	1658	rBV2	420	186	0.01%	0.002%
33	6.378	1658	1660	1664	rVB3	737	436	0.03%	0.004%
34	6.407	1664	1669	1670	rBV2	308	265	0.02%	0.002%
35	6.442	1670	1680	1694	rBV3	8091	17725	1.06%	0.143%
36	6.529	1704	1707	1709	rBV	496	279	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034971.D
 Acq On : 04 Apr 2024 12:22
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.558	1712	1716	1722	rBV2	648	703	0.04%	0.006%
38	6.580	1722	1723	1725	rBV2	299	85	0.01%	0.001%
39	6.593	1725	1727	1730	rBV3	313	235	0.01%	0.002%
40	6.638	1739	1741	1742	rBV	427	155	0.01%	0.001%
41	6.715	1763	1765	1766	rBV	209	71	0.00%	0.001%
42	6.725	1766	1768	1770	rVV2	217	112	0.01%	0.001%
43	6.815	1794	1796	1798	rBV2	391	233	0.01%	0.002%
44	6.854	1806	1808	1810	rBV2	243	121	0.01%	0.001%
45	6.873	1812	1814	1815	rBV2	430	154	0.01%	0.001%
46	6.912	1816	1826	1858	rBV	178826	347646	20.88%	2.808%
47	7.243	1917	1929	1953	rBV	714549	1267085	76.11%	10.233%
48	7.551	2016	2025	2048	rBV	121116	230084	13.82%	1.858%
49	7.918	2136	2139	2143	rBV3	335	247	0.01%	0.002%
50	7.989	2158	2161	2162	rBV3	842	474	0.03%	0.004%
51	8.027	2164	2173	2215	rVV2	308991	733398	44.05%	5.923%
52	8.529	2327	2329	2330	rBV	973	403	0.02%	0.003%
53	8.783	2397	2408	2440	rBV	719824	1195123	71.78%	9.652%
54	9.230	2544	2547	2549	rBV2	716	508	0.03%	0.004%
55	9.249	2551	2553	2557	rVB3	685	420	0.03%	0.003%
56	9.310	2568	2572	2573	rBV2	445	221	0.01%	0.002%
57	9.487	2620	2627	2628	rBV2	519	500	0.03%	0.004%
58	9.526	2637	2639	2640	rBV	422	190	0.01%	0.002%
59	9.558	2647	2649	2651	rBV	437	232	0.01%	0.002%
60	9.661	2678	2681	2684	rVB3	362	232	0.01%	0.002%
61	9.747	2705	2708	2710	rBV2	491	332	0.02%	0.003%
62	9.841	2734	2737	2742	rBV4	492	387	0.02%	0.003%
63	9.892	2751	2753	2755	rBV2	244	81	0.00%	0.001%
64	9.924	2760	2763	2764	rBV2	251	124	0.01%	0.001%
65	9.995	2781	2785	2787	rBV2	257	192	0.01%	0.002%
66	10.021	2789	2793	2804	rVB4	662	929	0.06%	0.008%
67	10.104	2815	2819	2821	rBV2	458	322	0.02%	0.003%
68	10.149	2822	2833	2854	rVV	477282	760523	45.68%	6.142%
69	10.516	2945	2947	2950	rBV3	567	248	0.01%	0.002%
70	10.661	2988	2992	2994	rBV	460	324	0.02%	0.003%
71	10.686	2999	3000	3001	rBV	193	58	0.00%	0.000%
72	10.706	3002	3006	3007	rBV2	643	431	0.03%	0.003%
73	10.747	3017	3019	3022	rVB2	422	230	0.01%	0.002%
74	10.767	3022	3025	3029	rBV3	539	413	0.02%	0.003%
75	10.882	3059	3061	3065	rVB3	378	166	0.01%	0.001%
76	11.108	3128	3131	3134	rBV2	462	330	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034971.D
 Acq On : 04 Apr 2024 12:22
 Operator : SY/MD
 Sample : P1965-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07S0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3180	rBV	667569	1047975	62.95%	8.463%
78	11.506	3252	3255	3257	rBV	656	374	0.02%	0.003%
79	11.558	3259	3271	3294	rBV	686307	1097187	65.90%	8.861%
80	12.307	3501	3504	3506	rBV3	751	441	0.03%	0.004%
81	12.464	3551	3553	3557	rVB2	666	325	0.02%	0.003%
82	12.693	3622	3624	3626	rBV2	392	193	0.01%	0.002%
83	12.725	3630	3634	3636	rBV	359	279	0.02%	0.002%
84	12.741	3637	3639	3644	rVB2	676	581	0.03%	0.005%
85	12.776	3644	3650	3658	rBV3	873	1183	0.07%	0.010%
86	12.886	3682	3684	3685	rBV2	214	59	0.00%	0.000%
87	12.931	3696	3698	3699	rBV	535	199	0.01%	0.002%
88	13.091	3745	3748	3749	rBV2	533	335	0.02%	0.003%
89	13.156	3766	3768	3771	rBV2	459	298	0.02%	0.002%
90	13.207	3778	3784	3795	rVB7	4766	7474	0.45%	0.060%




Sum of corrected areas: 12382327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034971.D
Acq On : 04 Apr 2024 12:22
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

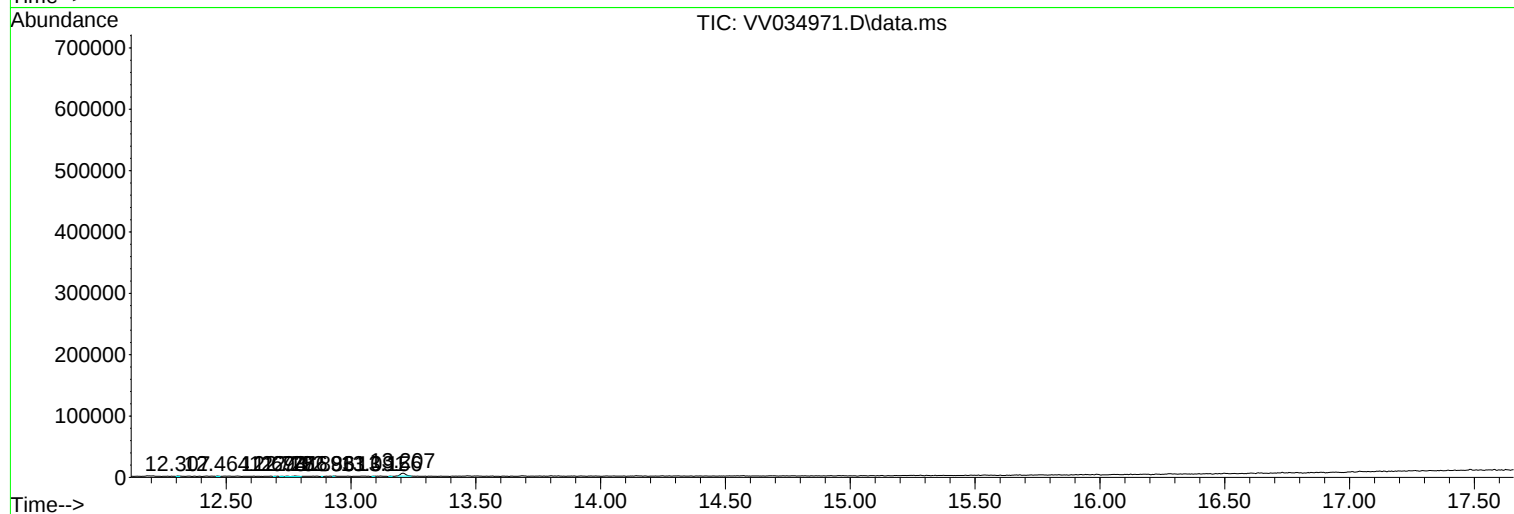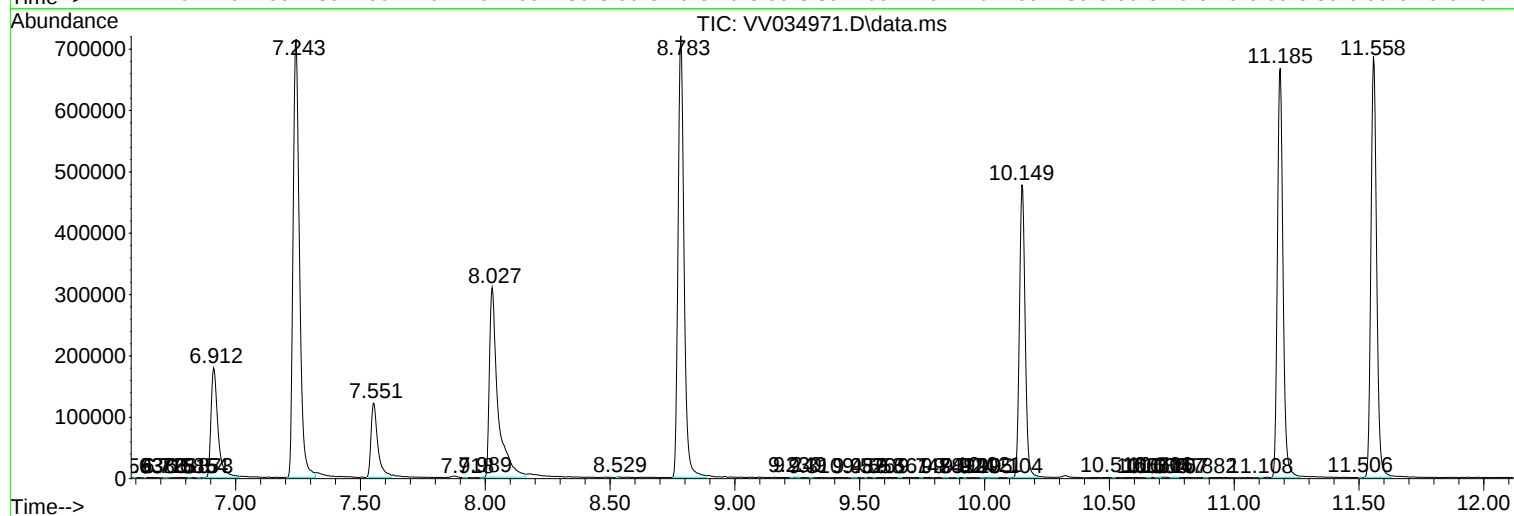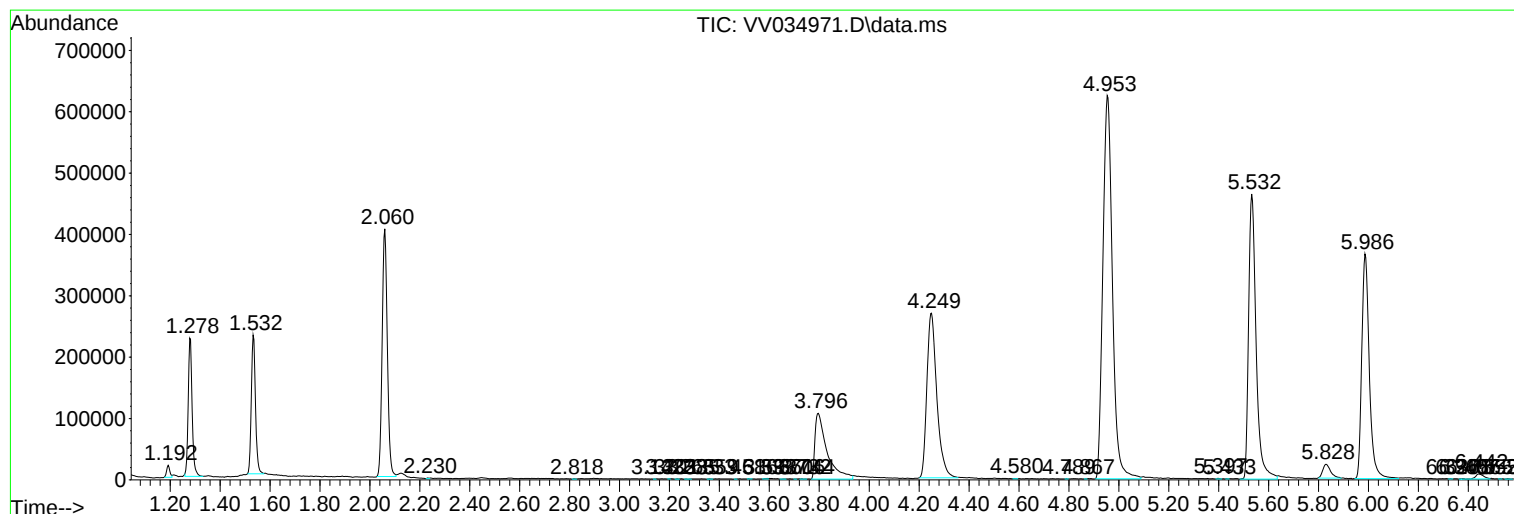

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034971.D
Acq On : 04 Apr 2024 12:22
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034971.D
Acq On : 04 Apr 2024 12:22
Operator : SY/MD
Sample : P1965-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc