

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034973.D
 Acq On : 04 Apr 2024 13:10
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	42	47	52	rBV	17624	16997	1.06%	0.143%
2	1.278	68	74	92	rVB	219846	240782	14.99%	2.027%
3	1.532	146	153	172	rVB	218005	253641	15.79%	2.135%
4	2.060	307	317	332	rBV	386006	562354	35.00%	4.735%
5	2.487	449	450	453	rBV2	441	196	0.01%	0.002%
6	2.552	466	470	471	rBV2	917	654	0.04%	0.006%
7	2.735	523	527	528	rBV3	426	269	0.02%	0.002%
8	2.835	554	558	561	rBV3	510	468	0.03%	0.004%
9	2.860	564	566	569	rBV3	476	258	0.02%	0.002%
10	2.892	569	576	578	rBV4	796	884	0.06%	0.007%
11	2.953	592	595	597	rBV3	318	195	0.01%	0.002%
12	3.002	607	610	614	rVB4	611	420	0.03%	0.004%
13	3.092	636	638	643	rVB2	599	447	0.03%	0.004%
14	3.121	643	647	648	rBV	409	266	0.02%	0.002%
15	3.172	661	663	666	rVB2	469	233	0.01%	0.002%
16	3.188	666	668	671	rBV3	481	336	0.02%	0.003%
17	3.510	764	768	771	rVB	247	191	0.01%	0.002%
18	3.571	783	787	789	rBV5	399	308	0.02%	0.003%
19	3.658	810	814	817	rVB3	393	272	0.02%	0.002%
20	3.706	826	829	832	rBV2	281	222	0.01%	0.002%
21	3.796	848	857	902	rBV	99659	333150	20.74%	2.805%
22	4.246	983	997	1038	rBV	257371	724364	45.09%	6.099%
23	4.828	1175	1178	1180	rBV	589	360	0.02%	0.003%
24	4.953	1201	1217	1250	rBV2	606974	1606516	100.00%	13.526%
25	5.532	1386	1397	1437	rBV	429402	906976	56.46%	7.636%
26	5.760	1463	1468	1473	rVB5	1230	1203	0.07%	0.010%
27	5.828	1479	1489	1505	rBV2	24494	53911	3.36%	0.454%
28	5.986	1525	1538	1567	rBV	357287	748088	46.57%	6.298%
29	6.256	1620	1622	1625	rVB2	438	193	0.01%	0.002%
30	6.310	1635	1639	1642	rVB4	582	521	0.03%	0.004%
31	6.326	1642	1644	1648	rBV4	541	323	0.02%	0.003%
32	6.445	1668	1681	1697	rBV2	7845	17960	1.12%	0.151%
33	6.645	1739	1743	1745	rBV2	674	551	0.03%	0.005%
34	6.677	1751	1753	1756	rBV2	551	322	0.02%	0.003%
35	6.696	1756	1759	1763	rVV2	364	283	0.02%	0.002%
36	6.715	1763	1765	1768	rBV3	333	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034973.D
 Acq On : 04 Apr 2024 13:10
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.786	1784	1787	1790	rBV3	440	277	0.02%	0.002%
38	6.809	1790	1794	1797	rBV2	502	323	0.02%	0.003%
39	6.825	1797	1799	1801	rBV2	430	198	0.01%	0.002%
40	6.912	1815	1826	1853	rBV	173373	339560	21.14%	2.859%
41	7.162	1901	1904	1905	rBV2	647	336	0.02%	0.003%
42	7.243	1917	1929	1953	rBV	687260	1227013	76.38%	10.331%
43	7.551	2016	2025	2056	rBV	115080	222893	13.87%	1.877%
44	7.786	2097	2098	2100	rBV	433	202	0.01%	0.002%
45	7.870	2116	2124	2133	rBV7	1965	3807	0.24%	0.032%
46	7.921	2138	2140	2144	rVB3	402	290	0.02%	0.002%
47	7.992	2159	2162	2163	rBV	630	338	0.02%	0.003%
48	8.027	2164	2173	2213	rVV2	298770	705293	43.90%	5.938%
49	8.442	2298	2302	2306	rVB5	802	548	0.03%	0.005%
50	8.519	2324	2326	2329	rBV3	416	232	0.01%	0.002%
51	8.593	2348	2349	2351	rBV	484	250	0.02%	0.002%
52	8.632	2358	2361	2365	rBV3	543	335	0.02%	0.003%
53	8.651	2365	2367	2371	rVB	540	364	0.02%	0.003%
54	8.680	2371	2376	2380	rBV4	467	464	0.03%	0.004%
55	8.706	2381	2384	2390	rVB4	729	605	0.04%	0.005%
56	8.783	2397	2408	2443	rBV	667045	1117572	69.56%	9.409%
57	9.172	2524	2529	2534	rBV5	793	941	0.06%	0.008%
58	9.272	2557	2560	2563	rVB3	295	200	0.01%	0.002%
59	9.294	2563	2567	2569	rBV2	485	338	0.02%	0.003%
60	9.378	2591	2593	2598	rBV2	207	217	0.01%	0.002%
61	9.423	2604	2607	2610	rBV2	557	393	0.02%	0.003%
62	9.474	2618	2623	2624	rBV	435	310	0.02%	0.003%
63	9.645	2672	2676	2684	rVB4	798	864	0.05%	0.007%
64	9.677	2684	2686	2689	rBV2	386	201	0.01%	0.002%
65	9.715	2695	2698	2699	rBV	425	242	0.02%	0.002%
66	9.776	2714	2717	2722	rVB2	507	337	0.02%	0.003%
67	9.805	2722	2726	2728	rBV2	324	261	0.02%	0.002%
68	9.908	2755	2758	2761	rBV3	320	217	0.01%	0.002%
69	10.056	2802	2804	2808	rVB	329	230	0.01%	0.002%
70	10.075	2808	2810	2814	rVB	388	272	0.02%	0.002%
71	10.101	2814	2818	2821	rBV3	540	455	0.03%	0.004%
72	10.149	2822	2833	2856	rBV	461171	731537	45.54%	6.159%
73	10.317	2878	2885	2887	rBV3	2248	2347	0.15%	0.020%
74	10.358	2896	2898	2901	rBV	416	191	0.01%	0.002%
75	10.516	2944	2947	2950	rVB3	568	329	0.02%	0.003%
76	10.673	2993	2996	2998	rBV3	266	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034973.D
 Acq On : 04 Apr 2024 13:10
 Operator : SY/MD
 Sample : P1988-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.789	3030	3032	3036	rBV2	351	245	0.02%	0.002%
78	10.841	3044	3048	3049	rBV	409	302	0.02%	0.003%
79	10.886	3058	3062	3066	rBV2	603	577	0.04%	0.005%
80	11.130	3135	3138	3143	rVB3	705	617	0.04%	0.005%
81	11.185	3143	3155	3188	rBV	617969	969352	60.34%	8.161%
82	11.448	3234	3237	3240	rBV3	472	391	0.02%	0.003%
83	11.509	3254	3256	3259	rBV3	368	262	0.02%	0.002%
84	11.558	3259	3271	3296	rBV	671489	1065003	66.29%	8.967%
85	11.844	3357	3360	3364	rBV3	577	556	0.03%	0.005%
86	11.950	3389	3393	3394	rBV3	381	301	0.02%	0.003%
87	11.982	3399	3403	3407	rBV2	542	351	0.02%	0.003%
88	12.011	3410	3412	3414	rBV2	310	199	0.01%	0.002%
89	12.062	3424	3428	3433	rBV3	467	386	0.02%	0.003%
90	12.120	3444	3446	3449	rBV	417	247	0.02%	0.002%
91	12.487	3557	3560	3563	rBV2	719	491	0.03%	0.004%
92	12.805	3657	3659	3662	rBV2	371	202	0.01%	0.002%
93	12.824	3663	3665	3667	rBV2	473	264	0.02%	0.002%
94	12.892	3683	3686	3688	rBV2	443	298	0.02%	0.003%
95	12.950	3701	3704	3707	rBV3	547	441	0.03%	0.004%
96	13.098	3747	3750	3753	rBV2	434	273	0.02%	0.002%
97	13.114	3753	3755	3758	rBV	496	266	0.02%	0.002%
98	13.275	3803	3805	3807	rBV2	365	185	0.01%	0.002%
99	13.342	3823	3826	3829	rBV3	566	429	0.03%	0.004%
100	14.156	4077	4079	4083	rBV3	556	412	0.03%	0.003%




Sum of corrected areas: 11877372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034973.D
Acq On : 04 Apr 2024 13:10
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

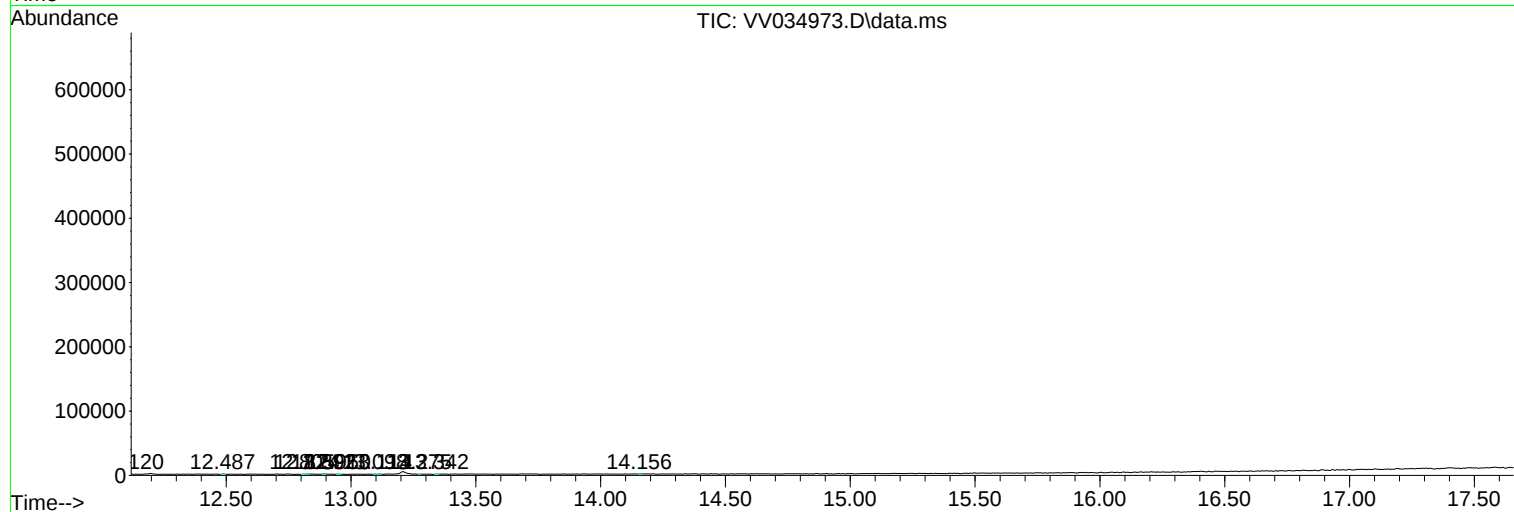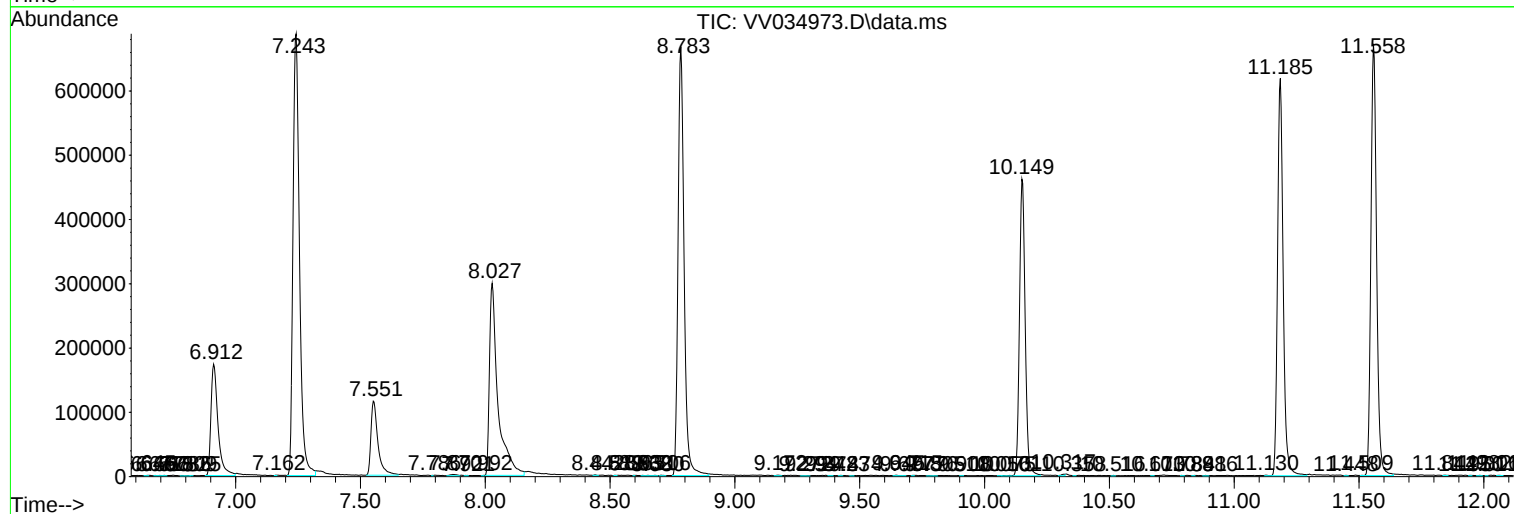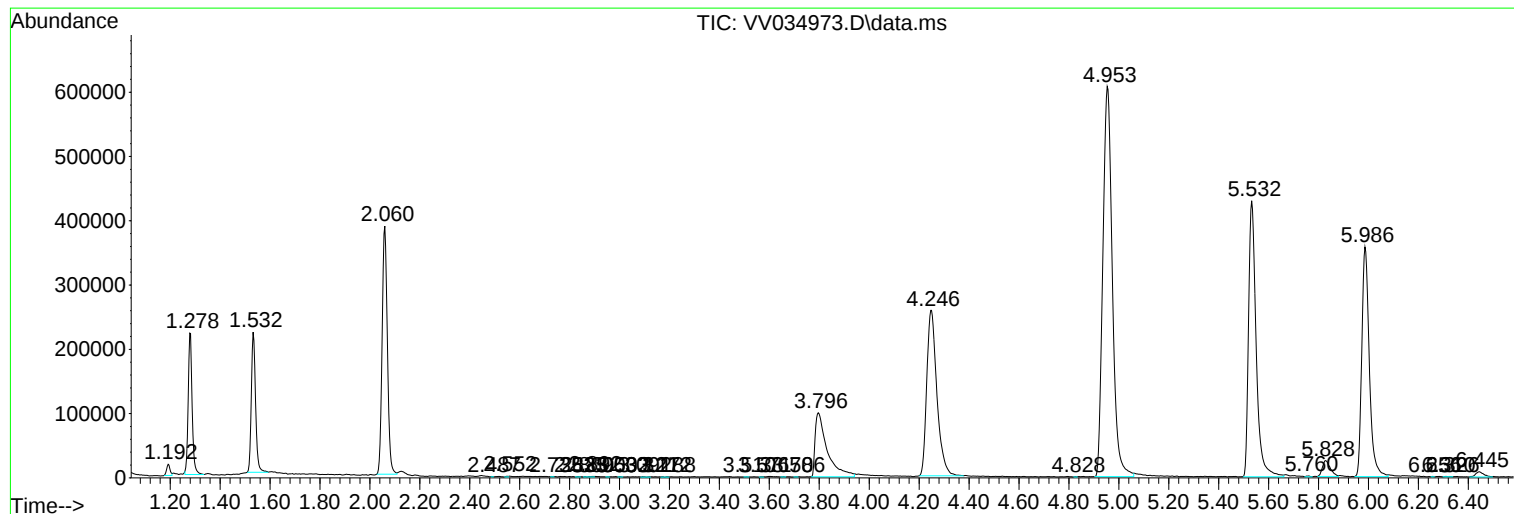

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034973.D
Acq On : 04 Apr 2024 13:10
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034973.D
Acq On : 04 Apr 2024 13:10
Operator : SY/MD
Sample : P1988-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------