

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034974.D
 Acq On : 04 Apr 2024 13:33
 Operator : SY/MD
 Sample : P1988-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	42	47	52	rBV	14756	13816	0.85%	0.117%
2	1.281	68	75	92	rVB	225455	244082	15.09%	2.066%
3	1.532	146	153	174	rVB	226353	260830	16.13%	2.208%
4	2.060	307	317	331	rBV	396587	572042	35.37%	4.842%
5	2.587	479	481	482	rBV2	633	247	0.02%	0.002%
6	2.687	510	512	514	rBV3	489	248	0.02%	0.002%
7	2.773	536	539	542	rBV2	516	299	0.02%	0.003%
8	2.805	545	549	553	rBV2	616	508	0.03%	0.004%
9	2.825	553	555	558	rVB2	448	201	0.01%	0.002%
10	2.886	572	574	576	rBV3	360	163	0.01%	0.001%
11	3.050	622	625	626	rBV	442	194	0.01%	0.002%
12	3.076	629	633	634	rBV2	449	296	0.02%	0.003%
13	3.140	650	653	655	rBV2	466	282	0.02%	0.002%
14	3.195	668	670	674	rVB3	366	212	0.01%	0.002%
15	3.220	674	678	682	rBV2	629	453	0.03%	0.004%
16	3.236	682	683	686	rVB2	260	104	0.01%	0.001%
17	3.256	686	689	694	rBV	359	358	0.02%	0.003%
18	3.278	694	696	698	rBV	337	186	0.01%	0.002%
19	3.342	713	716	719	rBV2	502	306	0.02%	0.003%
20	3.455	749	751	753	rVB2	320	154	0.01%	0.001%
21	3.567	782	786	790	rBV3	602	535	0.03%	0.005%
22	3.648	809	811	814	rVB	278	115	0.01%	0.001%
23	3.690	818	824	828	rBV2	514	471	0.03%	0.004%
24	3.722	832	834	838	rBV2	665	361	0.02%	0.003%
25	3.741	838	840	845	rVB2	325	194	0.01%	0.002%
26	3.796	848	857	893	rBV	98480	314853	19.47%	2.665%
27	4.249	983	998	1036	rBV	259832	721498	44.61%	6.107%
28	4.561	1093	1095	1097	rBV3	544	206	0.01%	0.002%
29	4.632	1115	1117	1120	rBV2	307	128	0.01%	0.001%
30	4.670	1126	1129	1131	rBV3	343	212	0.01%	0.002%
31	4.699	1136	1138	1140	rVB	589	216	0.01%	0.002%
32	4.715	1140	1143	1146	rBV2	431	282	0.02%	0.002%
33	4.735	1147	1149	1154	rVV3	493	357	0.02%	0.003%
34	4.860	1185	1188	1189	rBV2	460	234	0.01%	0.002%
35	4.953	1202	1217	1249	rBV2	611110	1617469	100.00%	13.692%
36	5.403	1355	1357	1358	rBV	512	204	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034974.D
 Acq On : 04 Apr 2024 13:33
 Operator : SY/MD
 Sample : P1988-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.493	1382	1385	1386	rBV2	671	449	0.03%	0.004%
38	5.532	1386	1397	1430	rVV	416602	880232	54.42%	7.451%
39	5.828	1480	1489	1505	rBV4	24697	54262	3.35%	0.459%
40	5.985	1525	1538	1569	rBV	356988	755301	46.70%	6.394%
41	6.333	1643	1646	1648	rBV3	594	448	0.03%	0.004%
42	6.442	1673	1680	1694	rVB3	6439	12375	0.77%	0.105%
43	6.561	1714	1717	1721	rBV3	385	323	0.02%	0.003%
44	6.609	1727	1732	1735	rBV3	568	539	0.03%	0.005%
45	6.635	1737	1740	1741	rBV	442	206	0.01%	0.002%
46	6.670	1750	1751	1754	rVB2	359	172	0.01%	0.001%
47	6.693	1754	1758	1760	rBV4	459	342	0.02%	0.003%
48	6.712	1760	1764	1768	rVV2	557	511	0.03%	0.004%
49	6.731	1768	1770	1773	rVV2	383	264	0.02%	0.002%
50	6.747	1773	1775	1778	rVB3	639	288	0.02%	0.002%
51	6.873	1809	1814	1816	rBV3	268	180	0.01%	0.002%
52	6.911	1816	1826	1855	rBV2	174631	342064	21.15%	2.896%
53	7.243	1918	1929	1952	rBV	702110	1236567	76.45%	10.467%
54	7.551	2016	2025	2056	rBV	120570	226037	13.97%	1.913%
55	7.876	2115	2126	2129	rBV4	1956	2838	0.18%	0.024%
56	7.908	2135	2136	2142	rVB3	714	533	0.03%	0.005%
57	8.027	2161	2173	2211	rBV2	290986	696764	43.08%	5.898%
58	8.532	2329	2330	2333	rVB2	346	126	0.01%	0.001%
59	8.558	2335	2338	2340	rBV	841	527	0.03%	0.004%
60	8.783	2397	2408	2440	rBV	662898	1093048	67.58%	9.253%
61	9.181	2530	2532	2536	rVB2	653	394	0.02%	0.003%
62	9.226	2542	2546	2547	rBV2	412	253	0.02%	0.002%
63	9.252	2552	2554	2556	rVB	280	119	0.01%	0.001%
64	9.281	2556	2563	2568	rBV3	674	955	0.06%	0.008%
65	9.419	2603	2606	2609	rVB	342	200	0.01%	0.002%
66	9.445	2613	2614	2616	rBV	219	107	0.01%	0.001%
67	9.464	2617	2620	2623	rBV2	410	269	0.02%	0.002%
68	9.484	2623	2626	2631	rBV3	484	488	0.03%	0.004%
69	9.689	2686	2690	2692	rBV2	364	293	0.02%	0.002%
70	9.741	2704	2706	2710	rBV	242	150	0.01%	0.001%
71	9.776	2715	2717	2727	rVB	356	449	0.03%	0.004%
72	9.818	2727	2730	2731	rBV	318	183	0.01%	0.002%
73	9.876	2746	2748	2751	rVB2	215	103	0.01%	0.001%
74	9.898	2752	2755	2759	rVB3	553	413	0.03%	0.003%
75	9.998	2782	2786	2788	rBV4	666	430	0.03%	0.004%
76	10.149	2820	2833	2865	rBV	453212	729985	45.13%	6.179%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034974.D
 Acq On : 04 Apr 2024 13:33
 Operator : SY/MD
 Sample : P1988-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.406	2910	2913	2914	rBV2	293	158	0.01%	0.001%
78	10.503	2941	2943	2947	rBV2	308	213	0.01%	0.002%
79	10.545	2954	2956	2961	rVB3	444	244	0.02%	0.002%
80	10.660	2989	2992	2994	rBV2	410	295	0.02%	0.002%
81	10.722	2998	3011	3015	rBV6	1235	2190	0.14%	0.019%
82	10.796	3027	3034	3036	rBV	459	528	0.03%	0.004%
83	10.812	3036	3039	3041	rBV2	390	281	0.02%	0.002%
84	10.966	3084	3087	3091	rVB3	675	489	0.03%	0.004%
85	11.004	3097	3099	3100	rBV3	290	124	0.01%	0.001%
86	11.114	3131	3133	3135	rBV	233	134	0.01%	0.001%
87	11.130	3135	3138	3140	rBV3	1067	705	0.04%	0.006%
88	11.185	3144	3155	3180	rBV	596490	944039	58.37%	7.991%
89	11.558	3259	3271	3292	rBV	667377	1064400	65.81%	9.010%
90	12.406	3533	3535	3538	rVB2	543	257	0.02%	0.002%
91	12.448	3546	3548	3553	rVB2	668	440	0.03%	0.004%
92	12.506	3564	3566	3569	rBV	324	250	0.02%	0.002%
93	12.712	3625	3630	3632	rBV3	574	451	0.03%	0.004%
94	12.744	3638	3640	3641	rBV3	294	104	0.01%	0.001%
95	12.853	3670	3674	3676	rBV2	439	354	0.02%	0.003%
96	13.033	3727	3730	3731	rBV2	285	177	0.01%	0.001%
97	13.207	3778	3784	3792	rVB8	3338	5318	0.33%	0.045%
98	13.339	3821	3825	3828	rVB2	670	452	0.03%	0.004%
99	13.355	3828	3830	3831	rBV	419	158	0.01%	0.001%
100	13.779	3960	3962	3963	rBV	466	193	0.01%	0.002%




Sum of corrected areas: 11813457

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034974.D
Acq On : 04 Apr 2024 13:33
Operator : SY/MD
Sample : P1988-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

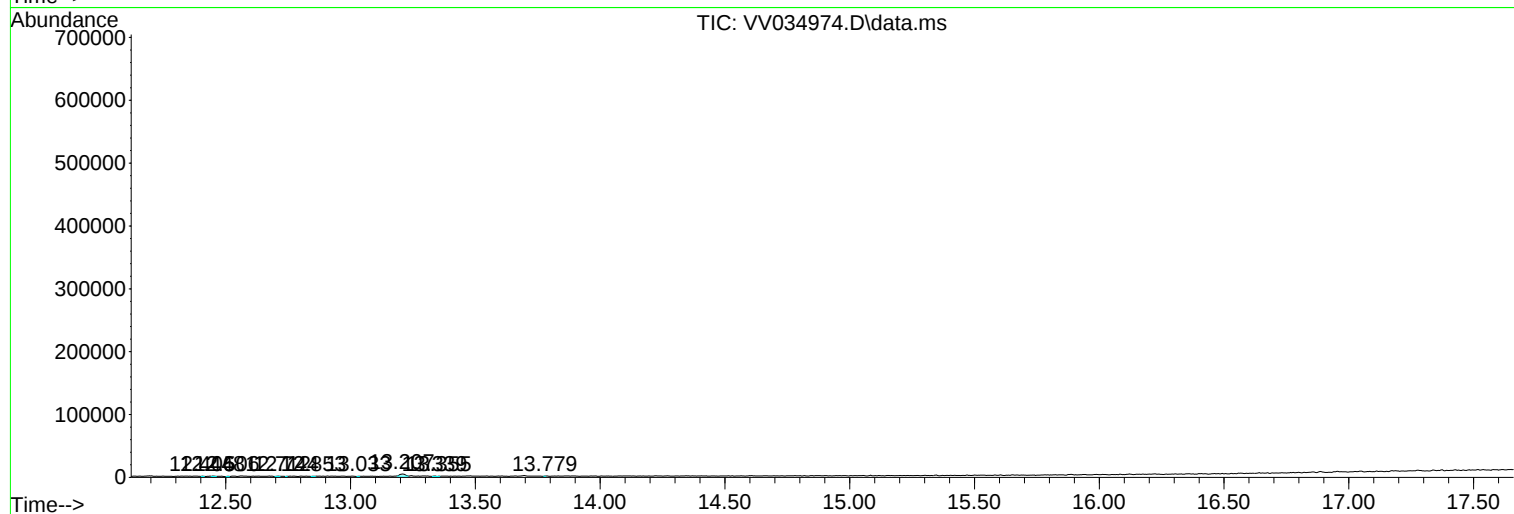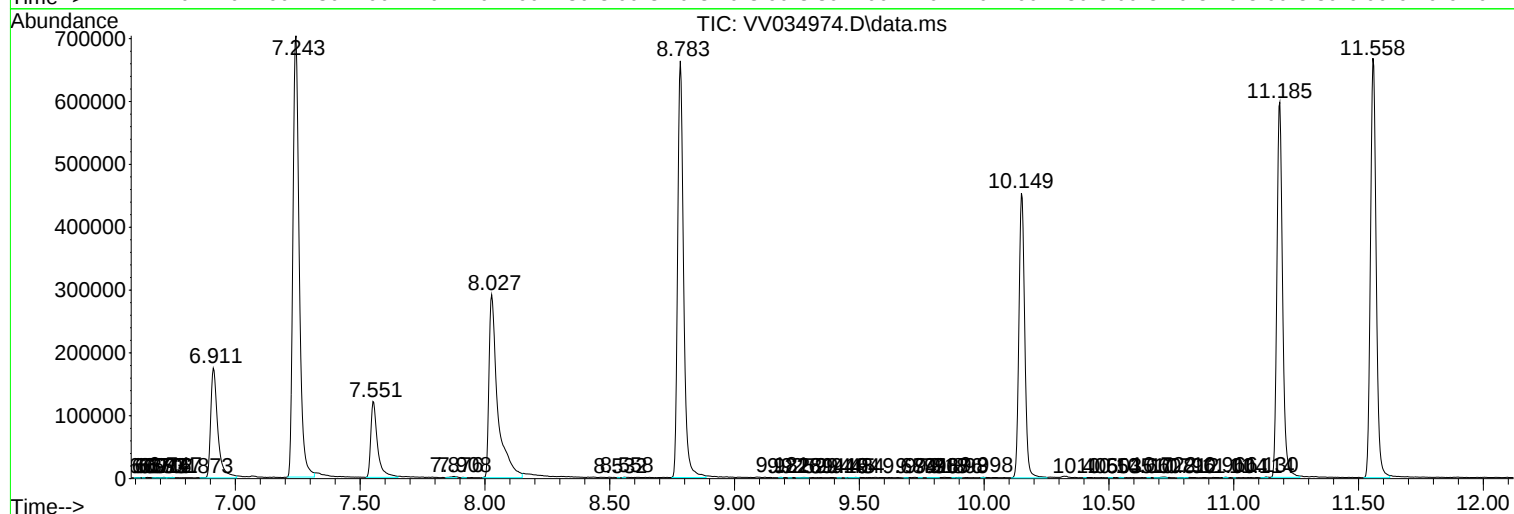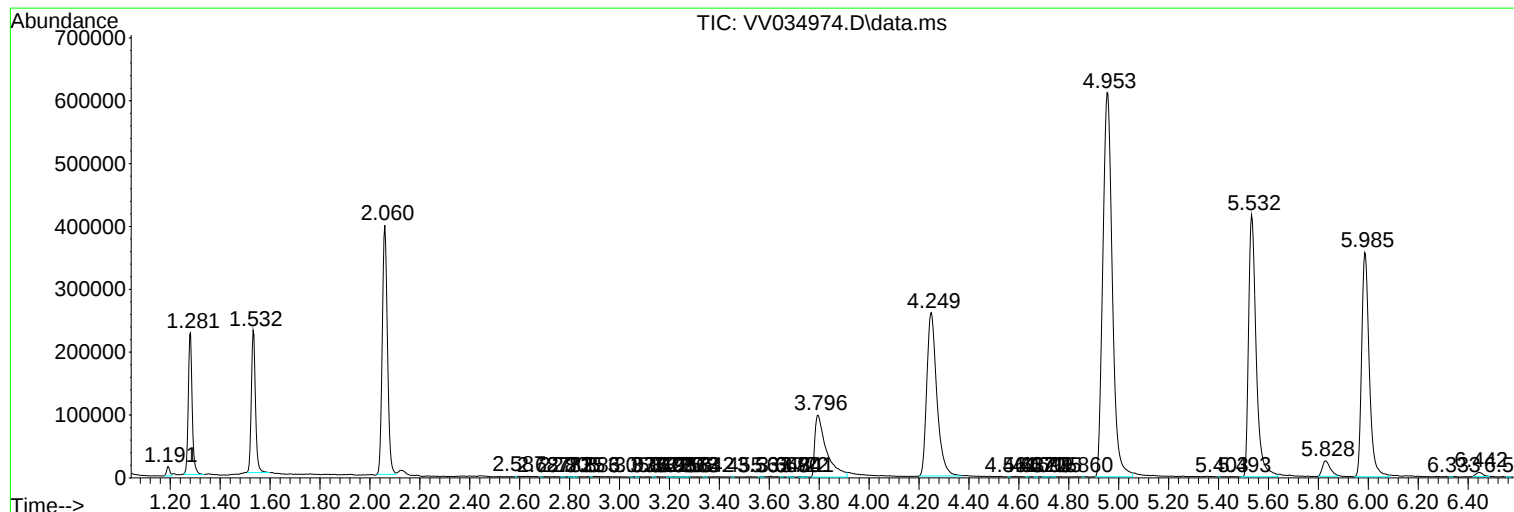

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034974.D
Acq On : 04 Apr 2024 13:33
Operator : SY/MD
Sample : P1988-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034974.D
Acq On : 04 Apr 2024 13:33
Operator : SY/MD
Sample : P1988-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------