

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034975.D
 Acq On : 04 Apr 2024 13:57
 Operator : SY/MD
 Sample : P1965-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	219736	238104	14.47%	1.994%
2	1.532	146	153	168	rVB	233127	264063	16.04%	2.212%
3	2.060	307	317	339	rBV	395375	571714	34.73%	4.789%
4	2.870	567	569	572	rBV2	379	195	0.01%	0.002%
5	2.957	594	596	597	rBV	329	152	0.01%	0.001%
6	3.037	616	621	622	rBV3	384	311	0.02%	0.003%
7	3.060	626	628	631	rBV	342	210	0.01%	0.002%
8	3.143	652	654	657	rVB3	543	292	0.02%	0.002%
9	3.188	666	668	671	rVB2	312	155	0.01%	0.001%
10	3.207	671	674	677	rBV2	431	327	0.02%	0.003%
11	3.233	677	682	685	rBV2	426	370	0.02%	0.003%
12	3.256	688	689	693	rVB2	322	193	0.01%	0.002%
13	3.297	697	702	704	rBV4	475	374	0.02%	0.003%
14	3.330	710	712	715	rVB3	408	174	0.01%	0.001%
15	3.416	735	739	743	rBV2	331	282	0.02%	0.002%
16	3.449	747	749	752	rBV2	135	78	0.00%	0.001%
17	3.468	752	755	759	rVV3	429	292	0.02%	0.002%
18	3.500	763	765	767	rBV2	194	108	0.01%	0.001%
19	3.535	773	776	778	rVB2	520	303	0.02%	0.003%
20	3.558	778	783	791	rBV3	380	463	0.03%	0.004%
21	3.590	791	793	794	rBV	306	147	0.01%	0.001%
22	3.674	816	819	822	rVB2	253	164	0.01%	0.001%
23	3.699	822	827	830	rVB2	412	306	0.02%	0.003%
24	3.796	848	857	902	rBV2	105247	332000	20.17%	2.781%
25	4.249	983	998	1032	rBV	252764	650677	39.53%	5.450%
26	4.712	1139	1142	1143	rBV	124	79	0.00%	0.001%
27	4.728	1143	1147	1148	rVV2	316	184	0.01%	0.002%
28	4.760	1156	1157	1160	rBV2	259	105	0.01%	0.001%
29	4.822	1173	1176	1177	rBV	323	161	0.01%	0.001%
30	4.867	1185	1190	1194	rBV3	568	588	0.04%	0.005%
31	4.953	1202	1217	1256	rBV2	616098	1646046	100.00%	13.787%
32	5.423	1359	1363	1365	rBV2	782	622	0.04%	0.005%
33	5.458	1371	1374	1378	rVB3	582	368	0.02%	0.003%
34	5.481	1379	1381	1383	rBV	559	243	0.01%	0.002%
35	5.532	1386	1397	1433	rBV	440886	921677	55.99%	7.720%
36	5.831	1479	1490	1511	rBV2	18688	42291	2.57%	0.354%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034975.D
 Acq On : 04 Apr 2024 13:57
 Operator : SY/MD
 Sample : P1965-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1526	1538	1568	rBV	359859	757161	46.00%	6.342%
38	6.313	1637	1640	1642	rBV2	435	227	0.01%	0.002%
39	6.339	1644	1648	1653	rVB5	738	781	0.05%	0.007%
40	6.403	1665	1668	1671	rBV4	443	272	0.02%	0.002%
41	6.420	1671	1673	1679	rVV4	473	450	0.03%	0.004%
42	6.539	1707	1710	1712	rBV2	290	125	0.01%	0.001%
43	6.555	1712	1715	1718	rVB2	341	191	0.01%	0.002%
44	6.571	1718	1720	1721	rBV	394	168	0.01%	0.001%
45	6.622	1732	1736	1739	rBV3	328	268	0.02%	0.002%
46	6.677	1752	1753	1756	rBV	298	153	0.01%	0.001%
47	6.773	1779	1783	1788	rBV2	477	441	0.03%	0.004%
48	6.802	1788	1792	1795	rBV3	385	286	0.02%	0.002%
49	6.850	1804	1807	1809	rBV	329	197	0.01%	0.002%
50	6.911	1815	1826	1856	rBV	174764	343787	20.89%	2.879%
51	7.243	1918	1929	1968	rBV	697087	1248553	75.85%	10.458%
52	7.555	2016	2026	2050	rBV	117749	221538	13.46%	1.856%
53	7.934	2142	2144	2147	rBV2	315	175	0.01%	0.001%
54	8.027	2164	2173	2218	rBV2	311865	727873	44.22%	6.097%
55	8.558	2334	2338	2340	rBV2	570	489	0.03%	0.004%
56	8.632	2358	2361	2363	rBV4	834	532	0.03%	0.004%
57	8.680	2374	2376	2378	rVB	397	142	0.01%	0.001%
58	8.693	2378	2380	2383	rVB3	662	336	0.02%	0.003%
59	8.715	2383	2387	2390	rBV3	707	552	0.03%	0.005%
60	8.738	2390	2394	2397	rBV	404	348	0.02%	0.003%
61	8.783	2397	2408	2435	rBV	689260	1132440	68.80%	9.485%
62	9.111	2508	2510	2514	rBV	555	342	0.02%	0.003%
63	9.136	2514	2518	2520	rBV4	500	373	0.02%	0.003%
64	9.172	2527	2529	2530	rBV	712	265	0.02%	0.002%
65	9.230	2542	2547	2553	rBV5	383	548	0.03%	0.005%
66	9.339	2580	2581	2583	rBV	237	101	0.01%	0.001%
67	9.355	2583	2586	2590	rVV4	464	390	0.02%	0.003%
68	9.378	2591	2593	2599	rVB5	463	338	0.02%	0.003%
69	9.461	2616	2619	2621	rBV2	647	352	0.02%	0.003%
70	9.548	2644	2646	2648	rBV	344	170	0.01%	0.001%
71	9.590	2657	2659	2662	rBV2	341	215	0.01%	0.002%
72	9.718	2697	2699	2700	rBV	270	96	0.01%	0.001%
73	9.780	2715	2718	2720	rVB	351	205	0.01%	0.002%
74	9.796	2720	2723	2724	rBV	171	108	0.01%	0.001%
75	9.866	2741	2745	2748	rBV	396	297	0.02%	0.002%
76	9.944	2763	2769	2774	rBV3	461	687	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034975.D
 Acq On : 04 Apr 2024 13:57
 Operator : SY/MD
 Sample : P1965-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.021	2791	2793	2796	rVB2	392	193	0.01%	0.002%
78	10.079	2809	2811	2815	rBV	433	303	0.02%	0.003%
79	10.111	2818	2821	2822	rBV2	251	119	0.01%	0.001%
80	10.149	2822	2833	2857	rBV	480547	764468	46.44%	6.403%
81	10.484	2932	2937	2941	rBV2	535	478	0.03%	0.004%
82	10.506	2941	2944	2946	rVB3	503	305	0.02%	0.003%
83	10.558	2957	2960	2963	rBV	237	185	0.01%	0.002%
84	10.574	2963	2965	2966	rBV	334	169	0.01%	0.001%
85	10.619	2977	2979	2981	rBV2	145	92	0.01%	0.001%
86	10.635	2983	2984	2986	rVV	282	77	0.00%	0.001%
87	10.683	2997	2999	3003	rBV2	254	198	0.01%	0.002%
88	10.792	3030	3033	3035	rBV	383	248	0.02%	0.002%
89	10.831	3044	3045	3048	rVB2	328	86	0.01%	0.001%
90	10.972	3086	3089	3090	rBV	272	175	0.01%	0.001%
91	10.995	3095	3096	3100	rVV2	318	197	0.01%	0.002%
92	11.079	3120	3122	3126	rBV2	381	306	0.02%	0.003%
93	11.185	3144	3155	3182	rBV	623492	982051	59.66%	8.225%
94	11.558	3260	3271	3295	rBV	673882	1067397	64.85%	8.940%
95	12.027	3416	3417	3419	rBV	260	137	0.01%	0.001%
96	12.088	3434	3436	3442	rVB3	427	357	0.02%	0.003%
97	12.358	3518	3520	3525	rBV2	385	158	0.01%	0.001%
98	12.458	3547	3551	3554	rBV3	484	528	0.03%	0.004%
99	13.210	3777	3785	3793	rBV7	2945	4790	0.29%	0.040%
100	13.705	3937	3939	3943	rBV3	534	387	0.02%	0.003%




Sum of corrected areas: 11939194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034975.D
Acq On : 04 Apr 2024 13:57
Operator : SY/MD
Sample : P1965-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

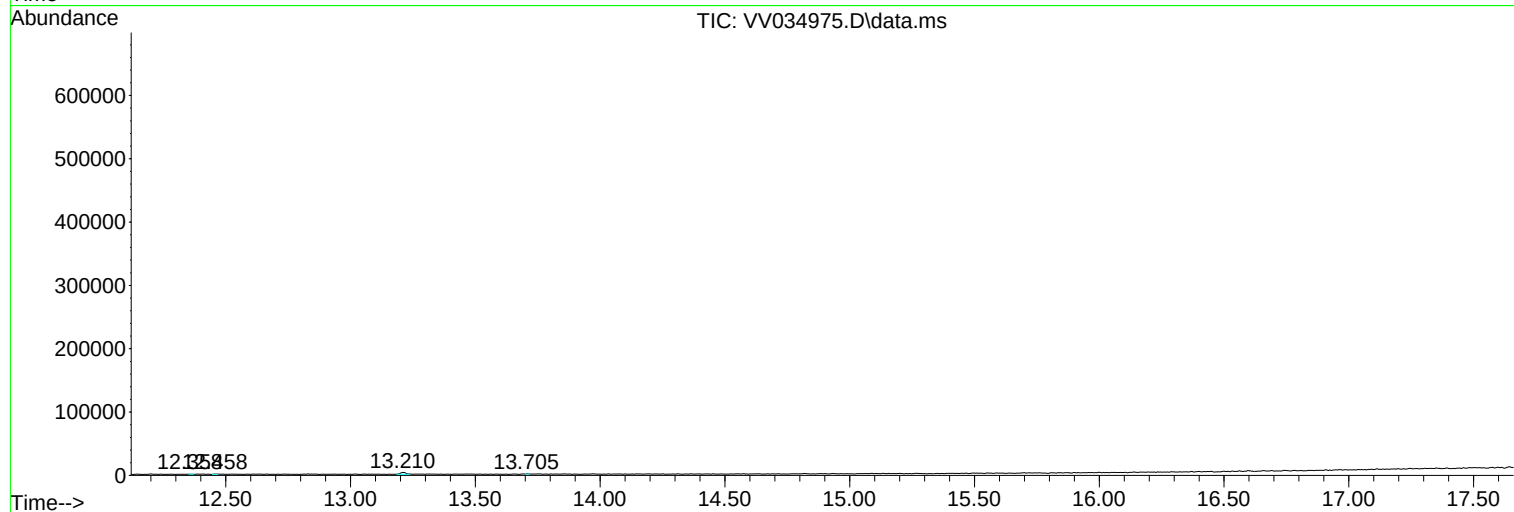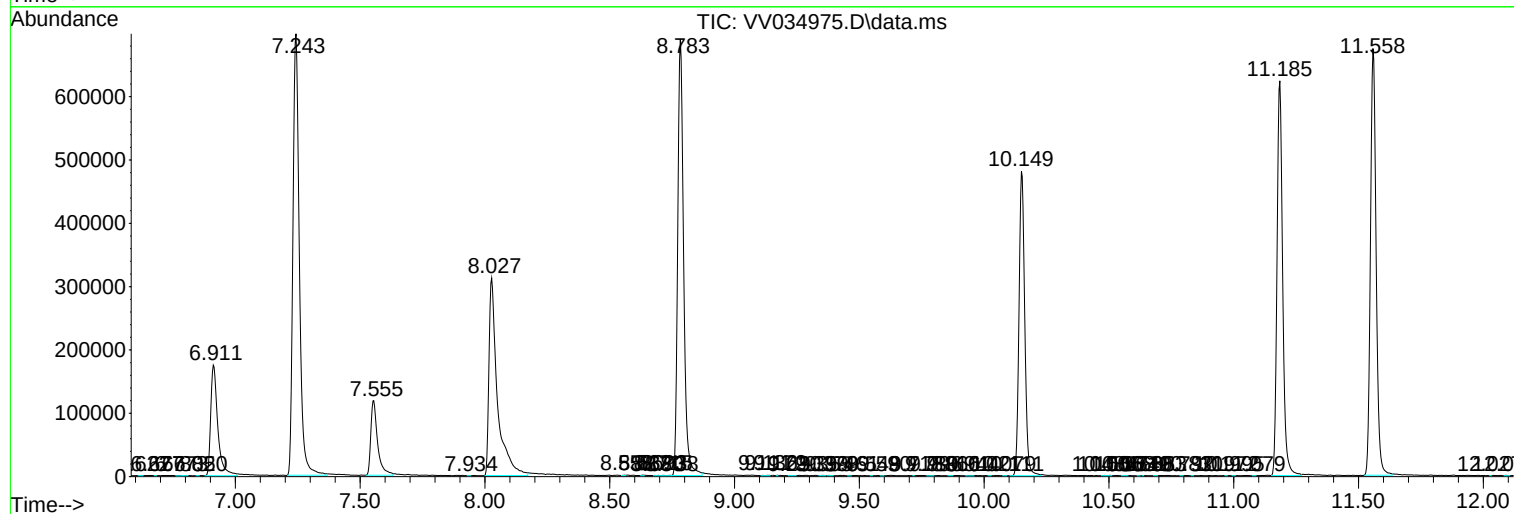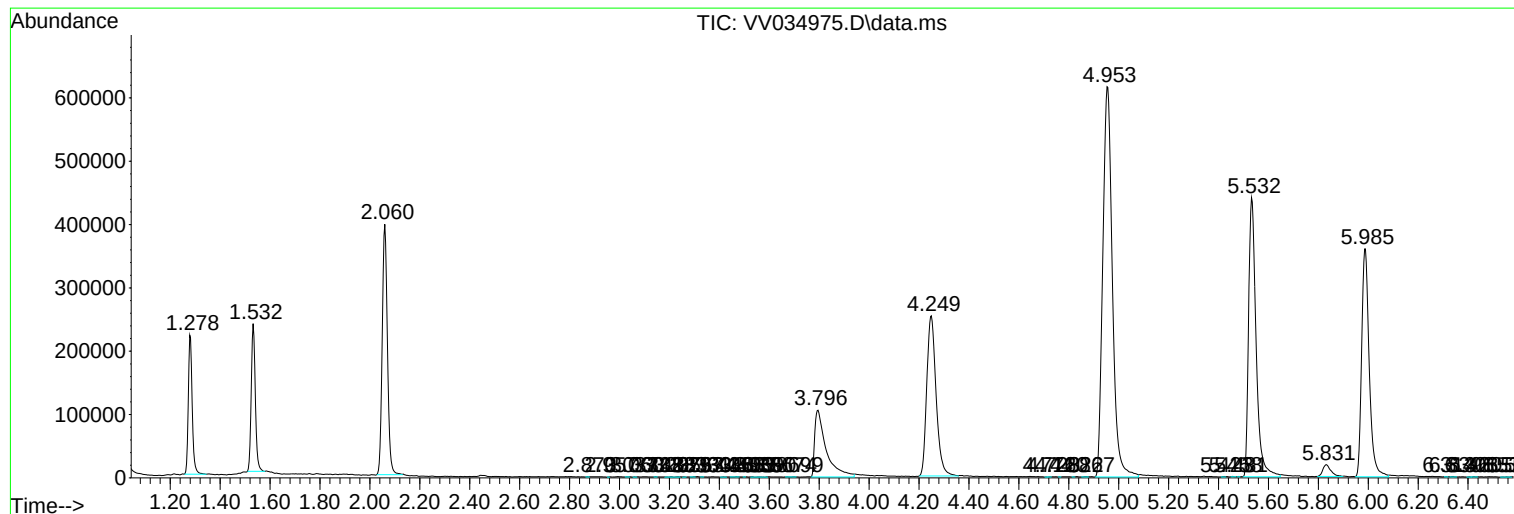

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034975.D
Acq On : 04 Apr 2024 13:57
Operator : SY/MD
Sample : P1965-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034975.D
Acq On : 04 Apr 2024 13:57
Operator : SY/MD
Sample : P1965-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------