

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034977.D
 Acq On : 04 Apr 2024 14:45
 Operator : SY/MD
 Sample : P1987-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	207209	221428	14.18%	1.927%
2	1.532	146	153	169	rVB	225453	253475	16.23%	2.206%
3	2.059	307	317	333	rBV	375080	541862	34.69%	4.716%
4	2.821	552	554	556	rBV	236	154	0.01%	0.001%
5	2.841	558	560	566	rBV4	316	290	0.02%	0.003%
6	2.905	578	580	581	rBV4	468	165	0.01%	0.001%
7	2.928	584	587	589	rBV2	394	258	0.02%	0.002%
8	2.973	598	601	603	rBV3	329	231	0.01%	0.002%
9	3.050	622	625	626	rBV	347	194	0.01%	0.002%
10	3.104	638	642	645	rBV2	371	232	0.01%	0.002%
11	3.127	645	649	651	rVB2	463	261	0.02%	0.002%
12	3.317	705	708	709	rBV2	366	191	0.01%	0.002%
13	3.349	716	718	722	rVB2	310	163	0.01%	0.001%
14	3.397	730	733	735	rVB	381	227	0.01%	0.002%
15	3.432	741	744	745	rBV	254	147	0.01%	0.001%
16	3.474	754	757	764	rVB2	431	312	0.02%	0.003%
17	3.539	772	777	779	rBV2	445	401	0.03%	0.003%
18	3.564	783	785	787	rBV	314	169	0.01%	0.001%
19	3.590	791	793	798	rVB3	268	218	0.01%	0.002%
20	3.616	798	801	803	rBV	356	260	0.02%	0.002%
21	3.654	811	813	816	rBV3	219	148	0.01%	0.001%
22	3.706	825	829	831	rVV2	546	329	0.02%	0.003%
23	3.719	831	833	837	rVB3	327	199	0.01%	0.002%
24	3.796	848	857	902	rBV	101575	321889	20.61%	2.801%
25	4.249	984	998	1022	rBV	239415	610234	39.07%	5.311%
26	4.702	1136	1139	1142	rVB3	419	245	0.02%	0.002%
27	4.751	1152	1154	1155	rBV	303	128	0.01%	0.001%
28	4.802	1167	1170	1172	rVB3	427	215	0.01%	0.002%
29	4.883	1192	1195	1198	rVB	486	260	0.02%	0.002%
30	4.953	1202	1217	1252	rBV2	589807	1562094	100.00%	13.594%
31	5.233	1301	1304	1305	rBV2	633	327	0.02%	0.003%
32	5.272	1314	1316	1320	rVB4	557	427	0.03%	0.004%
33	5.294	1320	1323	1325	rBV3	590	325	0.02%	0.003%
34	5.474	1376	1379	1381	rBV3	417	229	0.01%	0.002%
35	5.532	1386	1397	1429	rBV	427787	897672	57.47%	7.812%
36	5.831	1479	1490	1511	rBV3	11859	29109	1.86%	0.253%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034977.D
 Acq On : 04 Apr 2024 14:45
 Operator : SY/MD
 Sample : P1987-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1525	1538	1573	rBV	342731	724051	46.35%	6.301%
38	6.333	1644	1646	1648	rBV2	381	190	0.01%	0.002%
39	6.365	1652	1656	1657	rBV3	492	323	0.02%	0.003%
40	6.493	1693	1696	1702	rBV3	561	554	0.04%	0.005%
41	6.616	1731	1734	1737	rBV3	578	532	0.03%	0.005%
42	6.808	1792	1794	1797	rVB2	511	303	0.02%	0.003%
43	6.870	1810	1813	1816	rVB2	525	311	0.02%	0.003%
44	6.911	1816	1826	1849	rBV	167171	322565	20.65%	2.807%
45	7.149	1897	1900	1902	rBV4	652	433	0.03%	0.004%
46	7.243	1918	1929	1957	rBV	666114	1176688	75.33%	10.240%
47	7.503	2008	2010	2013	rBV2	464	308	0.02%	0.003%
48	7.554	2016	2026	2046	rBV	113331	210278	13.46%	1.830%
49	7.789	2095	2099	2101	rVB3	717	554	0.04%	0.005%
50	7.812	2101	2106	2109	rBV3	897	745	0.05%	0.006%
51	7.956	2147	2151	2152	rBV2	655	318	0.02%	0.003%
52	7.969	2152	2155	2157	rVB3	494	292	0.02%	0.003%
53	7.988	2158	2161	2164	rBV	335	234	0.01%	0.002%
54	8.027	2164	2173	2214	rBV2	300627	710830	45.50%	6.186%
55	8.583	2344	2346	2348	rBV3	333	178	0.01%	0.002%
56	8.657	2367	2369	2371	rBV2	361	178	0.01%	0.002%
57	8.693	2378	2380	2382	rBV	352	168	0.01%	0.001%
58	8.783	2396	2408	2440	rBV	671431	1108938	70.99%	9.651%
59	9.159	2524	2525	2528	rBV2	515	187	0.01%	0.002%
60	9.249	2551	2553	2556	rBV2	472	190	0.01%	0.002%
61	9.271	2556	2560	2563	rBV3	562	479	0.03%	0.004%
62	9.339	2577	2581	2582	rBV2	359	271	0.02%	0.002%
63	9.384	2593	2595	2598	rBV2	357	225	0.01%	0.002%
64	9.439	2608	2612	2613	rBV	462	266	0.02%	0.002%
65	9.513	2629	2635	2637	rBV2	363	298	0.02%	0.003%
66	9.529	2637	2640	2645	rVV	253	247	0.02%	0.002%
67	9.570	2651	2653	2655	rVB	455	148	0.01%	0.001%
68	9.612	2661	2666	2668	rBV2	464	374	0.02%	0.003%
69	9.763	2710	2713	2716	rBV3	412	297	0.02%	0.003%
70	9.779	2716	2718	2720	rVB2	329	139	0.01%	0.001%
71	9.818	2727	2730	2737	rVB3	470	588	0.04%	0.005%
72	9.857	2737	2742	2744	rBV2	621	477	0.03%	0.004%
73	9.882	2748	2750	2753	rBV2	237	154	0.01%	0.001%
74	10.088	2809	2814	2816	rBV2	476	443	0.03%	0.004%
75	10.149	2822	2833	2859	rBV	475209	759109	48.60%	6.606%
76	10.487	2936	2938	2943	rVB2	444	301	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034977.D
 Acq On : 04 Apr 2024 14:45
 Operator : SY/MD
 Sample : P1987-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.513	2943	2946	2948	rBV3	542	323	0.02%	0.003%
78	10.554	2955	2959	2961	rBV3	432	251	0.02%	0.002%
79	10.596	2969	2972	2974	rBV	183	145	0.01%	0.001%
80	10.654	2985	2990	2997	rVB2	633	723	0.05%	0.006%
81	10.696	2997	3003	3004	rBV2	587	522	0.03%	0.005%
82	10.789	3030	3032	3036	rVB2	365	194	0.01%	0.002%
83	10.876	3057	3059	3061	rBV	339	202	0.01%	0.002%
84	11.072	3117	3120	3123	rVB2	469	343	0.02%	0.003%
85	11.130	3132	3138	3144	rBV7	1553	2361	0.15%	0.021%
86	11.185	3144	3155	3178	rBV	600739	980511	62.77%	8.533%
87	11.561	3260	3272	3300	rBV	641111	1025449	65.65%	8.924%
88	12.027	3412	3417	3419	rBV3	682	631	0.04%	0.005%
89	12.117	3442	3445	3446	rBV	411	179	0.01%	0.002%
90	12.213	3473	3475	3476	rBV	484	208	0.01%	0.002%
91	12.274	3491	3494	3496	rVB	443	232	0.01%	0.002%
92	12.336	3508	3513	3514	rBV	395	361	0.02%	0.003%
93	12.381	3525	3527	3531	rVB	365	245	0.02%	0.002%
94	12.551	3578	3580	3581	rBV	396	126	0.01%	0.001%
95	13.207	3777	3784	3799	rVB7	4735	8639	0.55%	0.075%
96	13.268	3800	3803	3807	rBV	621	494	0.03%	0.004%
97	13.355	3825	3830	3833	rBV	485	464	0.03%	0.004%
98	13.432	3852	3854	3857	rBV3	467	248	0.02%	0.002%
99	13.599	3904	3906	3909	rBV	356	198	0.01%	0.002%
100	13.664	3923	3926	3927	rBV2	442	295	0.02%	0.003%




Sum of corrected areas: 11490976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034977.D
Acq On : 04 Apr 2024 14:45
Operator : SY/MD
Sample : P1987-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

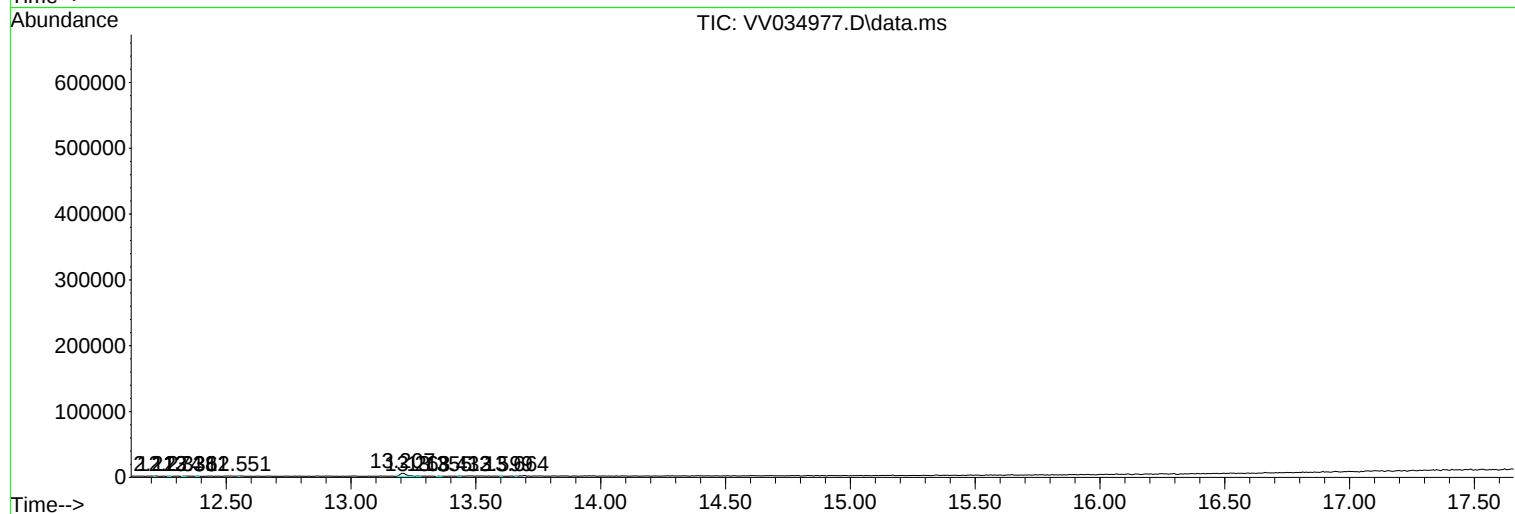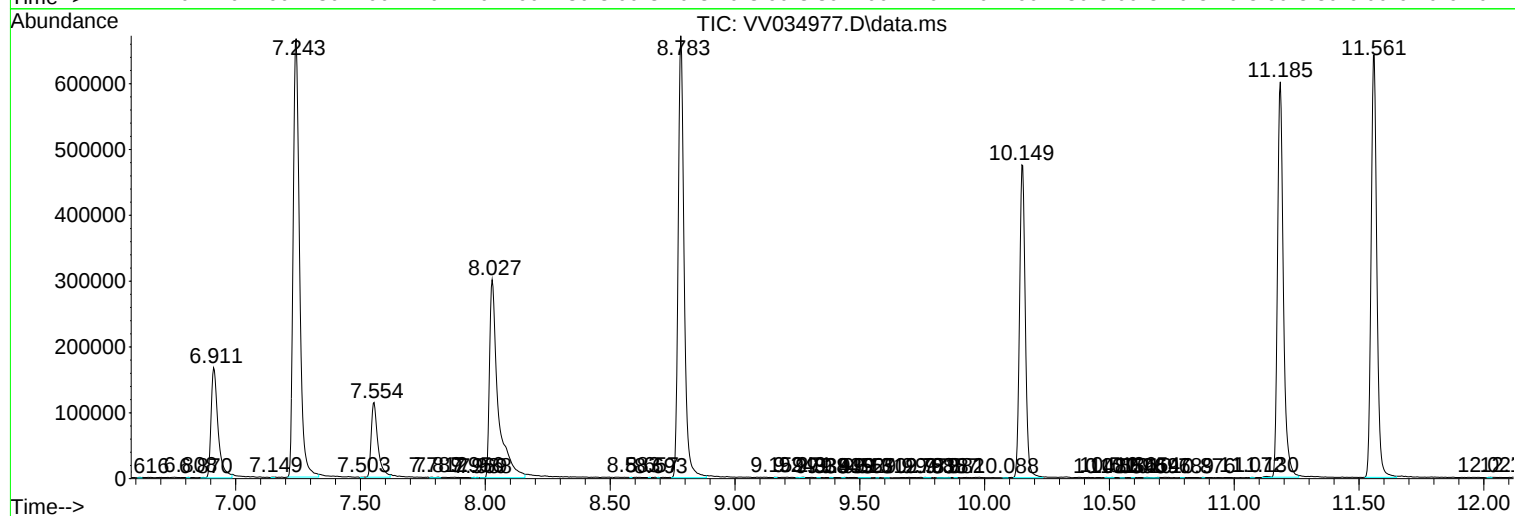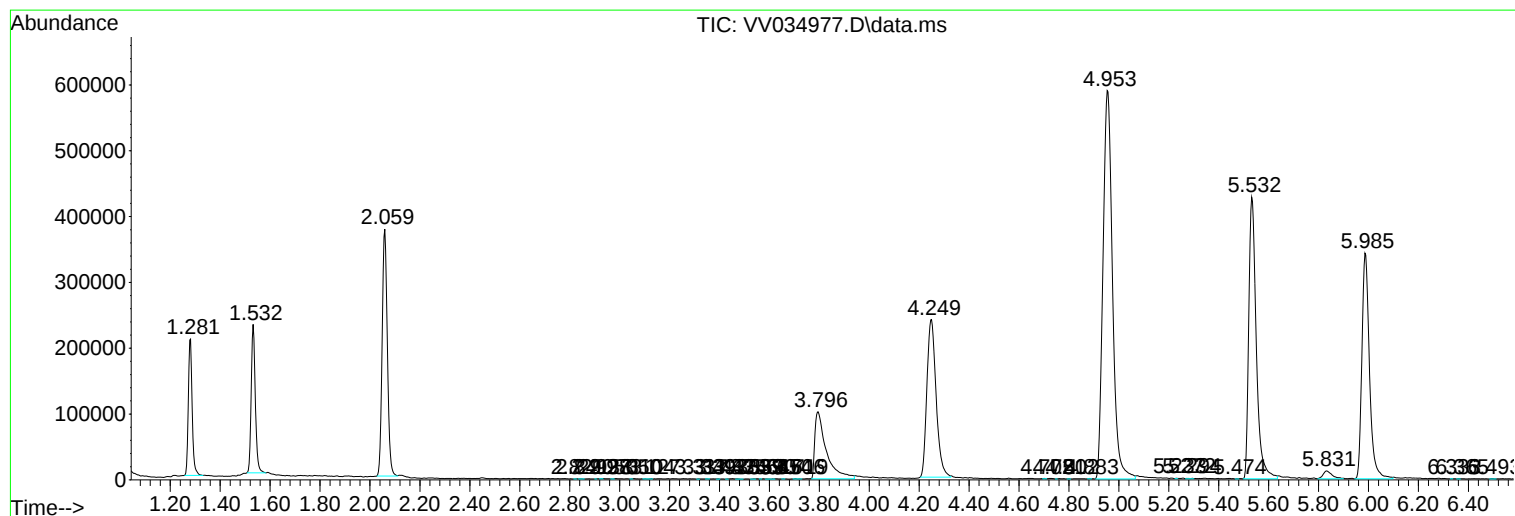

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034977.D
Acq On : 04 Apr 2024 14:45
Operator : SY/MD
Sample : P1987-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034977.D
Acq On : 04 Apr 2024 14:45
Operator : SY/MD
Sample : P1987-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------