

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034978.D
 Acq On : 04 Apr 2024 15:09
 Operator : SY/MD
 Sample : P1987-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	206993	217799	13.98%	1.924%
2	1.532	146	153	183	rVB	224931	277241	17.80%	2.449%
3	2.060	308	317	333	rVB	372126	534664	34.33%	4.723%
4	2.744	526	530	533	rBV2	416	334	0.02%	0.003%
5	2.812	550	551	552	rBV	287	108	0.01%	0.001%
6	2.844	557	561	563	rBV2	247	191	0.01%	0.002%
7	3.043	620	623	626	rBV2	300	234	0.02%	0.002%
8	3.063	626	629	631	rBV	198	158	0.01%	0.001%
9	3.127	647	649	652	rBV2	504	301	0.02%	0.003%
10	3.143	652	654	656	rBV	233	146	0.01%	0.001%
11	3.275	692	695	698	rBV2	442	265	0.02%	0.002%
12	3.333	709	713	716	rBV2	275	305	0.02%	0.003%
13	3.433	741	744	747	rVB	446	222	0.01%	0.002%
14	3.619	799	802	804	rBV	377	214	0.01%	0.002%
15	3.661	813	815	816	rBV	275	104	0.01%	0.001%
16	3.796	848	857	902	rBV	98532	314348	20.18%	2.777%
17	4.246	983	997	1030	rBV	237201	609648	39.14%	5.385%
18	4.474	1066	1068	1069	rBV	490	195	0.01%	0.002%
19	4.812	1166	1173	1175	rBV4	618	743	0.05%	0.007%
20	4.953	1201	1217	1262	rBV2	580719	1557501	100.00%	13.758%
21	5.272	1314	1316	1319	rBV	646	284	0.02%	0.003%
22	5.391	1351	1353	1357	rVB2	596	243	0.02%	0.002%
23	5.426	1362	1364	1369	rVB4	538	378	0.02%	0.003%
24	5.494	1380	1385	1386	rBV	662	487	0.03%	0.004%
25	5.532	1386	1397	1434	rVV	422330	888451	57.04%	7.848%
26	5.831	1480	1490	1502	rBV4	10807	24244	1.56%	0.214%
27	5.989	1525	1539	1571	rBV	340451	715291	45.93%	6.318%
28	6.262	1620	1624	1625	rBV2	614	407	0.03%	0.004%
29	6.342	1647	1649	1651	rBV2	505	224	0.01%	0.002%
30	6.378	1658	1660	1661	rBV	325	111	0.01%	0.001%
31	6.426	1673	1675	1677	rVB2	330	133	0.01%	0.001%
32	6.465	1685	1687	1690	rVB3	667	319	0.02%	0.003%
33	6.493	1690	1696	1698	rBV2	631	722	0.05%	0.006%
34	6.583	1722	1724	1725	rBV	180	64	0.00%	0.001%
35	6.593	1725	1727	1728	rVB2	240	73	0.00%	0.001%
36	6.603	1728	1730	1732	rBV2	272	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034978.D
 Acq On : 04 Apr 2024 15:09
 Operator : SY/MD
 Sample : P1987-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.686	1754	1756	1757	rBV	382	129	0.01%	0.001%
38	6.712	1763	1764	1765	rBV	286	90	0.01%	0.001%
39	6.802	1789	1792	1793	rBV	129	92	0.01%	0.001%
40	6.818	1793	1797	1799	rVV2	639	427	0.03%	0.004%
41	6.850	1804	1807	1809	rVB2	253	144	0.01%	0.001%
42	6.870	1809	1813	1815	rBV2	219	122	0.01%	0.001%
43	6.911	1815	1826	1857	rBV	161654	319683	20.53%	2.824%
44	7.172	1905	1907	1911	rVB4	918	515	0.03%	0.005%
45	7.243	1918	1929	1955	rBV	653589	1161482	74.57%	10.259%
46	7.555	2016	2026	2043	rBV	108399	199146	12.79%	1.759%
47	7.854	2117	2119	2120	rBV	550	227	0.01%	0.002%
48	8.027	2163	2173	2223	rBV2	287000	691959	44.43%	6.112%
49	8.397	2286	2288	2290	rBV3	608	311	0.02%	0.003%
50	8.551	2332	2336	2338	rBV4	673	494	0.03%	0.004%
51	8.606	2350	2353	2358	rVB5	875	667	0.04%	0.006%
52	8.635	2358	2362	2364	rBV3	747	542	0.03%	0.005%
53	8.783	2396	2408	2441	rBV	650729	1093345	70.20%	9.658%
54	9.001	2474	2476	2479	rBV3	762	428	0.03%	0.004%
55	9.095	2501	2505	2507	rBV	527	324	0.02%	0.003%
56	9.120	2510	2513	2514	rBV2	430	209	0.01%	0.002%
57	9.175	2527	2530	2535	rBV3	631	510	0.03%	0.005%
58	9.233	2546	2548	2552	rVB2	805	423	0.03%	0.004%
59	9.429	2606	2609	2611	rBV2	382	213	0.01%	0.002%
60	9.509	2631	2634	2636	rBV2	424	281	0.02%	0.002%
61	9.587	2649	2658	2662	rBV3	466	726	0.05%	0.006%
62	9.632	2668	2672	2674	rBV	270	225	0.01%	0.002%
63	9.641	2674	2675	2678	rVV	424	195	0.01%	0.002%
64	9.731	2701	2703	2705	rBV	257	121	0.01%	0.001%
65	9.802	2723	2725	2727	rBV	235	120	0.01%	0.001%
66	9.841	2736	2737	2739	rVB	276	106	0.01%	0.001%
67	9.905	2753	2757	2758	rBV	221	190	0.01%	0.002%
68	9.956	2770	2773	2775	rBV2	374	207	0.01%	0.002%
69	9.998	2783	2786	2788	rBV3	425	216	0.01%	0.002%
70	10.072	2806	2809	2812	rBV2	529	278	0.02%	0.002%
71	10.088	2812	2814	2816	rBV	388	210	0.01%	0.002%
72	10.149	2821	2833	2857	rBV	471911	749190	48.10%	6.618%
73	10.316	2881	2885	2887	rBV3	1572	1103	0.07%	0.010%
74	10.458	2924	2929	2930	rBV	403	317	0.02%	0.003%
75	10.532	2949	2952	2956	rVB2	489	325	0.02%	0.003%
76	10.554	2957	2959	2961	rVV2	225	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034978.D
 Acq On : 04 Apr 2024 15:09
 Operator : SY/MD
 Sample : P1987-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.599	2969	2973	2975	rBV2	404	334	0.02%	0.003%
78	10.635	2983	2984	2987	rBV	277	188	0.01%	0.002%
79	10.693	3000	3002	3006	rVB3	372	233	0.01%	0.002%
80	10.770	3025	3026	3027	rBV3	375	103	0.01%	0.001%
81	10.815	3037	3040	3043	rVB2	461	319	0.02%	0.003%
82	10.879	3057	3060	3062	rBV3	231	190	0.01%	0.002%
83	10.921	3071	3073	3074	rBV2	288	73	0.00%	0.001%
84	10.931	3074	3076	3078	rBV	289	162	0.01%	0.001%
85	10.976	3088	3090	3095	rBV2	249	217	0.01%	0.002%
86	11.027	3103	3106	3109	rBV2	481	424	0.03%	0.004%
87	11.085	3122	3124	3125	rBV	231	94	0.01%	0.001%
88	11.107	3129	3131	3132	rBV	203	92	0.01%	0.001%
89	11.185	3144	3155	3181	rBV	589985	936546	60.13%	8.273%
90	11.558	3260	3271	3296	rBV	631607	1004555	64.50%	8.873%
91	12.033	3417	3419	3422	rBV2	387	153	0.01%	0.001%
92	12.207	3471	3473	3476	rVB2	416	201	0.01%	0.002%
93	12.268	3488	3492	3493	rBV2	523	385	0.02%	0.003%
94	12.818	3660	3663	3665	rBV	551	274	0.02%	0.002%
95	12.873	3677	3680	3685	rVB3	500	405	0.03%	0.004%
96	13.043	3731	3733	3737	rBV3	495	238	0.02%	0.002%
97	13.059	3737	3738	3740	rBV	255	80	0.01%	0.001%
98	13.204	3780	3783	3796	rVB6	2536	3695	0.24%	0.033%
99	13.332	3822	3823	3825	rBV2	421	188	0.01%	0.002%
100	14.255	4108	4110	4114	rBV3	445	242	0.02%	0.002%




Sum of corrected areas: 11321094

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034978.D
Acq On : 04 Apr 2024 15:09
Operator : SY/MD
Sample : P1987-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

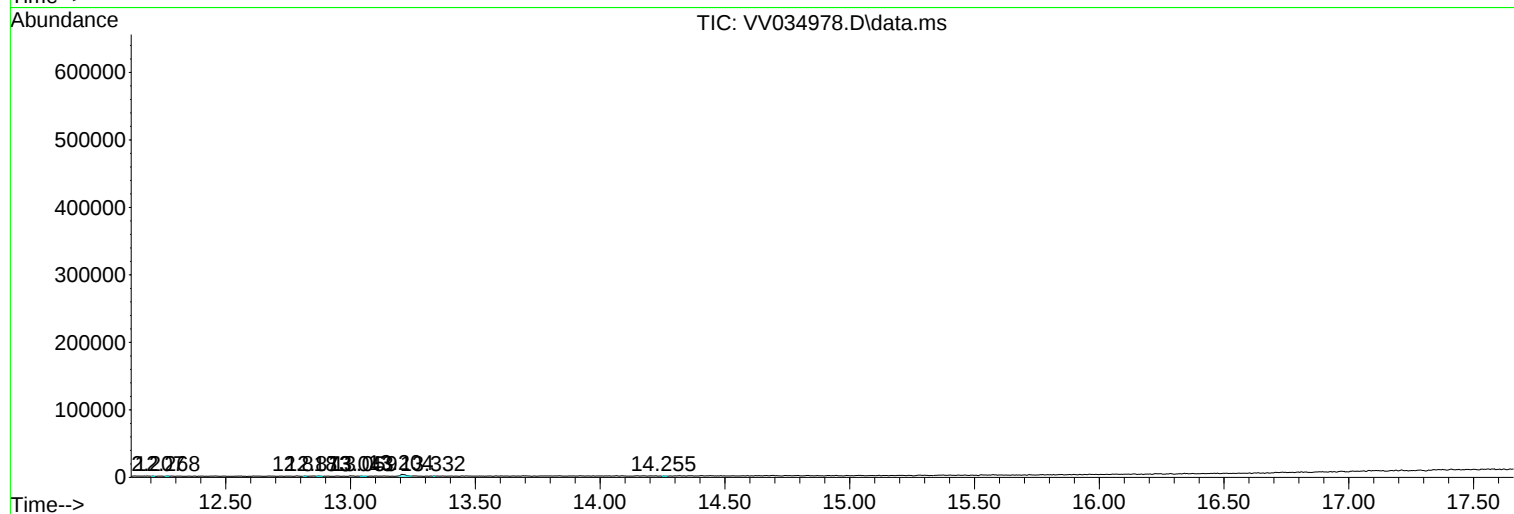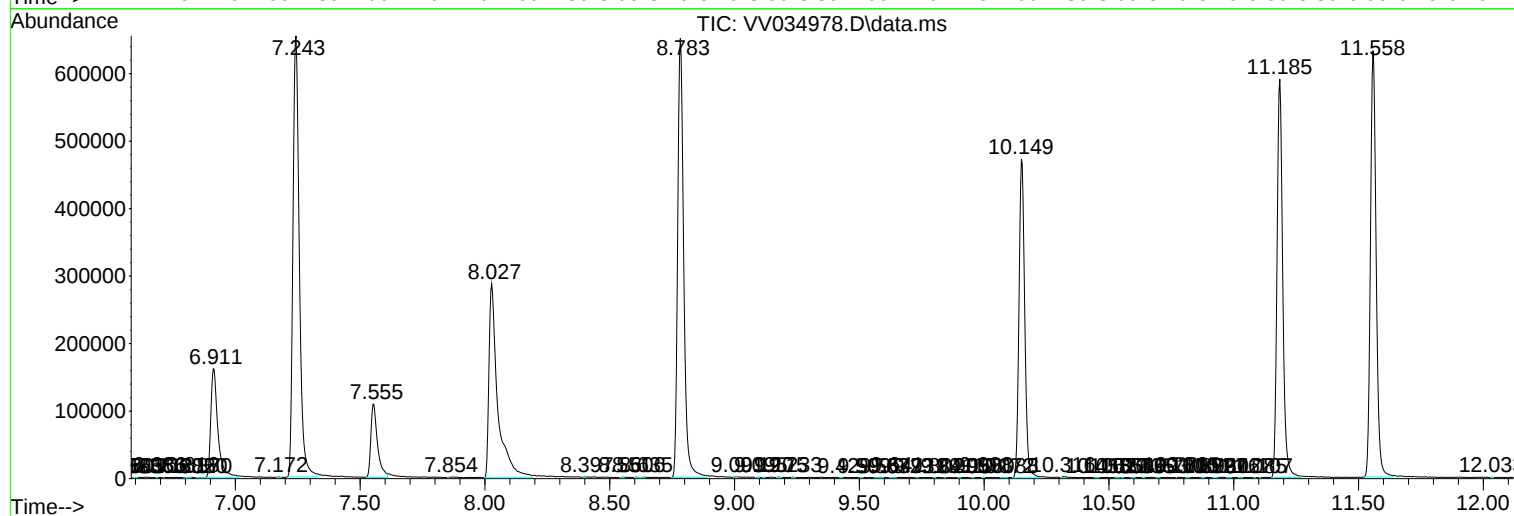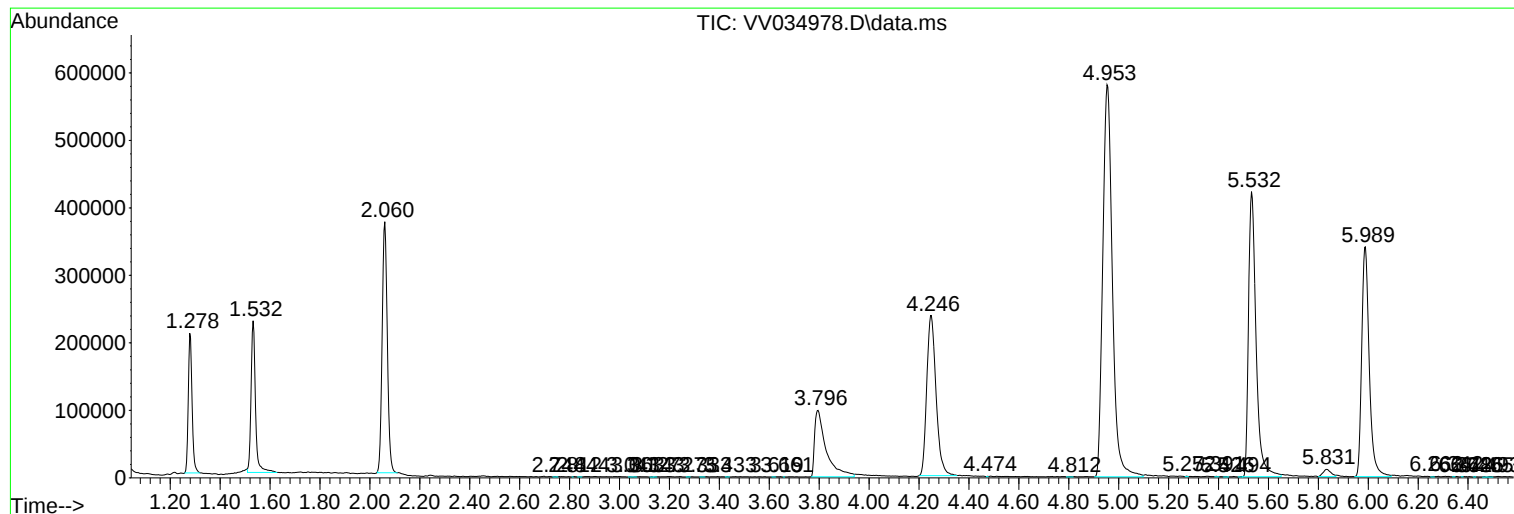

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034978.D
Acq On : 04 Apr 2024 15:09
Operator : SY/MD
Sample : P1987-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034978.D
Acq On : 04 Apr 2024 15:09
Operator : SY/MD
Sample : P1987-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------