

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034979.D
 Acq On : 04 Apr 2024 15:33
 Operator : SY/MD
 Sample : P1987-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	209710	225621	14.40%	1.963%
2	1.532	146	153	176	rVB	232851	283903	18.12%	2.470%
3	2.059	307	317	333	rBV	380525	547991	34.98%	4.768%
4	2.879	570	572	575	rBV3	525	378	0.02%	0.003%
5	2.966	596	599	603	rBV	542	405	0.03%	0.004%
6	3.034	618	620	621	rBV	433	191	0.01%	0.002%
7	3.098	638	640	642	rVB	326	85	0.01%	0.001%
8	3.140	650	653	656	rBV2	280	169	0.01%	0.001%
9	3.182	661	666	667	rBV	389	302	0.02%	0.003%
10	3.371	723	725	727	rBV	295	162	0.01%	0.001%
11	3.384	727	729	734	rVB3	481	337	0.02%	0.003%
12	3.420	737	740	742	rBV2	384	224	0.01%	0.002%
13	3.477	757	758	759	rBV2	282	77	0.00%	0.001%
14	3.558	779	783	786	rBV3	385	394	0.03%	0.003%
15	3.577	786	789	795	rVB2	337	329	0.02%	0.003%
16	3.606	795	798	802	rBV3	244	212	0.01%	0.002%
17	3.657	811	814	816	rBV2	253	169	0.01%	0.001%
18	3.719	829	833	835	rBV3	431	270	0.02%	0.002%
19	3.757	843	845	847	rBV2	236	107	0.01%	0.001%
20	3.793	847	856	901	rBV	105955	328594	20.98%	2.859%
21	4.246	983	997	1029	rBV	243919	627077	40.03%	5.456%
22	4.657	1123	1125	1129	rVB3	337	245	0.02%	0.002%
23	4.677	1129	1131	1135	rBV	339	240	0.02%	0.002%
24	4.744	1150	1152	1154	rBV	564	253	0.02%	0.002%
25	4.773	1156	1161	1165	rBV	394	351	0.02%	0.003%
26	4.796	1165	1168	1170	rBV3	444	281	0.02%	0.002%
27	4.860	1185	1188	1189	rBV	451	215	0.01%	0.002%
28	4.956	1201	1218	1255	rBV2	588638	1566525	100.00%	13.629%
29	5.407	1356	1358	1359	rBV2	334	110	0.01%	0.001%
30	5.464	1374	1376	1377	rBV2	519	211	0.01%	0.002%
31	5.532	1386	1397	1432	rBV	419428	890410	56.84%	7.747%
32	5.985	1525	1538	1570	rBV	350337	732872	46.78%	6.376%
33	6.352	1649	1652	1654	rBV3	675	433	0.03%	0.004%
34	6.384	1661	1662	1665	rBV2	468	180	0.01%	0.002%
35	6.442	1675	1680	1683	rBV4	626	670	0.04%	0.006%
36	6.542	1708	1711	1712	rBV	243	99	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034979.D
 Acq On : 04 Apr 2024 15:33
 Operator : SY/MD
 Sample : P1987-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.554	1712	1715	1716	rBV3	304	150	0.01%	0.001%
38	6.625	1731	1737	1739	rBV2	638	529	0.03%	0.005%
39	6.673	1748	1752	1754	rBV3	417	229	0.01%	0.002%
40	6.735	1769	1771	1773	rBV3	631	342	0.02%	0.003%
41	6.773	1780	1783	1787	rBV2	287	252	0.02%	0.002%
42	6.799	1789	1791	1797	rVB4	422	405	0.03%	0.004%
43	6.844	1802	1805	1807	rBV	533	333	0.02%	0.003%
44	6.911	1816	1826	1858	rBV	167734	327603	20.91%	2.850%
45	7.117	1889	1890	1895	rBV2	481	306	0.02%	0.003%
46	7.243	1918	1929	1961	rBV	662580	1189006	75.90%	10.344%
47	7.554	2016	2026	2054	rBV	112897	216197	13.80%	1.881%
48	7.921	2138	2140	2146	rVB3	610	482	0.03%	0.004%
49	7.947	2146	2148	2153	rBV4	435	426	0.03%	0.004%
50	7.992	2159	2162	2163	rBV	221	110	0.01%	0.001%
51	8.027	2164	2173	2219	rBV2	315428	718720	45.88%	6.253%
52	8.529	2327	2329	2331	rBV2	584	346	0.02%	0.003%
53	8.622	2356	2358	2360	rBV3	484	179	0.01%	0.002%
54	8.683	2376	2377	2378	rBV3	349	121	0.01%	0.001%
55	8.783	2396	2408	2436	rBV	668285	1096535	70.00%	9.540%
56	9.185	2529	2533	2536	rBV3	512	439	0.03%	0.004%
57	9.307	2568	2571	2575	rBV	545	398	0.03%	0.003%
58	9.361	2584	2588	2592	rBV3	554	500	0.03%	0.004%
59	9.532	2639	2641	2644	rBV2	364	215	0.01%	0.002%
60	9.587	2654	2658	2659	rBV	448	267	0.02%	0.002%
61	9.651	2673	2678	2679	rBV	350	212	0.01%	0.002%
62	9.677	2684	2686	2687	rBV	342	135	0.01%	0.001%
63	9.715	2693	2698	2700	rBV3	457	437	0.03%	0.004%
64	9.750	2708	2709	2711	rBV	224	120	0.01%	0.001%
65	9.850	2738	2740	2744	rVB2	444	252	0.02%	0.002%
66	9.873	2744	2747	2748	rBV2	369	241	0.02%	0.002%
67	9.953	2769	2772	2777	rVB2	422	316	0.02%	0.003%
68	10.001	2784	2787	2790	rBV3	443	333	0.02%	0.003%
69	10.033	2794	2797	2799	rBV2	245	160	0.01%	0.001%
70	10.152	2822	2834	2861	rBV	471561	757562	48.36%	6.591%
71	10.503	2941	2943	2947	rBV2	414	223	0.01%	0.002%
72	10.728	3008	3013	3018	rBV3	466	479	0.03%	0.004%
73	10.767	3023	3025	3027	rBV	308	112	0.01%	0.001%
74	10.779	3027	3029	3031	rBV	423	215	0.01%	0.002%
75	10.837	3045	3047	3055	rBV2	410	382	0.02%	0.003%
76	10.905	3066	3068	3070	rBV2	399	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034979.D
 Acq On : 04 Apr 2024 15:33
 Operator : SY/MD
 Sample : P1987-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	10.943	3078	3080	3082	rVB2	256	79	0.01%	0.001%
78	10.963	3083	3086	3091	rVB3	423	339	0.02%	0.003%
79	11.001	3096	3098	3104	rBV3	395	339	0.02%	0.003%
80	11.123	3133	3136	3138	rBV2	566	375	0.02%	0.003%
81	11.185	3144	3155	3185	rBV	593742	938460	59.91%	8.165%
82	11.558	3259	3271	3299	rBV	636922	1022744	65.29%	8.898%
83	11.969	3397	3399	3403	rVB2	505	239	0.02%	0.002%
84	12.127	3446	3448	3453	rBV2	416	340	0.02%	0.003%
85	13.056	3733	3737	3740	rBV2	456	327	0.02%	0.003%
86	13.172	3769	3773	3774	rBV	487	374	0.02%	0.003%
87	13.207	3779	3784	3795	rVV6	2752	4534	0.29%	0.039%
88	13.451	3856	3860	3862	rBV2	546	439	0.03%	0.004%




Sum of corrected areas: 11494103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034979.D
Acq On : 04 Apr 2024 15:33
Operator : SY/MD
Sample : P1987-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

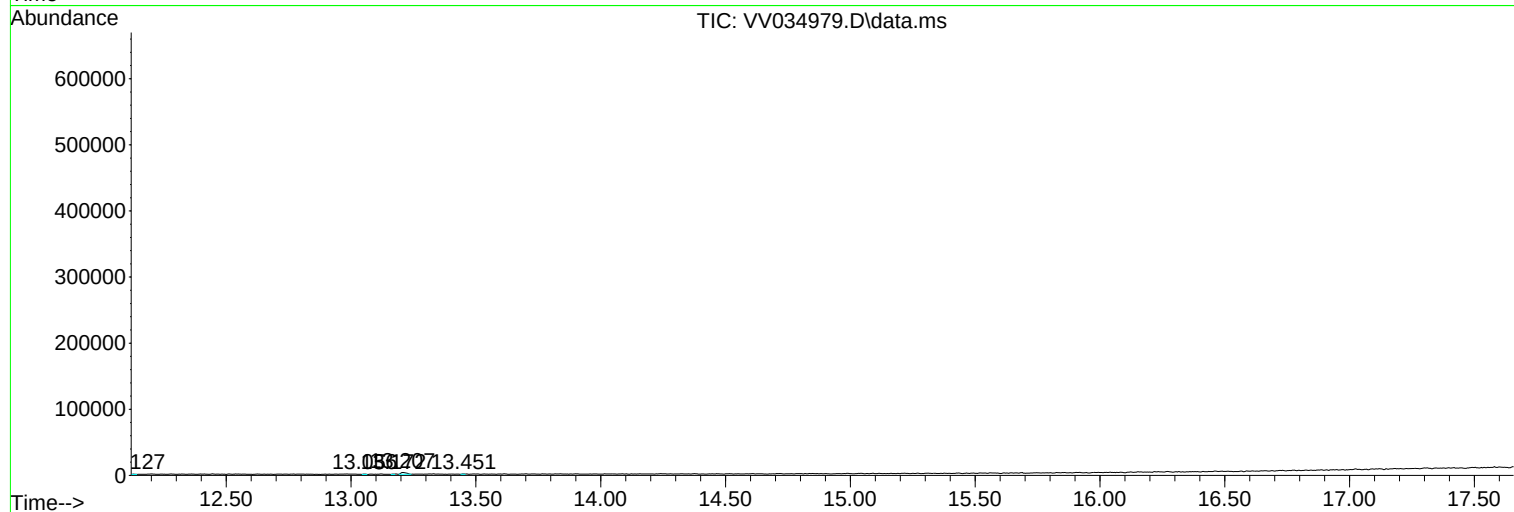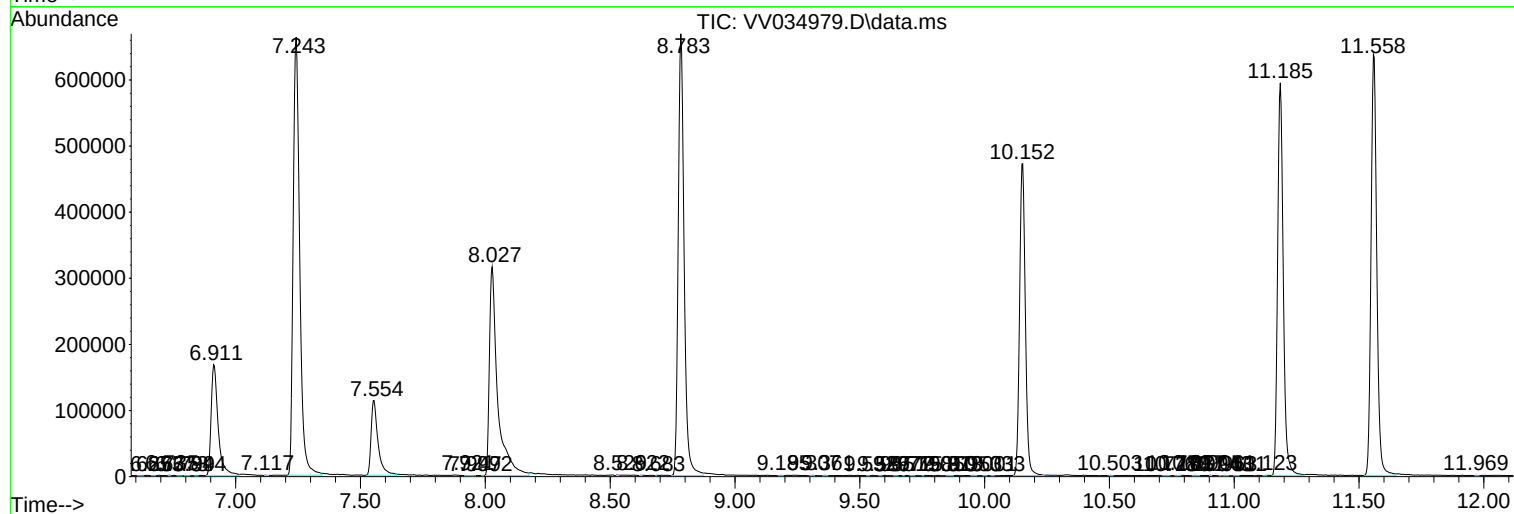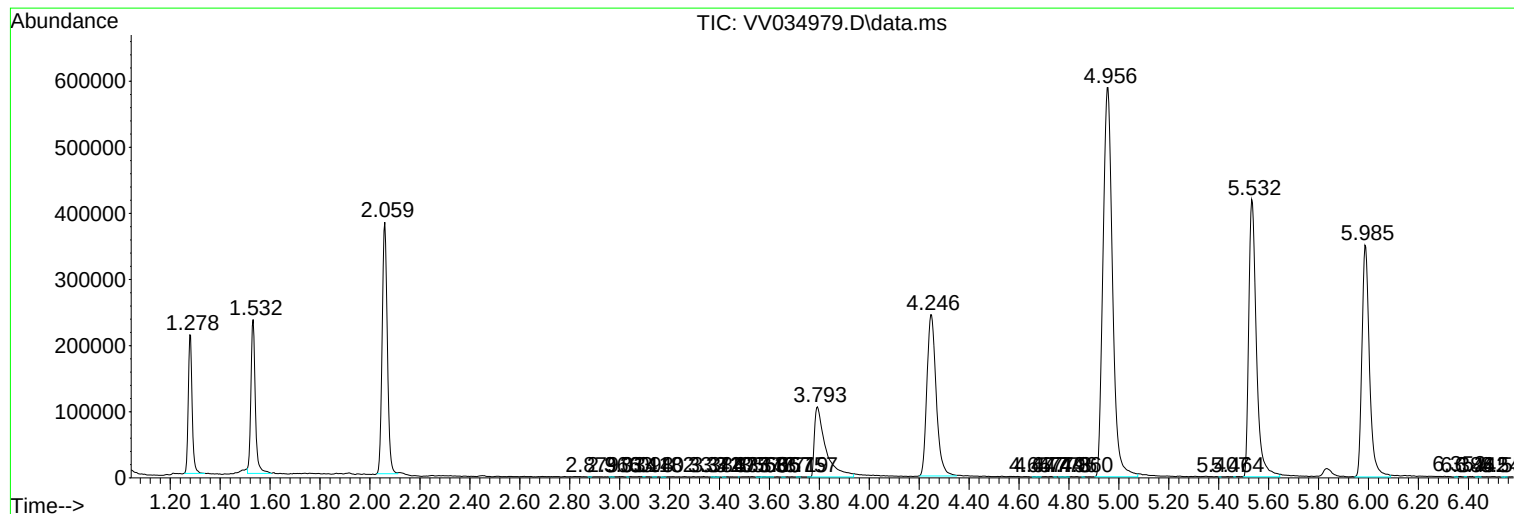

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034979.D
Acq On : 04 Apr 2024 15:33
Operator : SY/MD
Sample : P1987-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034979.D
Acq On : 04 Apr 2024 15:33
Operator : SY/MD
Sample : P1987-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------