

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034980.D
 Acq On : 04 Apr 2024 15:57
 Operator : SY/MD
 Sample : P1987-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rBV	203535	217573	14.00%	1.891%
2	1.532	146	153	178	rVB	222769	264560	17.02%	2.299%
3	2.060	307	317	335	rBV	366183	531721	34.21%	4.621%
4	2.584	476	480	481	rBV2	440	314	0.02%	0.003%
5	2.642	495	498	502	rBV2	503	381	0.02%	0.003%
6	2.748	529	531	536	rBV3	479	286	0.02%	0.002%
7	2.880	570	572	575	rBV2	324	113	0.01%	0.001%
8	2.995	606	608	610	rVB2	451	191	0.01%	0.002%
9	3.011	611	613	617	rVB3	494	279	0.02%	0.002%
10	3.034	617	620	621	rBV	466	234	0.02%	0.002%
11	3.066	628	630	633	rBV	534	277	0.02%	0.002%
12	3.166	659	661	665	rBV2	350	187	0.01%	0.002%
13	3.204	671	673	674	rBV2	268	140	0.01%	0.001%
14	3.294	699	701	704	rBV	286	122	0.01%	0.001%
15	3.333	707	713	715	rVV4	542	431	0.03%	0.004%
16	3.388	725	730	735	rBV3	489	649	0.04%	0.006%
17	3.462	749	753	756	rBV	407	280	0.02%	0.002%
18	3.478	756	758	759	rBV	330	128	0.01%	0.001%
19	3.487	759	761	764	rBV	255	180	0.01%	0.002%
20	3.600	793	796	800	rVV2	385	306	0.02%	0.003%
21	3.645	806	810	813	rBV2	291	215	0.01%	0.002%
22	3.658	813	814	818	rBV2	344	164	0.01%	0.001%
23	3.796	846	857	898	rBV	105292	335711	21.60%	2.918%
24	4.246	983	997	1028	rBV	239761	620247	39.91%	5.391%
25	4.693	1134	1136	1139	rVB2	358	122	0.01%	0.001%
26	4.838	1178	1181	1182	rBV	268	171	0.01%	0.001%
27	4.953	1202	1217	1261	rBV2	584830	1554127	100.00%	13.507%
28	5.532	1386	1397	1433	rBV	434509	912282	58.70%	7.929%
29	5.834	1482	1491	1509	rVB5	11631	27166	1.75%	0.236%
30	5.941	1521	1524	1526	rBV2	532	341	0.02%	0.003%
31	5.986	1526	1538	1565	rBV	344434	720796	46.38%	6.265%
32	6.307	1636	1638	1640	rBV	601	279	0.02%	0.002%
33	6.342	1646	1649	1654	rVB3	519	385	0.02%	0.003%
34	6.375	1657	1659	1662	rVB2	604	363	0.02%	0.003%
35	6.394	1662	1665	1668	rBV2	421	270	0.02%	0.002%
36	6.432	1674	1677	1680	rBV3	642	446	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034980.D
 Acq On : 04 Apr 2024 15:57
 Operator : SY/MD
 Sample : P1987-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.465	1684	1687	1690	rBV2	295	278	0.02%	0.002%
38	6.522	1703	1705	1711	rBV3	328	414	0.03%	0.004%
39	6.641	1737	1742	1744	rBV2	515	500	0.03%	0.004%
40	6.670	1748	1751	1753	rBV2	441	291	0.02%	0.003%
41	6.703	1759	1761	1766	rBV3	463	337	0.02%	0.003%
42	6.783	1782	1786	1789	rVV4	511	381	0.02%	0.003%
43	6.802	1789	1792	1794	rVV2	368	200	0.01%	0.002%
44	6.912	1814	1826	1854	rBV	165586	328402	21.13%	2.854%
45	7.243	1918	1929	1958	rBV	651693	1165087	74.97%	10.126%
46	7.555	2016	2026	2058	rBV	113158	218298	14.05%	1.897%
47	7.944	2143	2147	2148	rBV2	596	472	0.03%	0.004%
48	7.973	2153	2156	2159	rBV3	561	466	0.03%	0.004%
49	8.027	2164	2173	2221	rBV2	315013	735814	47.35%	6.395%
50	8.545	2330	2334	2335	rBV2	660	404	0.03%	0.004%
51	8.715	2385	2387	2391	rVB	486	265	0.02%	0.002%
52	8.735	2391	2393	2396	rBV3	527	336	0.02%	0.003%
53	8.783	2397	2408	2437	rBV	675673	1114478	71.71%	9.686%
54	9.130	2514	2516	2521	rVB3	588	394	0.03%	0.003%
55	9.159	2521	2525	2527	rBV3	422	330	0.02%	0.003%
56	9.191	2533	2535	2536	rBV2	351	142	0.01%	0.001%
57	9.246	2547	2552	2554	rBV3	453	336	0.02%	0.003%
58	9.301	2565	2569	2572	rBV3	413	337	0.02%	0.003%
59	9.429	2605	2609	2613	rBV2	370	344	0.02%	0.003%
60	9.455	2615	2617	2620	rBV2	308	172	0.01%	0.001%
61	9.487	2625	2627	2630	rVV2	452	189	0.01%	0.002%
62	9.564	2648	2651	2653	rBV	296	188	0.01%	0.002%
63	9.596	2658	2661	2662	rBV2	335	169	0.01%	0.001%
64	9.635	2671	2673	2675	rVB	327	103	0.01%	0.001%
65	9.738	2700	2705	2709	rBV2	566	496	0.03%	0.004%
66	9.773	2713	2716	2719	rVB2	630	402	0.03%	0.003%
67	9.847	2735	2739	2742	rBV2	363	328	0.02%	0.003%
68	9.866	2743	2745	2749	rVV2	288	212	0.01%	0.002%
69	9.911	2757	2759	2762	rVB3	396	164	0.01%	0.001%
70	9.976	2777	2779	2781	rBV2	345	177	0.01%	0.002%
71	10.063	2803	2806	2810	rBV2	205	148	0.01%	0.001%
72	10.101	2816	2818	2821	rVB	386	172	0.01%	0.001%
73	10.149	2821	2833	2857	rBV	477287	764574	49.20%	6.645%
74	10.352	2894	2896	2899	rVB2	558	290	0.02%	0.003%
75	10.371	2899	2902	2909	rVB5	466	537	0.03%	0.005%
76	10.403	2909	2912	2916	rBV3	368	307	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034980.D
 Acq On : 04 Apr 2024 15:57
 Operator : SY/MD
 Sample : P1987-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.464	2928	2931	2933	rBV2	586	309	0.02%	0.003%
78	10.641	2982	2986	2988	rBV2	400	304	0.02%	0.003%
79	10.680	2996	2998	2999	rBV	348	178	0.01%	0.002%
80	10.725	3010	3012	3015	rBV	374	262	0.02%	0.002%
81	10.857	3050	3053	3058	rVB2	473	528	0.03%	0.005%
82	10.879	3058	3060	3062	rBV	280	162	0.01%	0.001%
83	10.953	3081	3083	3087	rVB2	345	194	0.01%	0.002%
84	10.989	3092	3094	3097	rVB2	474	234	0.02%	0.002%
85	11.185	3143	3155	3179	rBV	604722	953512	61.35%	8.287%
86	11.464	3239	3242	3244	rBV2	605	411	0.03%	0.004%
87	11.516	3255	3258	3259	rBV2	807	494	0.03%	0.004%
88	11.558	3259	3271	3295	rVV	641963	1017897	65.50%	8.847%
89	11.992	3405	3406	3410	rBV2	347	182	0.01%	0.002%
90	12.098	3436	3439	3442	rBV2	396	294	0.02%	0.003%
91	12.236	3480	3482	3483	rBV	400	153	0.01%	0.001%
92	12.278	3494	3495	3500	rVB2	523	293	0.02%	0.003%
93	12.313	3503	3506	3511	rVB	466	309	0.02%	0.003%
94	12.439	3543	3545	3550	rVB3	789	438	0.03%	0.004%
95	12.461	3550	3552	3554	rVB2	437	114	0.01%	0.001%
96	12.866	3677	3678	3679	rBV2	299	113	0.01%	0.001%
97	12.911	3690	3692	3696	rVB2	382	164	0.01%	0.001%
98	12.931	3696	3698	3700	rBV2	585	331	0.02%	0.003%
99	13.307	3813	3815	3818	rBV2	342	234	0.02%	0.002%
100	13.455	3858	3861	3862	rBV	645	302	0.02%	0.003%




Sum of corrected areas: 11505783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034980.D
Acq On : 04 Apr 2024 15:57
Operator : SY/MD
Sample : P1987-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

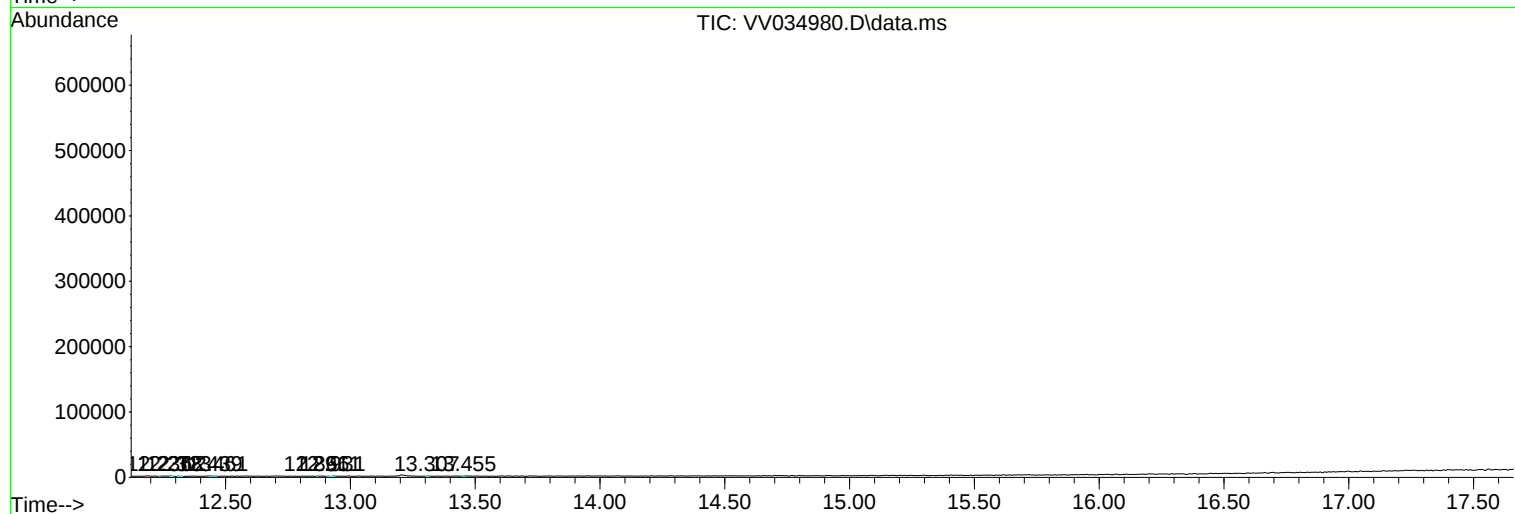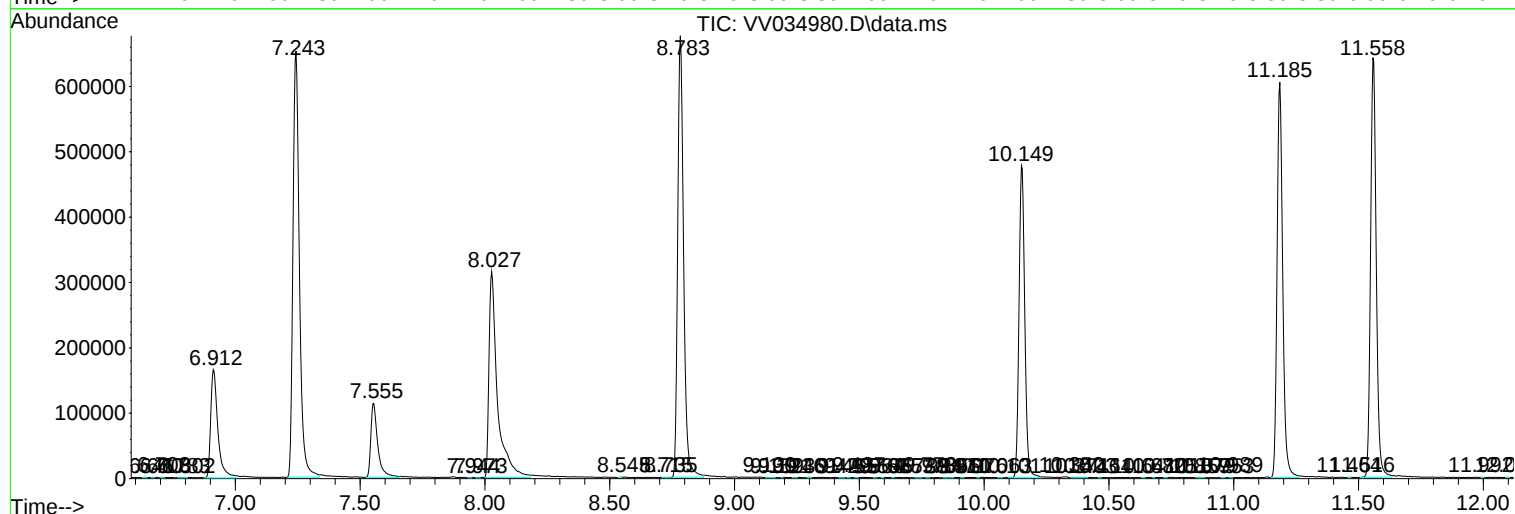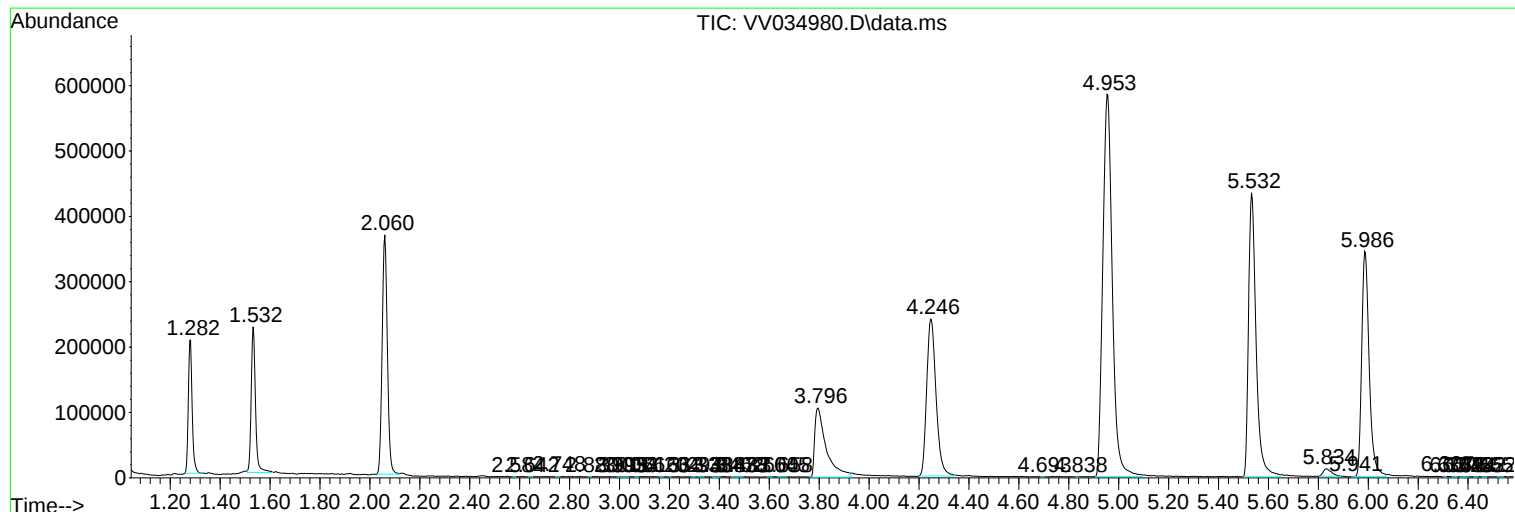

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034980.D
Acq On : 04 Apr 2024 15:57
Operator : SY/MD
Sample : P1987-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034980.D
Acq On : 04 Apr 2024 15:57
Operator : SY/MD
Sample : P1987-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------