

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034981.D
 Acq On : 04 Apr 2024 16:21
 Operator : SY/MD
 Sample : P1987-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	203814	217304	14.05%	1.908%
2	1.532	146	153	170	rVB	208618	240956	15.58%	2.116%
3	2.060	307	317	335	rBV	365750	532847	34.46%	4.679%
4	2.664	503	505	507	rBV	497	342	0.02%	0.003%
5	2.693	512	514	515	rBV	462	199	0.01%	0.002%
6	2.751	529	532	533	rBV3	337	181	0.01%	0.002%
7	2.963	596	598	600	rBV2	288	105	0.01%	0.001%
8	3.163	657	660	661	rBV2	303	139	0.01%	0.001%
9	3.237	682	683	685	rBV	293	120	0.01%	0.001%
10	3.275	693	695	697	rBV2	217	97	0.01%	0.001%
11	3.288	697	699	701	rBV	288	147	0.01%	0.001%
12	3.346	714	717	721	rBV4	561	541	0.03%	0.005%
13	3.452	748	750	751	rBV4	228	88	0.01%	0.001%
14	3.497	762	764	766	rBV	219	76	0.00%	0.001%
15	3.680	818	821	823	rBV	415	262	0.02%	0.002%
16	3.761	842	846	848	rBV3	204	172	0.01%	0.002%
17	3.796	848	857	895	rBV	100192	319106	20.64%	2.802%
18	4.249	982	998	1028	rBV	241672	626780	40.54%	5.504%
19	4.580	1097	1101	1104	rVB4	488	354	0.02%	0.003%
20	4.632	1114	1117	1125	rBV4	660	553	0.04%	0.005%
21	4.831	1174	1179	1182	rBV	517	548	0.04%	0.005%
22	4.851	1183	1185	1188	rVB2	486	207	0.01%	0.002%
23	4.870	1188	1191	1193	rBV3	481	262	0.02%	0.002%
24	4.886	1193	1196	1199	rVB2	706	480	0.03%	0.004%
25	4.953	1200	1217	1259	rBV2	576394	1546106	100.00%	13.577%
26	5.532	1386	1397	1437	rBV	431381	903148	58.41%	7.931%
27	5.831	1484	1490	1510	rVB5	12597	27043	1.75%	0.237%
28	5.986	1526	1538	1566	rBV	343303	714142	46.19%	6.271%
29	6.272	1625	1627	1628	rBV2	604	252	0.02%	0.002%
30	6.359	1649	1654	1657	rBV3	745	822	0.05%	0.007%
31	6.433	1675	1677	1679	rBV	233	90	0.01%	0.001%
32	6.449	1679	1682	1684	rBV2	386	248	0.02%	0.002%
33	6.484	1690	1693	1696	rBV2	372	223	0.01%	0.002%
34	6.561	1716	1717	1718	rBV2	361	114	0.01%	0.001%
35	6.703	1757	1761	1766	rBV5	799	824	0.05%	0.007%
36	6.825	1792	1799	1800	rBV2	331	309	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034981.D
 Acq On : 04 Apr 2024 16:21
 Operator : SY/MD
 Sample : P1987-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.834	1800	1802	1803	rBV	235	94	0.01%	0.001%
38	6.873	1813	1814	1815	rBV	173	63	0.00%	0.001%
39	6.912	1816	1826	1853	rBV	164696	322247	20.84%	2.830%
40	7.243	1918	1929	1953	rBV	651210	1159590	75.00%	10.183%
41	7.555	2017	2026	2051	rBV	111081	211304	13.67%	1.855%
42	7.995	2159	2163	2164	rBV2	565	364	0.02%	0.003%
43	8.027	2164	2173	2220	rVV2	306463	715456	46.27%	6.283%
44	8.481	2310	2314	2315	rBV2	777	568	0.04%	0.005%
45	8.661	2368	2370	2372	rBV2	353	186	0.01%	0.002%
46	8.783	2395	2408	2439	rBV	669709	1116188	72.19%	9.801%
47	9.246	2550	2552	2554	rBV	741	327	0.02%	0.003%
48	9.313	2569	2573	2574	rBV	520	353	0.02%	0.003%
49	9.384	2593	2595	2598	rBV2	440	246	0.02%	0.002%
50	9.458	2616	2618	2622	rVB	257	135	0.01%	0.001%
51	9.574	2652	2654	2655	rBV	288	121	0.01%	0.001%
52	9.657	2678	2680	2682	rBV	365	153	0.01%	0.001%
53	9.693	2688	2691	2694	rBV2	267	223	0.01%	0.002%
54	9.719	2694	2699	2701	rVV2	456	353	0.02%	0.003%
55	9.757	2709	2711	2712	rBV	261	79	0.01%	0.001%
56	9.776	2715	2717	2718	rBV	339	111	0.01%	0.001%
57	9.802	2723	2725	2731	rVB3	432	287	0.02%	0.003%
58	9.828	2731	2733	2734	rBV3	239	86	0.01%	0.001%
59	9.992	2779	2784	2786	rBV2	378	329	0.02%	0.003%
60	10.149	2819	2833	2858	rBV	476963	757249	48.98%	6.650%
61	10.378	2902	2904	2906	rBV2	390	161	0.01%	0.001%
62	10.458	2925	2929	2932	rBV	564	337	0.02%	0.003%
63	10.535	2949	2953	2956	rBV3	590	481	0.03%	0.004%
64	10.802	3033	3036	3039	rVB2	331	161	0.01%	0.001%
65	10.857	3051	3053	3054	rBV2	207	65	0.00%	0.001%
66	10.879	3059	3060	3063	rBV	280	167	0.01%	0.001%
67	10.937	3075	3078	3080	rBV2	463	345	0.02%	0.003%
68	10.992	3088	3095	3100	rBV2	622	769	0.05%	0.007%
69	11.037	3106	3109	3112	rBV2	354	194	0.01%	0.002%
70	11.185	3144	3155	3179	rBV	593575	943458	61.02%	8.285%
71	11.503	3251	3254	3257	rBV2	700	577	0.04%	0.005%
72	11.558	3260	3271	3296	rVV	641212	1016922	65.77%	8.930%
73	12.390	3526	3530	3531	rBV2	563	413	0.03%	0.004%
74	12.452	3547	3549	3553	rVB3	500	296	0.02%	0.003%
75	12.609	3591	3598	3601	rBV3	798	662	0.04%	0.006%
76	12.651	3609	3611	3613	rBV	298	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034981.D
Acq On : 04 Apr 2024 16:21
Operator : SY/MD
Sample : P1987-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R66

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.683	3620	3621	3623	rBV	323	162	0.01%	0.001%
78	12.956	3700	3706	3709	rBV2	716	748	0.05%	0.007%
79	12.995	3716	3718	3721	rBV2	476	305	0.02%	0.003%
80	13.162	3768	3770	3771	rBV	408	160	0.01%	0.001%
81	13.326	3818	3821	3822	rBV2	437	225	0.01%	0.002%




Sum of corrected areas: 11388038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034981.D
Acq On : 04 Apr 2024 16:21
Operator : SY/MD
Sample : P1987-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

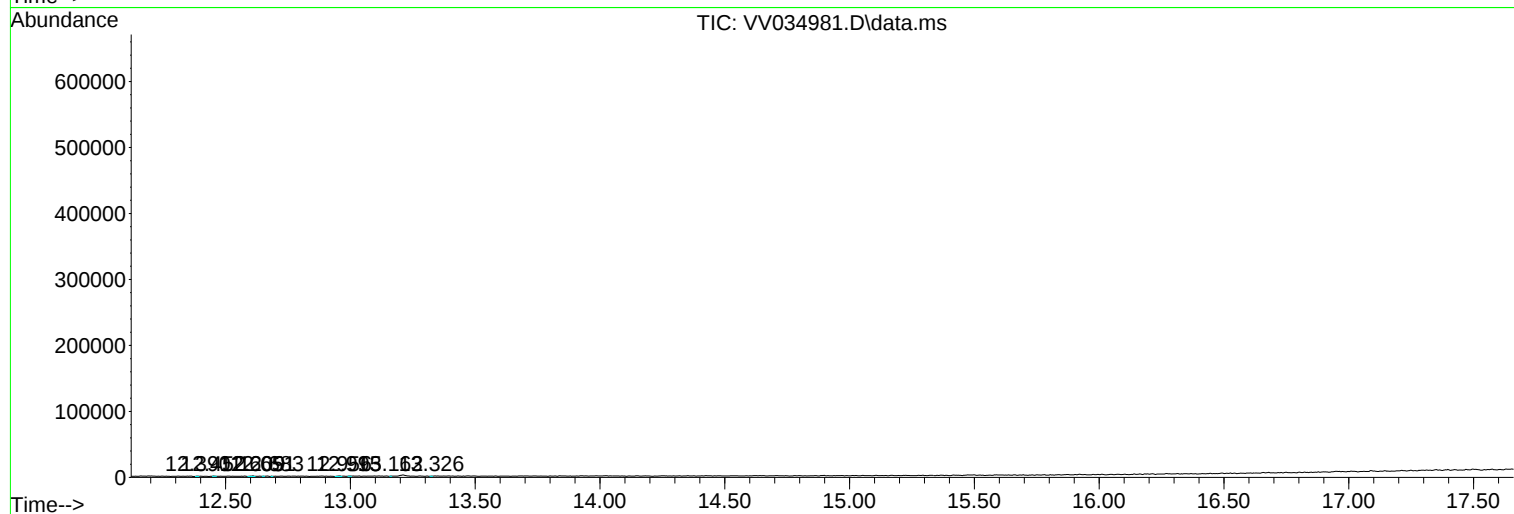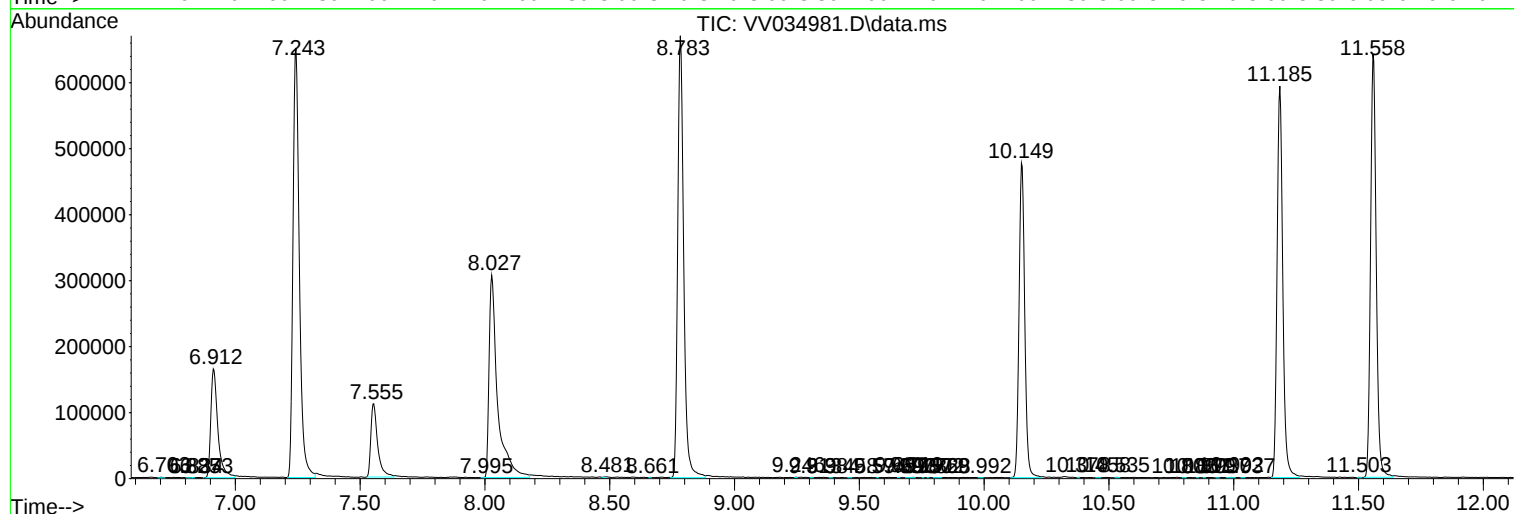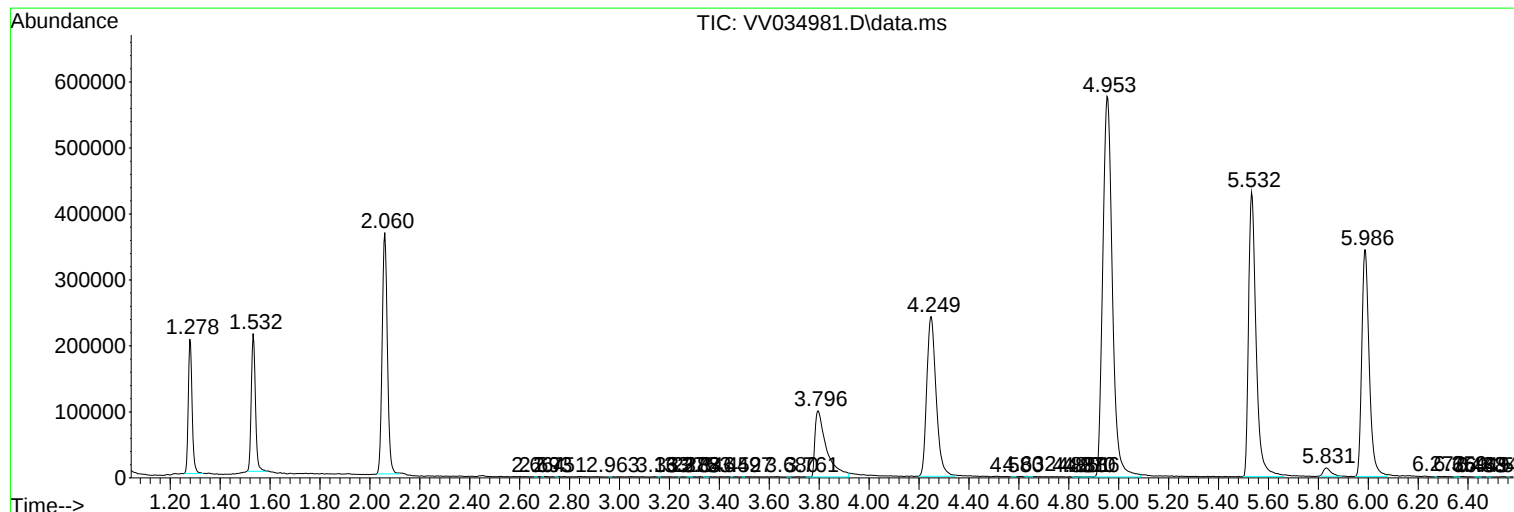

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034981.D
Acq On : 04 Apr 2024 16:21
Operator : SY/MD
Sample : P1987-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034981.D
Acq On : 04 Apr 2024 16:21
Operator : SY/MD
Sample : P1987-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------