

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034983.D
 Acq On : 04 Apr 2024 17:09
 Operator : SY/MD
 Sample : P1987-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	200444	216449	14.37%	1.898%
2	1.532	146	153	166	rVB	211623	240361	15.96%	2.108%
3	2.060	307	317	332	rBV	355580	517361	34.36%	4.537%
4	2.925	585	586	590	rVB	515	286	0.02%	0.003%
5	2.953	590	595	596	rBV2	511	373	0.02%	0.003%
6	3.050	621	625	627	rBV3	400	278	0.02%	0.002%
7	3.105	627	642	659	rBV3	13168	29275	1.94%	0.257%
8	3.233	680	682	688	rVB4	424	397	0.03%	0.003%
9	3.343	712	716	717	rBV	288	201	0.01%	0.002%
10	3.420	737	740	742	rBV2	486	297	0.02%	0.003%
11	3.461	748	753	754	rBV	387	247	0.02%	0.002%
12	3.510	764	768	773	rVB2	534	585	0.04%	0.005%
13	3.577	786	789	792	rBV2	358	291	0.02%	0.003%
14	3.648	809	811	816	rVB	415	309	0.02%	0.003%
15	3.696	824	826	829	rVV	391	247	0.02%	0.002%
16	3.722	832	834	838	rVB2	480	255	0.02%	0.002%
17	3.793	847	856	904	rBV2	108204	376505	25.00%	3.302%
18	4.246	981	997	1028	rBV	234508	614214	40.79%	5.386%
19	4.635	1116	1118	1122	rBV3	463	262	0.02%	0.002%
20	4.760	1154	1157	1160	rBV	595	366	0.02%	0.003%
21	4.879	1191	1194	1197	rBV2	401	199	0.01%	0.002%
22	4.953	1202	1217	1251	rBV2	562898	1505819	100.00%	13.205%
23	5.532	1386	1397	1432	rBV	429885	899074	59.71%	7.884%
24	5.834	1481	1491	1507	rBV4	10424	23477	1.56%	0.206%
25	5.986	1526	1538	1574	rBV	334193	706208	46.90%	6.193%
26	6.278	1626	1629	1631	rBV3	491	369	0.02%	0.003%
27	6.304	1635	1637	1639	rBV3	625	436	0.03%	0.004%
28	6.394	1663	1665	1668	rVB2	506	228	0.02%	0.002%
29	6.413	1668	1671	1674	rBV5	589	373	0.02%	0.003%
30	6.458	1683	1685	1689	rVB4	586	265	0.02%	0.002%
31	6.484	1689	1693	1695	rBV2	721	482	0.03%	0.004%
32	6.542	1709	1711	1715	rVB4	836	437	0.03%	0.004%
33	6.561	1715	1717	1720	rBV2	558	330	0.02%	0.003%
34	6.651	1742	1745	1748	rVB3	615	389	0.03%	0.003%
35	6.667	1748	1750	1752	rBV	311	216	0.01%	0.002%
36	6.703	1756	1761	1762	rBV3	454	306	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034983.D
 Acq On : 04 Apr 2024 17:09
 Operator : SY/MD
 Sample : P1987-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.754	1773	1777	1780	rBV3	302	192	0.01%	0.002%
38	6.796	1787	1790	1795	rVB2	507	342	0.02%	0.003%
39	6.821	1795	1798	1802	rBV2	471	327	0.02%	0.003%
40	6.863	1805	1811	1814	rBV3	467	415	0.03%	0.004%
41	6.912	1814	1826	1851	rBV	164186	318658	21.16%	2.794%
42	7.243	1918	1929	1956	rBV	639318	1138513	75.61%	9.984%
43	7.555	2017	2026	2051	rBV	108274	206705	13.73%	1.813%
44	7.760	2088	2090	2093	rBV2	734	464	0.03%	0.004%
45	7.796	2098	2101	2105	rVB3	913	586	0.04%	0.005%
46	7.960	2149	2152	2155	rBV2	345	222	0.01%	0.002%
47	7.985	2155	2160	2163	rVB4	513	545	0.04%	0.005%
48	8.027	2163	2173	2219	rBV2	308396	720952	47.88%	6.322%
49	8.667	2369	2372	2374	rBV3	377	266	0.02%	0.002%
50	8.722	2387	2389	2393	rBV3	483	326	0.02%	0.003%
51	8.783	2397	2408	2435	rBV	664449	1113136	73.92%	9.762%
52	9.050	2489	2491	2499	rBV5	731	859	0.06%	0.008%
53	9.169	2525	2528	2531	rBV2	451	344	0.02%	0.003%
54	9.220	2542	2544	2546	rBV	362	202	0.01%	0.002%
55	9.307	2568	2571	2573	rBV2	320	195	0.01%	0.002%
56	9.320	2573	2575	2579	rVB2	447	290	0.02%	0.003%
57	9.419	2603	2606	2613	rBV5	633	785	0.05%	0.007%
58	9.529	2637	2640	2642	rBV2	315	221	0.01%	0.002%
59	9.571	2648	2653	2657	rBV	375	410	0.03%	0.004%
60	9.619	2664	2668	2674	rVB	364	304	0.02%	0.003%
61	9.677	2683	2686	2687	rBV	335	204	0.01%	0.002%
62	9.709	2693	2696	2698	rBV2	280	183	0.01%	0.002%
63	9.796	2721	2723	2727	rVB2	519	235	0.02%	0.002%
64	9.815	2727	2729	2736	rVB3	535	323	0.02%	0.003%
65	9.863	2742	2744	2745	rBV2	331	189	0.01%	0.002%
66	9.998	2784	2786	2792	rVB3	521	382	0.03%	0.003%
67	10.037	2792	2798	2803	rBV3	403	580	0.04%	0.005%
68	10.082	2808	2812	2813	rBV	304	192	0.01%	0.002%
69	10.098	2813	2817	2820	rBV2	584	448	0.03%	0.004%
70	10.153	2822	2834	2860	rBV	473161	756734	50.25%	6.636%
71	10.310	2881	2883	2887	rBV2	709	586	0.04%	0.005%
72	10.371	2900	2902	2905	rBV2	490	206	0.01%	0.002%
73	10.432	2917	2921	2924	rBV2	535	415	0.03%	0.004%
74	10.490	2936	2939	2943	rBV3	353	292	0.02%	0.003%
75	10.667	2990	2994	2997	rBV2	456	328	0.02%	0.003%
76	10.699	3002	3004	3007	rVB3	529	226	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034983.D
 Acq On : 04 Apr 2024 17:09
 Operator : SY/MD
 Sample : P1987-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.876	3056	3059	3061	rBV	332	215	0.01%	0.002%
78	11.107	3127	3131	3133	rVB3	377	247	0.02%	0.002%
79	11.133	3136	3139	3143	rBV4	781	644	0.04%	0.006%
80	11.185	3144	3155	3176	rBV	605342	958236	63.64%	8.403%
81	11.490	3248	3250	3251	rBV2	454	191	0.01%	0.002%
82	11.558	3259	3271	3300	rBV	638862	1029264	68.35%	9.026%
83	11.853	3361	3363	3366	rVB	500	200	0.01%	0.002%
84	11.873	3366	3369	3370	rBV	405	196	0.01%	0.002%
85	11.960	3394	3396	3398	rBV2	443	206	0.01%	0.002%
86	12.008	3404	3411	3416	rBV3	732	917	0.06%	0.008%
87	12.059	3424	3427	3430	rBV2	523	426	0.03%	0.004%
88	12.162	3456	3459	3460	rBV	455	224	0.01%	0.002%
89	12.316	3503	3507	3509	rBV2	526	347	0.02%	0.003%
90	12.423	3538	3540	3542	rBV3	458	226	0.02%	0.002%
91	12.493	3559	3562	3565	rBV	470	332	0.02%	0.003%
92	12.542	3570	3577	3579	rBV	608	634	0.04%	0.006%
93	12.635	3603	3606	3609	rBV2	700	527	0.03%	0.005%
94	13.107	3750	3753	3757	rBV3	561	420	0.03%	0.004%
95	13.143	3761	3764	3767	rBV2	560	431	0.03%	0.004%
96	13.207	3779	3784	3791	rBV6	2414	3294	0.22%	0.029%
97	13.451	3857	3860	3865	rBV4	558	487	0.03%	0.004%
98	13.577	3897	3899	3905	rBV3	464	438	0.03%	0.004%
99	13.886	3992	3995	3996	rBV	486	224	0.01%	0.002%
100	13.934	4006	4010	4015	rBV2	843	868	0.06%	0.008%

Sum of corrected areas: 11403143




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034983.D
Acq On : 04 Apr 2024 17:09
Operator : SY/MD
Sample : P1987-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

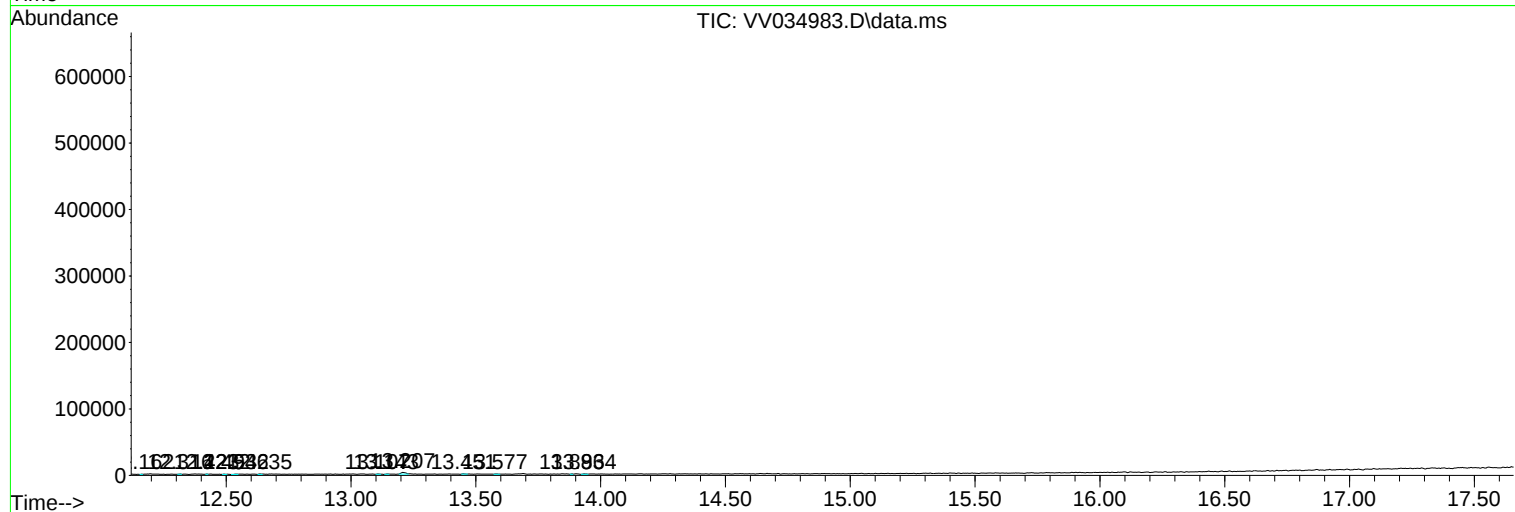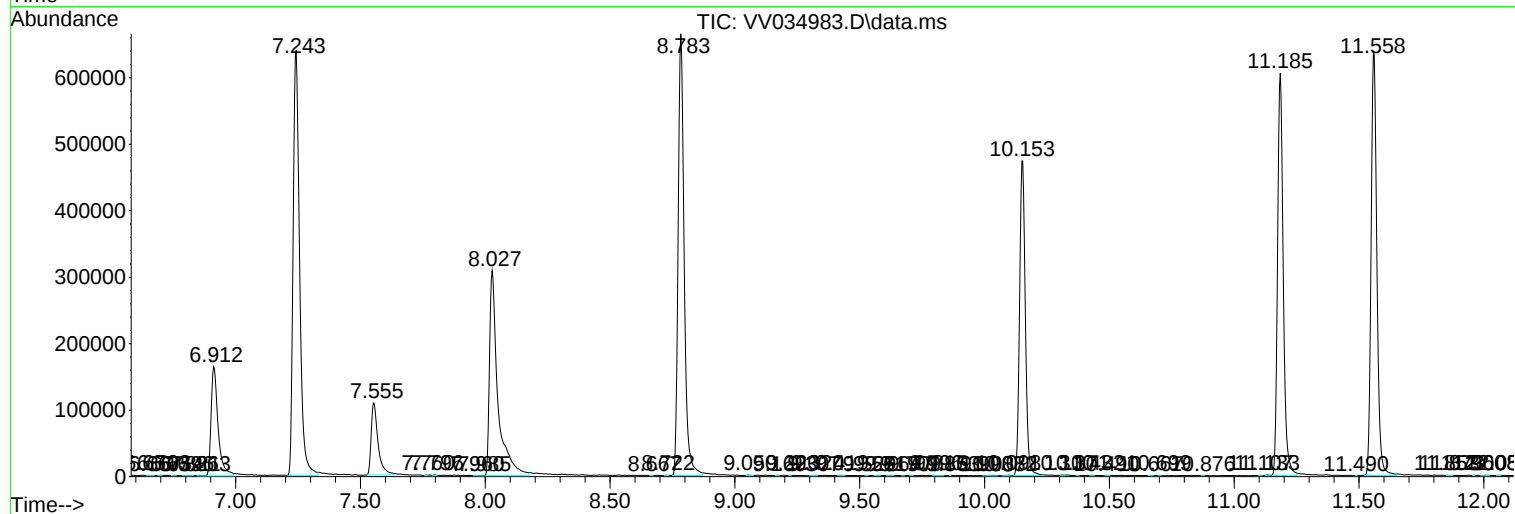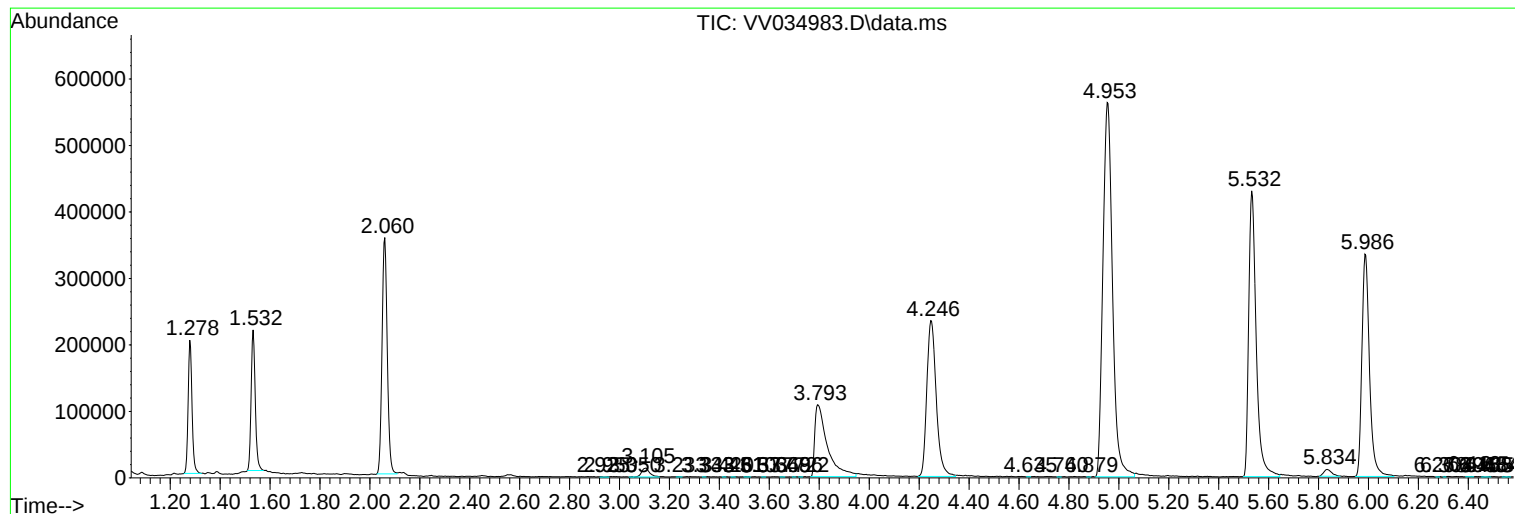

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034983.D
Acq On : 04 Apr 2024 17:09
Operator : SY/MD
Sample : P1987-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034983.D
Acq On : 04 Apr 2024 17:09
Operator : SY/MD
Sample : P1987-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------