

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034984.D
 Acq On : 04 Apr 2024 17:32
 Operator : SY/MD
 Sample : P1987-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV034984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	199251	211533	13.91%	1.863%
2	1.532	146	153	174	rVB	219404	258346	16.99%	2.276%
3	2.060	307	317	331	rBV	361156	524924	34.51%	4.624%
4	2.520	458	460	462	rBV3	533	221	0.01%	0.002%
5	2.835	554	558	560	rBV	491	446	0.03%	0.004%
6	2.947	591	593	595	rBV2	339	165	0.01%	0.001%
7	3.044	620	623	627	rBV	484	414	0.03%	0.004%
8	3.217	675	677	679	rBV2	399	190	0.01%	0.002%
9	3.317	705	708	710	rBV	357	268	0.02%	0.002%
10	3.346	715	717	718	rBV	181	81	0.01%	0.001%
11	3.384	728	729	730	rBV	160	36	0.00%	0.000%
12	3.410	735	737	739	rBV	444	268	0.02%	0.002%
13	3.468	751	755	757	rVB	378	252	0.02%	0.002%
14	3.487	759	761	762	rBV	296	98	0.01%	0.001%
15	3.536	774	776	780	rVB2	515	287	0.02%	0.003%
16	3.561	780	784	787	rBV3	492	312	0.02%	0.003%
17	3.581	787	790	793	rVV3	237	142	0.01%	0.001%
18	3.610	796	799	802	rVB2	460	305	0.02%	0.003%
19	3.658	810	814	817	rBV	383	272	0.02%	0.002%
20	3.700	817	827	831	rVV2	588	820	0.05%	0.007%
21	3.725	831	835	836	rBV	311	192	0.01%	0.002%
22	3.757	842	845	847	rVB	208	94	0.01%	0.001%
23	3.793	847	856	891	rBV	106142	324090	21.31%	2.855%
24	4.246	983	997	1032	rBV	241707	615147	40.44%	5.419%
25	4.680	1130	1132	1134	rVB	460	141	0.01%	0.001%
26	4.831	1177	1179	1180	rBV	305	113	0.01%	0.001%
27	4.876	1188	1193	1194	rBV	449	334	0.02%	0.003%
28	4.954	1202	1217	1248	rBV2	575369	1520998	100.00%	13.398%
29	5.481	1379	1381	1384	rBV4	571	280	0.02%	0.002%
30	5.532	1386	1397	1436	rVV	428546	899932	59.17%	7.927%
31	5.835	1479	1491	1510	rBV3	13046	30807	2.03%	0.271%
32	5.986	1525	1538	1576	rBV	338547	718874	47.26%	6.332%
33	6.362	1653	1655	1660	rVB	506	245	0.02%	0.002%
34	6.400	1664	1667	1670	rBV4	452	272	0.02%	0.002%
35	6.500	1692	1698	1699	rBV2	627	460	0.03%	0.004%
36	6.555	1707	1715	1716	rBV3	509	517	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034984.D
 Acq On : 04 Apr 2024 17:32
 Operator : SY/MD
 Sample : P1987-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.613	1730	1733	1740	rVB4	666	666	0.04%	0.006%
38	6.642	1740	1742	1743	rBV2	568	257	0.02%	0.002%
39	6.690	1753	1757	1758	rBV	348	217	0.01%	0.002%
40	6.735	1768	1771	1773	rBV3	379	185	0.01%	0.002%
41	6.757	1776	1778	1782	rBV3	517	410	0.03%	0.004%
42	6.799	1789	1791	1795	rVB2	589	330	0.02%	0.003%
43	6.822	1796	1798	1802	rBV2	270	162	0.01%	0.001%
44	6.912	1816	1826	1856	rBV	161353	318138	20.92%	2.802%
45	7.243	1918	1929	1961	rBV	641872	1145145	75.29%	10.087%
46	7.555	2016	2026	2061	rBV	110138	216471	14.23%	1.907%
47	7.947	2147	2148	2150	rBV	216	78	0.01%	0.001%
48	8.027	2163	2173	2215	rBV2	314692	726270	47.75%	6.397%
49	8.783	2396	2408	2436	rBV	672165	1110439	73.01%	9.781%
50	9.104	2506	2508	2511	rVB2	840	429	0.03%	0.004%
51	9.121	2511	2513	2517	rBV3	547	317	0.02%	0.003%
52	9.278	2555	2562	2564	rBV	573	625	0.04%	0.006%
53	9.445	2611	2614	2615	rBV	422	221	0.01%	0.002%
54	9.603	2660	2663	2665	rVB2	608	285	0.02%	0.003%
55	9.635	2669	2673	2675	rBV2	459	402	0.03%	0.004%
56	9.686	2687	2689	2691	rBV2	221	115	0.01%	0.001%
57	9.699	2691	2693	2697	rVV2	368	282	0.02%	0.002%
58	9.770	2713	2715	2718	rVB	583	271	0.02%	0.002%
59	9.802	2723	2725	2727	rBV	254	131	0.01%	0.001%
60	9.857	2739	2742	2746	rVB	603	353	0.02%	0.003%
61	9.931	2761	2765	2769	rBV3	428	408	0.03%	0.004%
62	9.979	2778	2780	2786	rVB3	728	653	0.04%	0.006%
63	10.027	2786	2795	2797	rBV	517	665	0.04%	0.006%
64	10.079	2810	2811	2812	rBB	114	56	0.00%	0.000%
65	10.149	2821	2833	2860	rBV	470736	755228	49.65%	6.652%
66	10.407	2910	2913	2918	rBV2	518	489	0.03%	0.004%
67	10.487	2936	2938	2940	rBV	435	150	0.01%	0.001%
68	10.500	2940	2942	2945	rVB	427	179	0.01%	0.002%
69	10.542	2950	2955	2960	rBV3	360	467	0.03%	0.004%
70	10.612	2975	2977	2982	rBV	239	156	0.01%	0.001%
71	10.670	2991	2995	2999	rBV2	360	434	0.03%	0.004%
72	10.838	3045	3047	3055	rVB3	476	460	0.03%	0.004%
73	10.876	3055	3059	3060	rBV2	493	338	0.02%	0.003%
74	10.979	3085	3091	3092	rBV3	731	710	0.05%	0.006%
75	11.014	3100	3102	3105	rBV2	457	294	0.02%	0.003%
76	11.075	3117	3121	3122	rBV	451	243	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034984.D
Acq On : 04 Apr 2024 17:32
Operator : SY/MD
Sample : P1987-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.111	3129	3132	3133	rBV2	293	148	0.01%	0.001%
78	11.133	3136	3139	3140	rBV2	462	283	0.02%	0.002%
79	11.185	3144	3155	3180	rBV	601680	949905	62.45%	8.367%
80	11.558	3259	3271	3297	rBV	635164	1005848	66.13%	8.860%
81	12.262	3487	3490	3494	rVB3	848	659	0.04%	0.006%
82	12.419	3537	3539	3540	rBV2	397	154	0.01%	0.001%
83	13.760	3954	3956	3959	rBV2	591	362	0.02%	0.003%
84	14.198	4090	4092	4095	rBV3	596	318	0.02%	0.003%




Sum of corrected areas: 11352682

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034984.D
Acq On : 04 Apr 2024 17:32
Operator : SY/MD
Sample : P1987-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

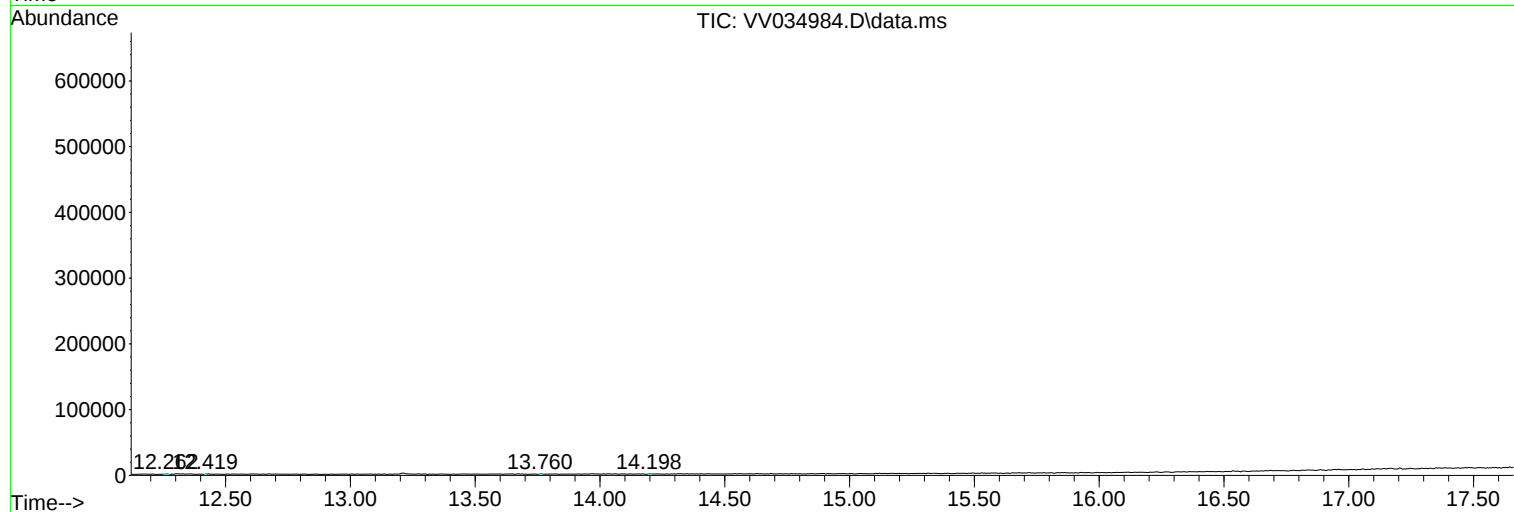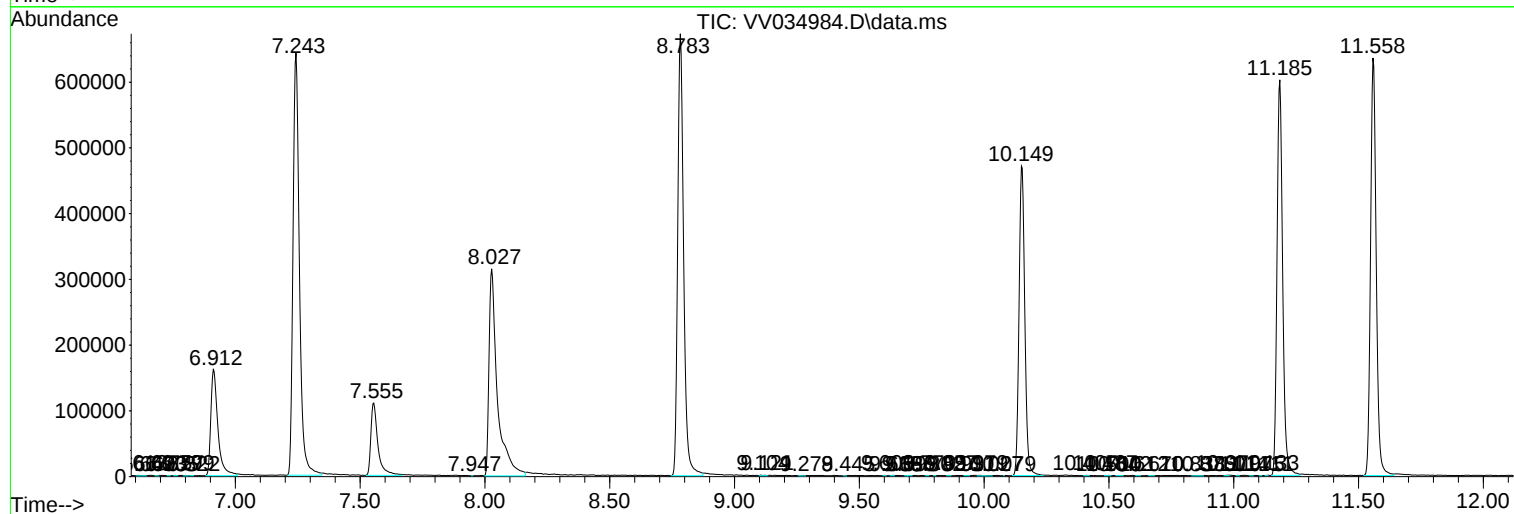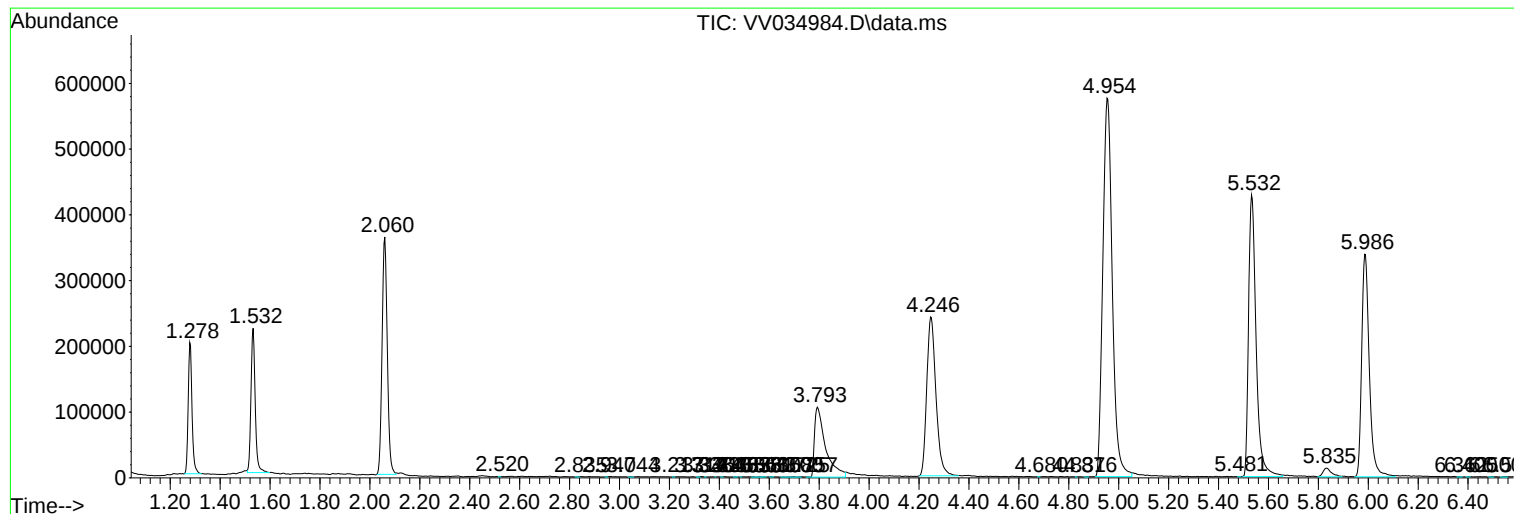

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034984.D
Acq On : 04 Apr 2024 17:32
Operator : SY/MD
Sample : P1987-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034984.D
Acq On : 04 Apr 2024 17:32
Operator : SY/MD
Sample : P1987-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc