

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040424\
 Data File : VV034985.D
 Acq On : 04 Apr 2024 17:56
 Operator : SY/MD
 Sample : P1987-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV034985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	193996	209536	14.11%	1.906%
2	1.532	146	153	178	rVB	210793	250211	16.85%	2.276%
3	2.060	307	317	331	rBV	348977	505260	34.03%	4.596%
4	2.719	518	522	526	rBV4	535	532	0.04%	0.005%
5	2.802	546	548	550	rBV2	507	200	0.01%	0.002%
6	2.886	571	574	577	rBV	509	283	0.02%	0.003%
7	2.957	594	596	602	rVB2	522	341	0.02%	0.003%
8	3.069	629	631	633	rBV	426	208	0.01%	0.002%
9	3.265	690	692	693	rBV	236	99	0.01%	0.001%
10	3.281	694	697	698	rVV	490	290	0.02%	0.003%
11	3.298	700	702	704	rVB2	395	187	0.01%	0.002%
12	3.365	721	723	725	rBV	345	143	0.01%	0.001%
13	3.462	751	753	755	rBV	279	107	0.01%	0.001%
14	3.478	755	758	760	rVV	342	166	0.01%	0.002%
15	3.490	760	762	767	rVB2	530	322	0.02%	0.003%
16	3.513	767	769	771	rBV	202	103	0.01%	0.001%
17	3.577	788	789	792	rBV	311	112	0.01%	0.001%
18	3.603	794	797	800	rVV2	469	318	0.02%	0.003%
19	3.796	848	857	888	rBV	98948	302466	20.37%	2.751%
20	4.249	983	998	1028	rBV	237752	620170	41.77%	5.641%
21	4.651	1121	1123	1124	rBV	337	103	0.01%	0.001%
22	4.767	1155	1159	1161	rBV2	429	360	0.02%	0.003%
23	4.863	1186	1189	1190	rBV	427	303	0.02%	0.003%
24	4.953	1202	1217	1247	rBV2	561539	1484594	100.00%	13.503%
25	5.471	1375	1378	1380	rVB	570	324	0.02%	0.003%
26	5.532	1383	1397	1424	rBV	412179	861902	58.06%	7.839%
27	5.831	1482	1490	1508	rBV2	15576	31887	2.15%	0.290%
28	5.989	1527	1539	1568	rBV	330265	690329	46.50%	6.279%
29	6.281	1628	1630	1634	rBV4	674	428	0.03%	0.004%
30	6.455	1682	1684	1687	rBV4	688	458	0.03%	0.004%
31	6.503	1697	1699	1703	rBV5	526	378	0.03%	0.003%
32	6.577	1720	1722	1724	rBV	377	188	0.01%	0.002%
33	6.593	1724	1727	1729	rVV2	521	308	0.02%	0.003%
34	6.613	1729	1733	1738	rVB5	870	651	0.04%	0.006%
35	6.635	1738	1740	1741	rBV	448	206	0.01%	0.002%
36	6.748	1773	1775	1780	rBV3	238	182	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
 Data File : VV034985.D
 Acq On : 04 Apr 2024 17:56
 Operator : SY/MD
 Sample : P1987-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.767	1780	1781	1783	rVB2	375	107	0.01%	0.001%
38	6.831	1798	1801	1803	rBV2	359	146	0.01%	0.001%
39	6.867	1810	1812	1814	rBV	435	240	0.02%	0.002%
40	6.912	1816	1826	1857	rVV	157357	310607	20.92%	2.825%
41	7.243	1918	1929	1955	rBV	624766	1112574	74.94%	10.119%
42	7.555	2016	2026	2046	rBV	106924	202256	13.62%	1.840%
43	7.982	2156	2159	2160	rBV	247	141	0.01%	0.001%
44	8.027	2164	2173	2215	rBV2	298259	698523	47.05%	6.353%
45	8.638	2361	2363	2364	rBV	359	173	0.01%	0.002%
46	8.738	2391	2394	2397	rVB2	586	326	0.02%	0.003%
47	8.783	2397	2408	2438	rBV	643873	1067933	71.93%	9.713%
48	9.037	2483	2487	2492	rVB4	951	935	0.06%	0.009%
49	9.149	2519	2522	2525	rBV2	487	448	0.03%	0.004%
50	9.233	2546	2548	2550	rVB2	560	194	0.01%	0.002%
51	9.256	2550	2555	2557	rBV2	326	281	0.02%	0.003%
52	9.329	2576	2578	2579	rBV	248	73	0.00%	0.001%
53	9.339	2579	2581	2582	rBV2	292	106	0.01%	0.001%
54	9.445	2610	2614	2616	rBV2	715	484	0.03%	0.004%
55	9.657	2676	2680	2681	rBV	316	265	0.02%	0.002%
56	9.741	2704	2706	2709	rBV2	544	310	0.02%	0.003%
57	9.789	2719	2721	2723	rVB	254	93	0.01%	0.001%
58	9.873	2745	2747	2750	rBV3	340	236	0.02%	0.002%
59	9.908	2755	2758	2762	rBV2	485	326	0.02%	0.003%
60	9.953	2768	2772	2775	rBV3	372	371	0.02%	0.003%
61	9.989	2780	2783	2786	rVB2	439	258	0.02%	0.002%
62	10.005	2786	2788	2790	rVB	467	176	0.01%	0.002%
63	10.027	2790	2795	2797	rBV	273	229	0.02%	0.002%
64	10.040	2797	2799	2801	rBV	217	130	0.01%	0.001%
65	10.075	2807	2810	2811	rBV	243	119	0.01%	0.001%
66	10.088	2811	2814	2815	rBV	473	254	0.02%	0.002%
67	10.153	2822	2834	2861	rBV	449328	726380	48.93%	6.607%
68	10.452	2921	2927	2933	rBV2	582	874	0.06%	0.008%
69	10.503	2941	2943	2944	rBV	399	174	0.01%	0.002%
70	10.593	2968	2971	2972	rBV2	413	191	0.01%	0.002%
71	10.622	2977	2980	2982	rBV2	311	164	0.01%	0.001%
72	10.934	3073	3077	3081	rBV3	573	499	0.03%	0.005%
73	10.982	3091	3092	3094	rBV	213	102	0.01%	0.001%
74	11.114	3130	3133	3134	rBV2	273	157	0.01%	0.001%
75	11.185	3144	3155	3177	rBV	578209	916701	61.75%	8.338%
76	11.445	3233	3236	3238	rBV	371	268	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034985.D
Acq On : 04 Apr 2024 17:56
Operator : SY/MD
Sample : P1987-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.513	3248	3257	3260	rBV6	4164	6400	0.43%	0.058%
78	11.561	3261	3272	3293	rVB	610485	978334	65.90%	8.898%
79	12.249	3484	3486	3488	rBV	289	112	0.01%	0.001%
80	12.284	3493	3497	3498	rBV3	708	470	0.03%	0.004%
81	12.468	3549	3554	3557	rBV4	587	648	0.04%	0.006%
82	12.535	3573	3575	3576	rBV	223	57	0.00%	0.001%
83	13.323	3818	3820	3823	rBV	575	401	0.03%	0.004%
84	14.236	4102	4104	4110	rBV3	585	578	0.04%	0.005%

Sum of corrected areas: 10994479




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034985.D
Acq On : 04 Apr 2024 17:56
Operator : SY/MD
Sample : P1987-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

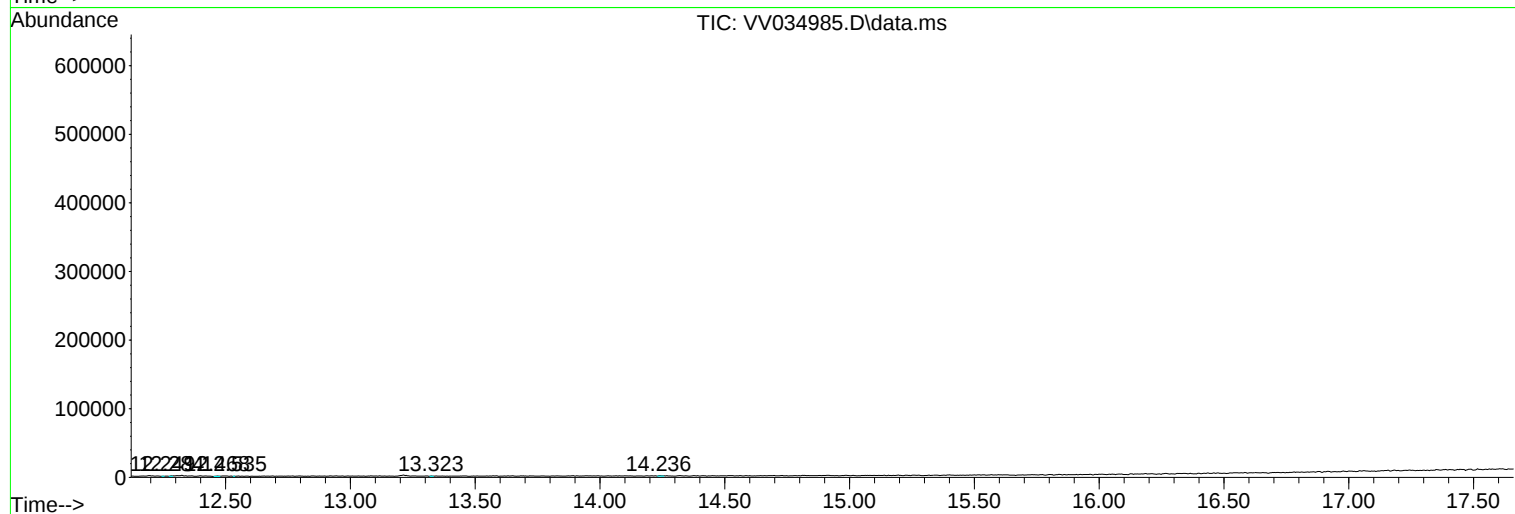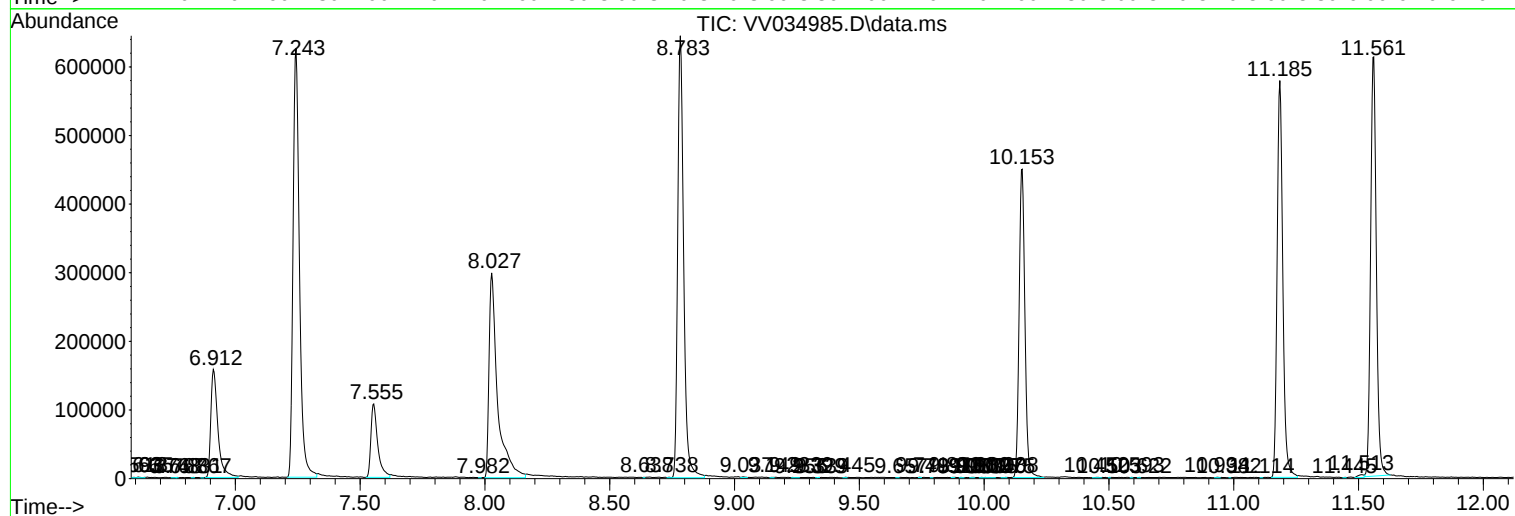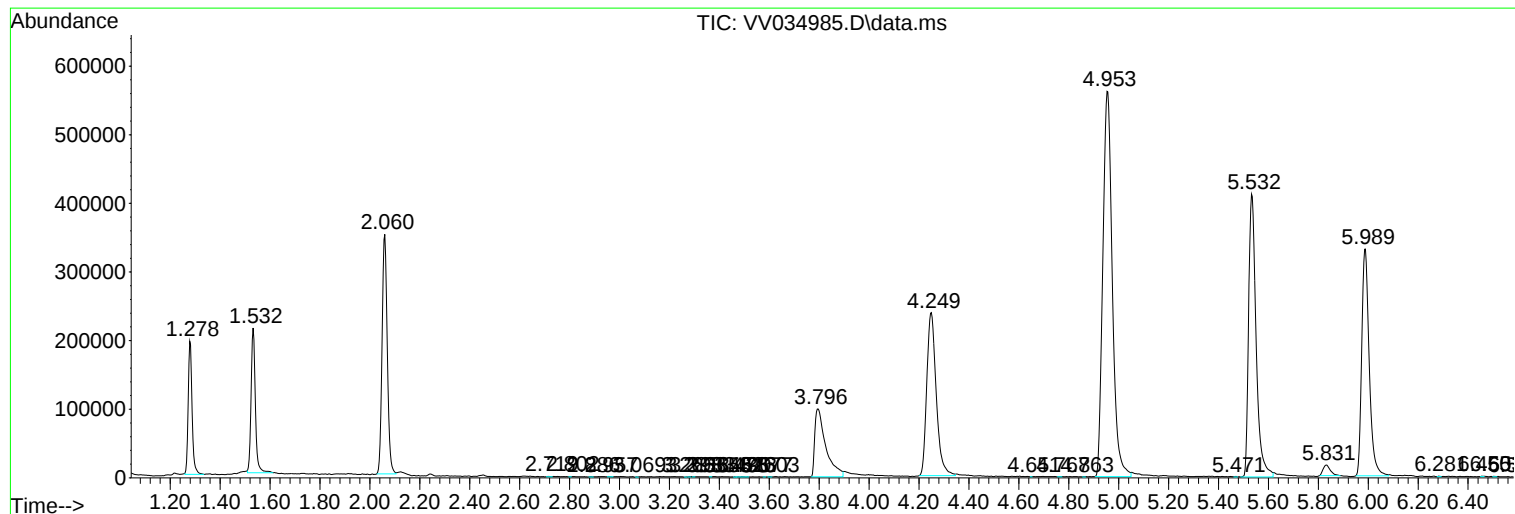

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034985.D
Acq On : 04 Apr 2024 17:56
Operator : SY/MD
Sample : P1987-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040424\
Data File : VV034985.D
Acq On : 04 Apr 2024 17:56
Operator : SY/MD
Sample : P1987-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------